

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022187.D
 Acq On : 04 Mar 2022 18:03
 Operator : SY/VA
 Sample : N1775-03
 Misc : 7.11g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 05 03:24:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	146941	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	143356	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	73137	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	29682	15.487	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.960%
7) Chloroethane-d5	2.879	69	26137	17.333	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.320%
11) 1,1-Dichloroethene-d2	4.013	63	38023	12.955	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.840%
21) 2-Butanone-d5	7.074	46	20940	64.982	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	129.960%
24) Chloroform-d	7.647	84	76374	23.296	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.200%
26) 1,2-Dichloroethane-d4	8.305	65	40627	23.840	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.360%
32) Benzene-d6	8.275	84	137445	20.601	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.400%
36) 1,2-Dichloropropane-d6	9.274	67	42684	23.037	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.160%
41) Toluene-d8	10.323	98	125282	18.888	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.560%
43) trans-1,3-Dichloroprop...	10.579	79	16046	19.532	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.120%
47) 2-Hexanone-d5	10.921	63	17910	58.772	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.540%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	43597	26.811	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	54039	23.004	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.000%
Target Compounds					Qvalue	
13) Acetone	4.141	43	1091	4.145	ug/L	61
37) 1,2-Dichloropropane	9.268	63	5332	3.298	ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
Data File : VW022187.D
Acq On : 04 Mar 2022 18:03
Operator : SY/VA
Sample : N1775-03
Misc : 7.11g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 05 03:24:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 05 03:21:21 2022
Response via : Initial Calibration




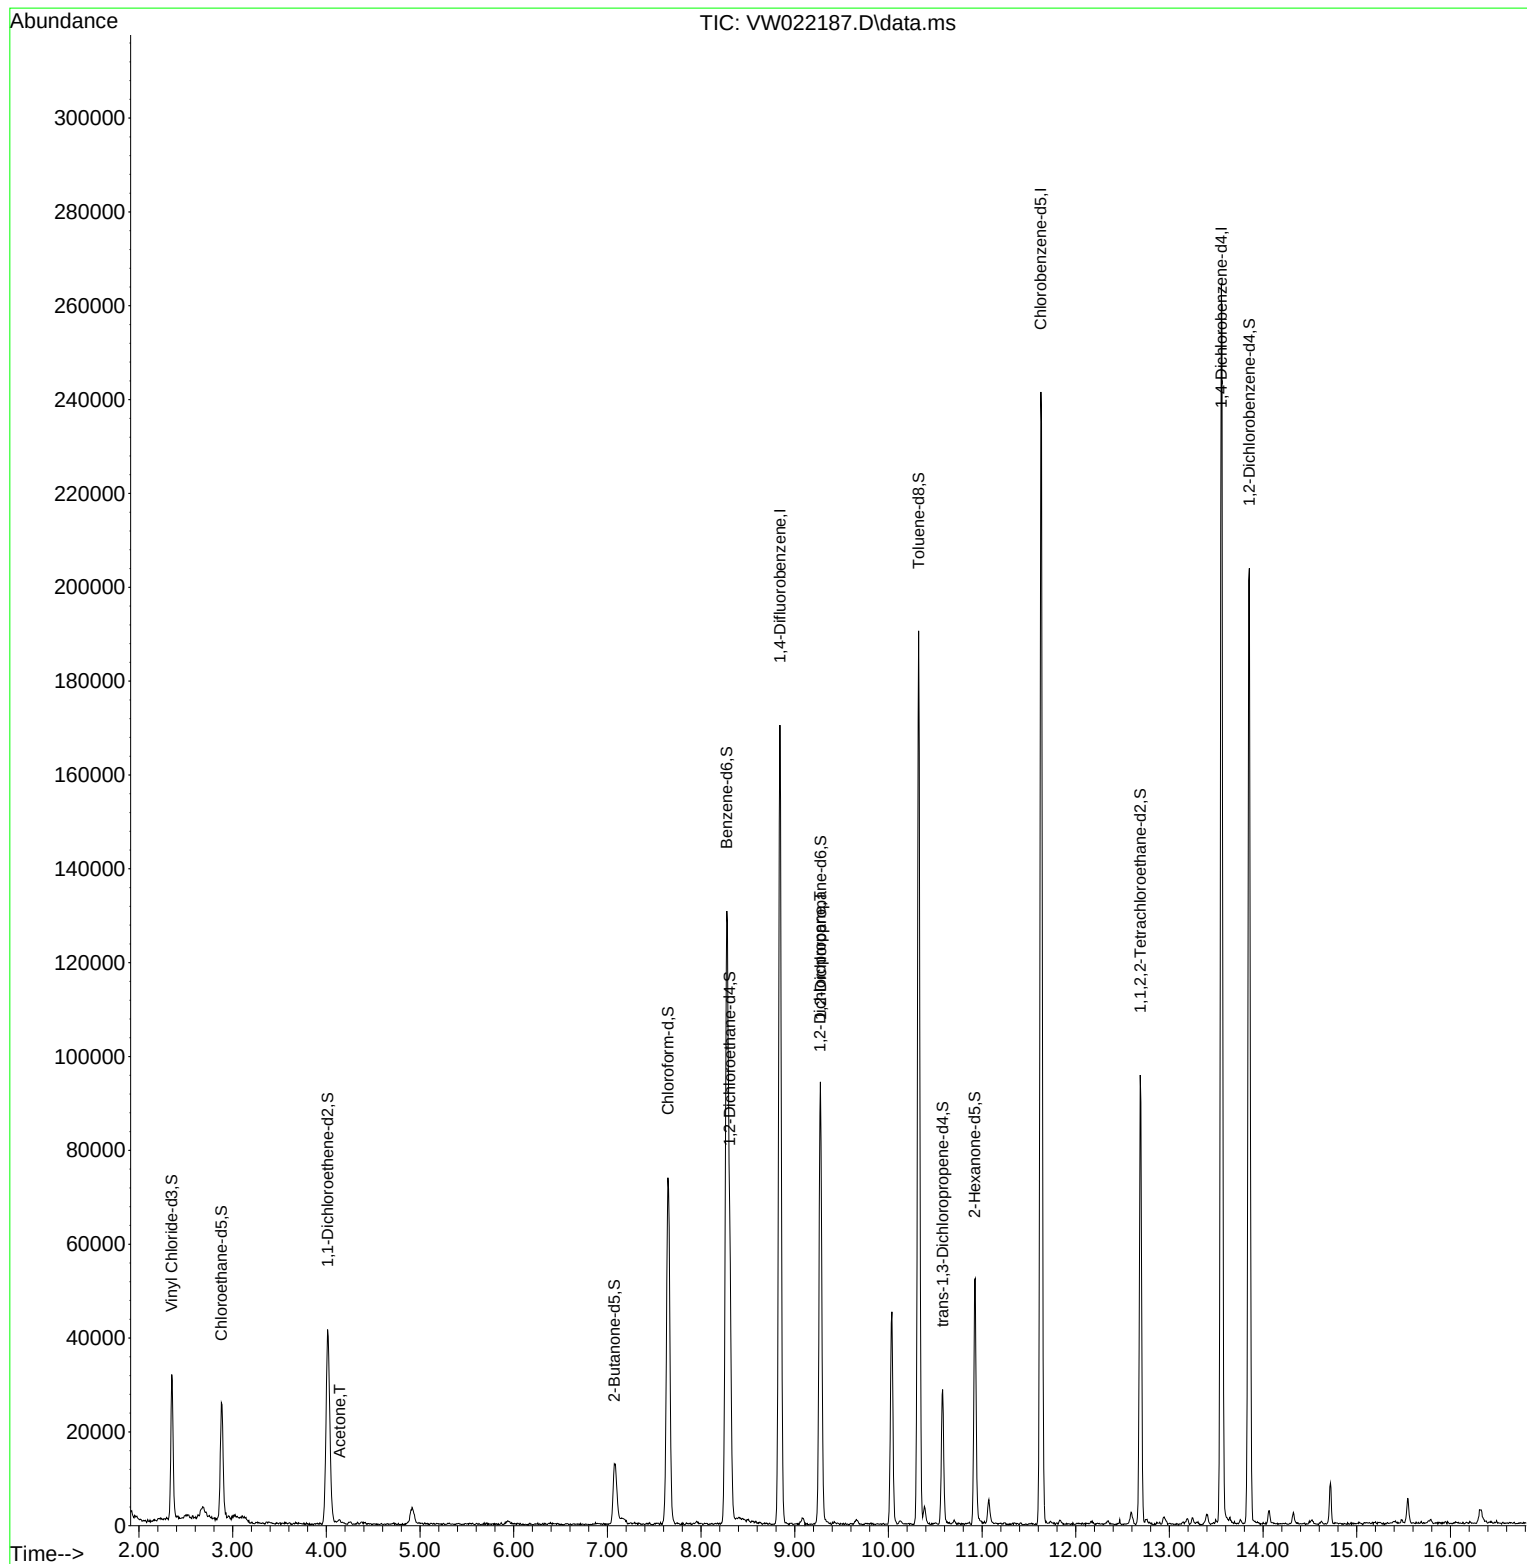


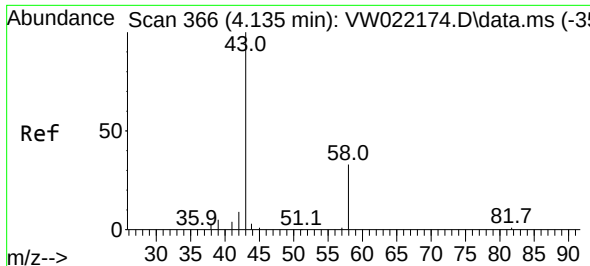

#13
Acetone
Concen: 4.145 ug/L
RT: 4.141 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW022187.D
Acq: 04 Mar 2022 18:03

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 43 Resp: 1091
Ion Ratio Lower Upper
43 100
58 12.1 0.0 69.2

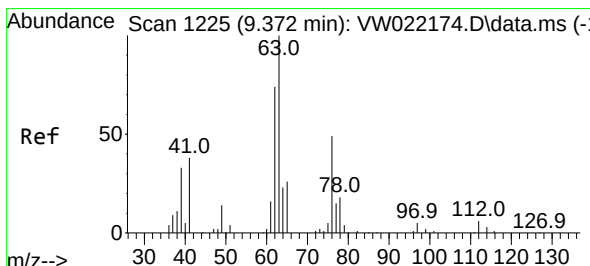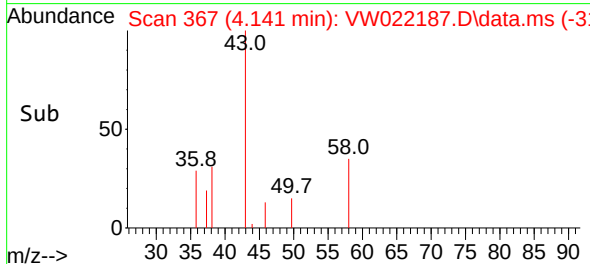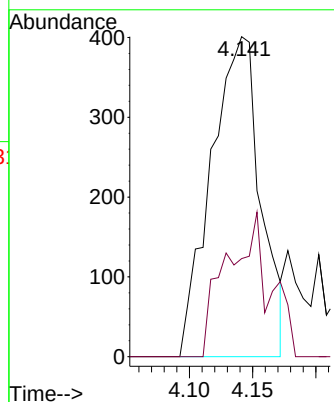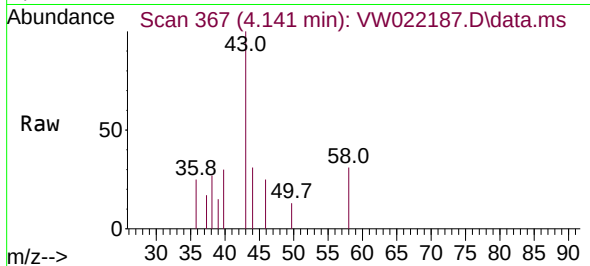

#37
1,2-Dichloropropane
Concen: 3.298 ug/L
RT: 9.268 min Scan# 1208
Delta R.T. -0.104 min
Lab File: VW022187.D
Acq: 04 Mar 2022 18:03

Tgt Ion: 63 Resp: 5332
Ion Ratio Lower Upper
63 100
112 0.0 4.1 6.1#

