




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022181.D
 Acq On : 04 Mar 2022 15:39
 Operator : SY/VA
 Sample : N1775-02
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRU8

Manual IntegrationsAPPROVED

Quant Time: Mar 05 03:23:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

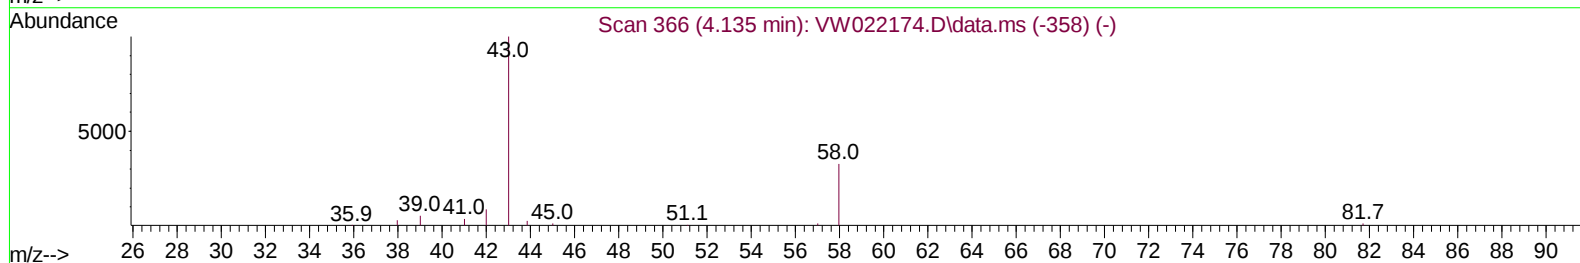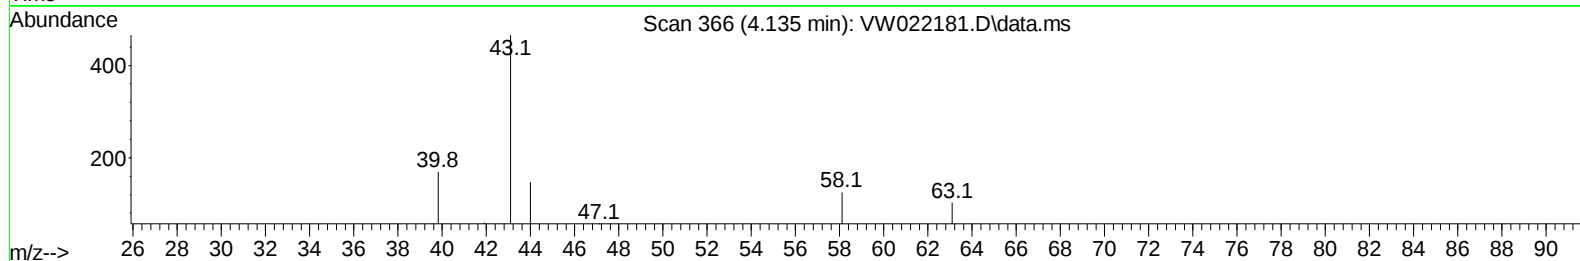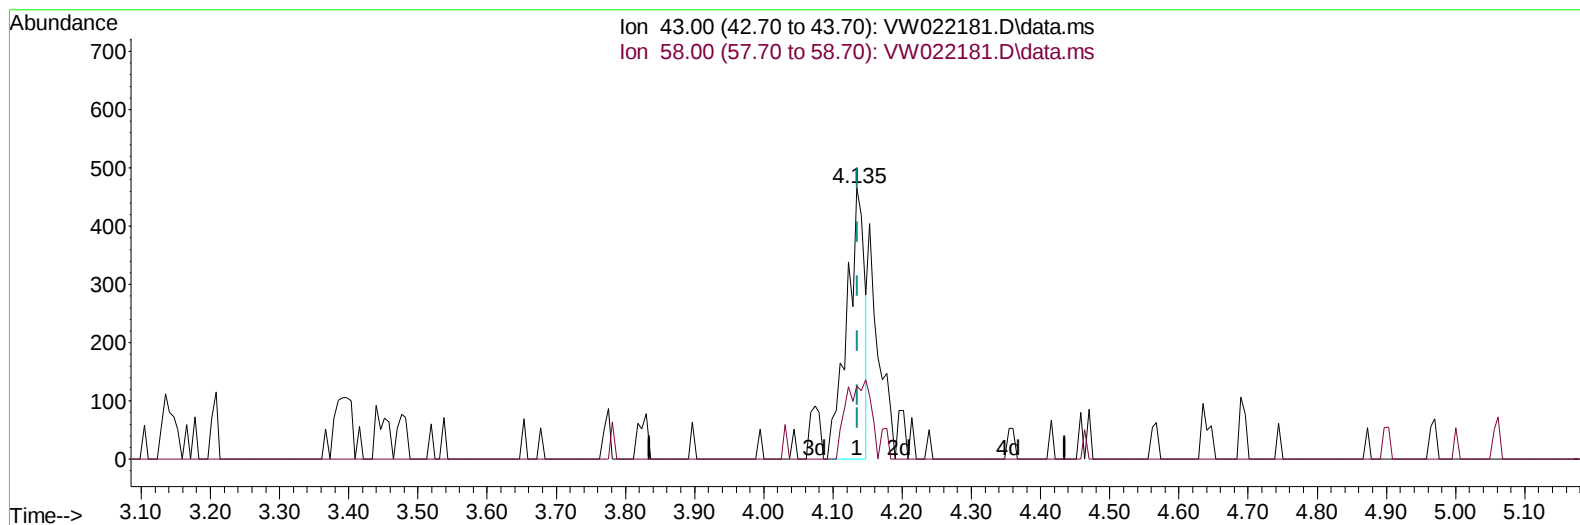

TIC: VW022181.D\data.ms

(13) Acetone (T)

4.135min (-0.000) 3.38 ug/L

response 819

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	16.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022181.D
 Acq On : 04 Mar 2022 15:39
 Operator : SY/VA
 Sample : N1775-02
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRU8

Manual IntegrationsAPPROVED

Quant Time: Mar 05 03:23:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

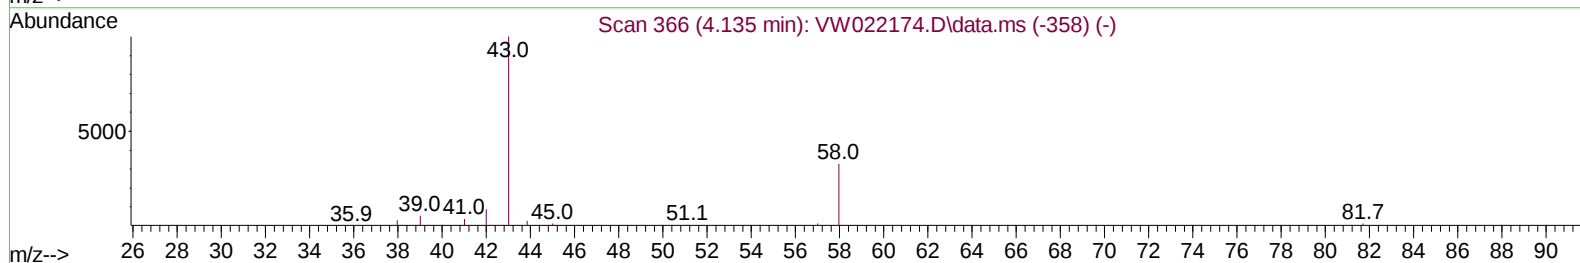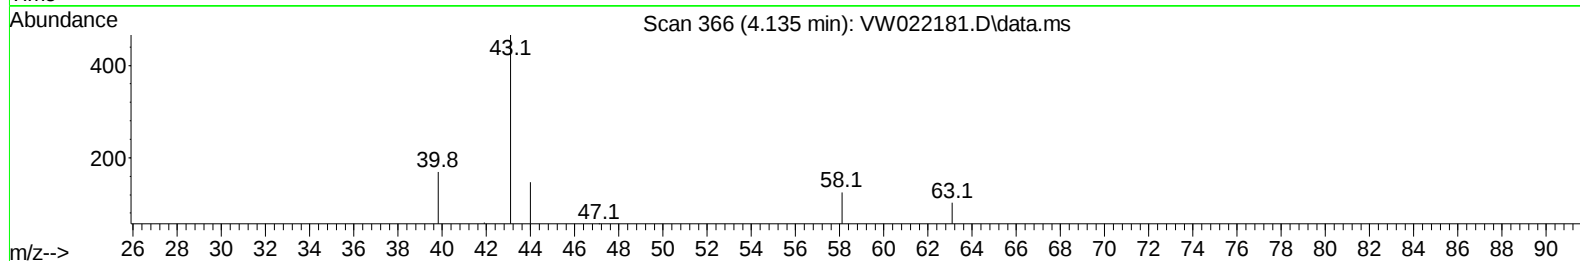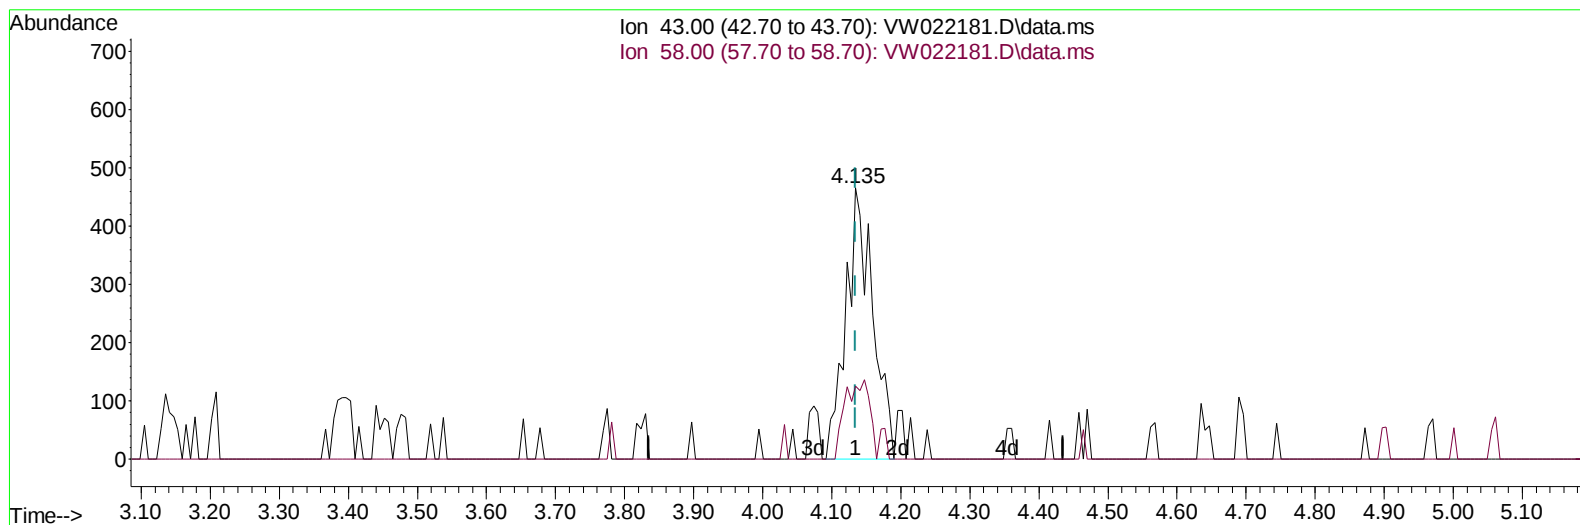

TIC: VW022181.D\data.ms

(13) Acetone (T)

4.135min (-0.000) 5.18 ug/L m

response 1256

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	10.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022181.D
 Acq On : 04 Mar 2022 15:39
 Operator : SY/VA
 Sample : N1775-02
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRU8

Manual IntegrationsAPPROVED

Quant Time: Mar 05 03:23:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	135325	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	132951	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	66864	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.348	65	23425	13.272	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	53.080%	
7) Chloroethane-d5	2.885	69	19331	13.920	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	55.680%	
11) 1,1-Dichloroethene-d2	4.019	63	32783	12.129	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	48.520%	
21) 2-Butanone-d5	7.085	46	24792	83.540	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	167.080%#	
24) Chloroform-d	7.652	84	65158	21.581	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	86.320%	
26) 1,2-Dichloroethane-d4	8.305	65	38828	24.740	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	98.960%	
32) Benzene-d6	8.274	84	116414	18.814	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	75.240%	
36) 1,2-Dichloropropane-d6	9.274	67	35720	20.788	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	83.160%	
41) Toluene-d8	10.323	98	107719	17.511	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	70.040%	
43) trans-1,3-Dichloroprop...	10.579	79	15151	19.886	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	79.560%	
47) 2-Hexanone-d5	10.926	63	19799	70.056	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	140.120%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	44882	29.762	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	119.040%	
66) 1,2-Dichlorobenzene-d4	13.853	152	52833	24.601	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	98.400%	
Target Compounds						
13) Acetone	4.135	43	1256m	5.182	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
Data File : VW022181.D
Acq On : 04 Mar 2022 15:39
Operator : SY/VA
Sample : N1775-02
Misc : 5.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRU8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 05 03:23:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 05 03:21:21 2022
Response via : Initial Calibration

