

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022181.D
 Acq On : 04 Mar 2022 15:39
 Operator : SY/VA
 Sample : N1775-02
 Misc : 5.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRU8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

Quant Time: Mar 05 03:23:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	135325	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	132951	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	66864	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.348	65	23425	13.272	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	53.080%		
7) Chloroethane-d5	2.885	69	19331	13.920	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	55.680%		
11) 1,1-Dichloroethene-d2	4.019	63	32783	12.129	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	48.520%		
21) 2-Butanone-d5	7.085	46	24792	83.540	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	167.080%#		
24) Chloroform-d	7.652	84	65158	21.581	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	86.320%		
26) 1,2-Dichloroethane-d4	8.305	65	38828	24.740	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	98.960%		
32) Benzene-d6	8.274	84	116414	18.814	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	75.240%		
36) 1,2-Dichloropropane-d6	9.274	67	35720	20.788	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	83.160%		
41) Toluene-d8	10.323	98	107719	17.511	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	70.040%		
43) trans-1,3-Dichloroprop...	10.579	79	15151	19.886	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.560%		
47) 2-Hexanone-d5	10.926	63	19799	70.056	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	140.120%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	44882	29.762	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	119.040%		
66) 1,2-Dichlorobenzene-d4	13.853	152	52833	24.601	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.400%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	1256m	5.182	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
Data File : VW022181.D
Acq On : 04 Mar 2022 15:39
Operator : SY/VA
Sample : N1775-02
Misc : 5.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBRU8

Quant Time: Mar 05 03:23:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 05 03:21:21 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/05/2022
Supervised By :Mahesh Dadoda 03/07/2022

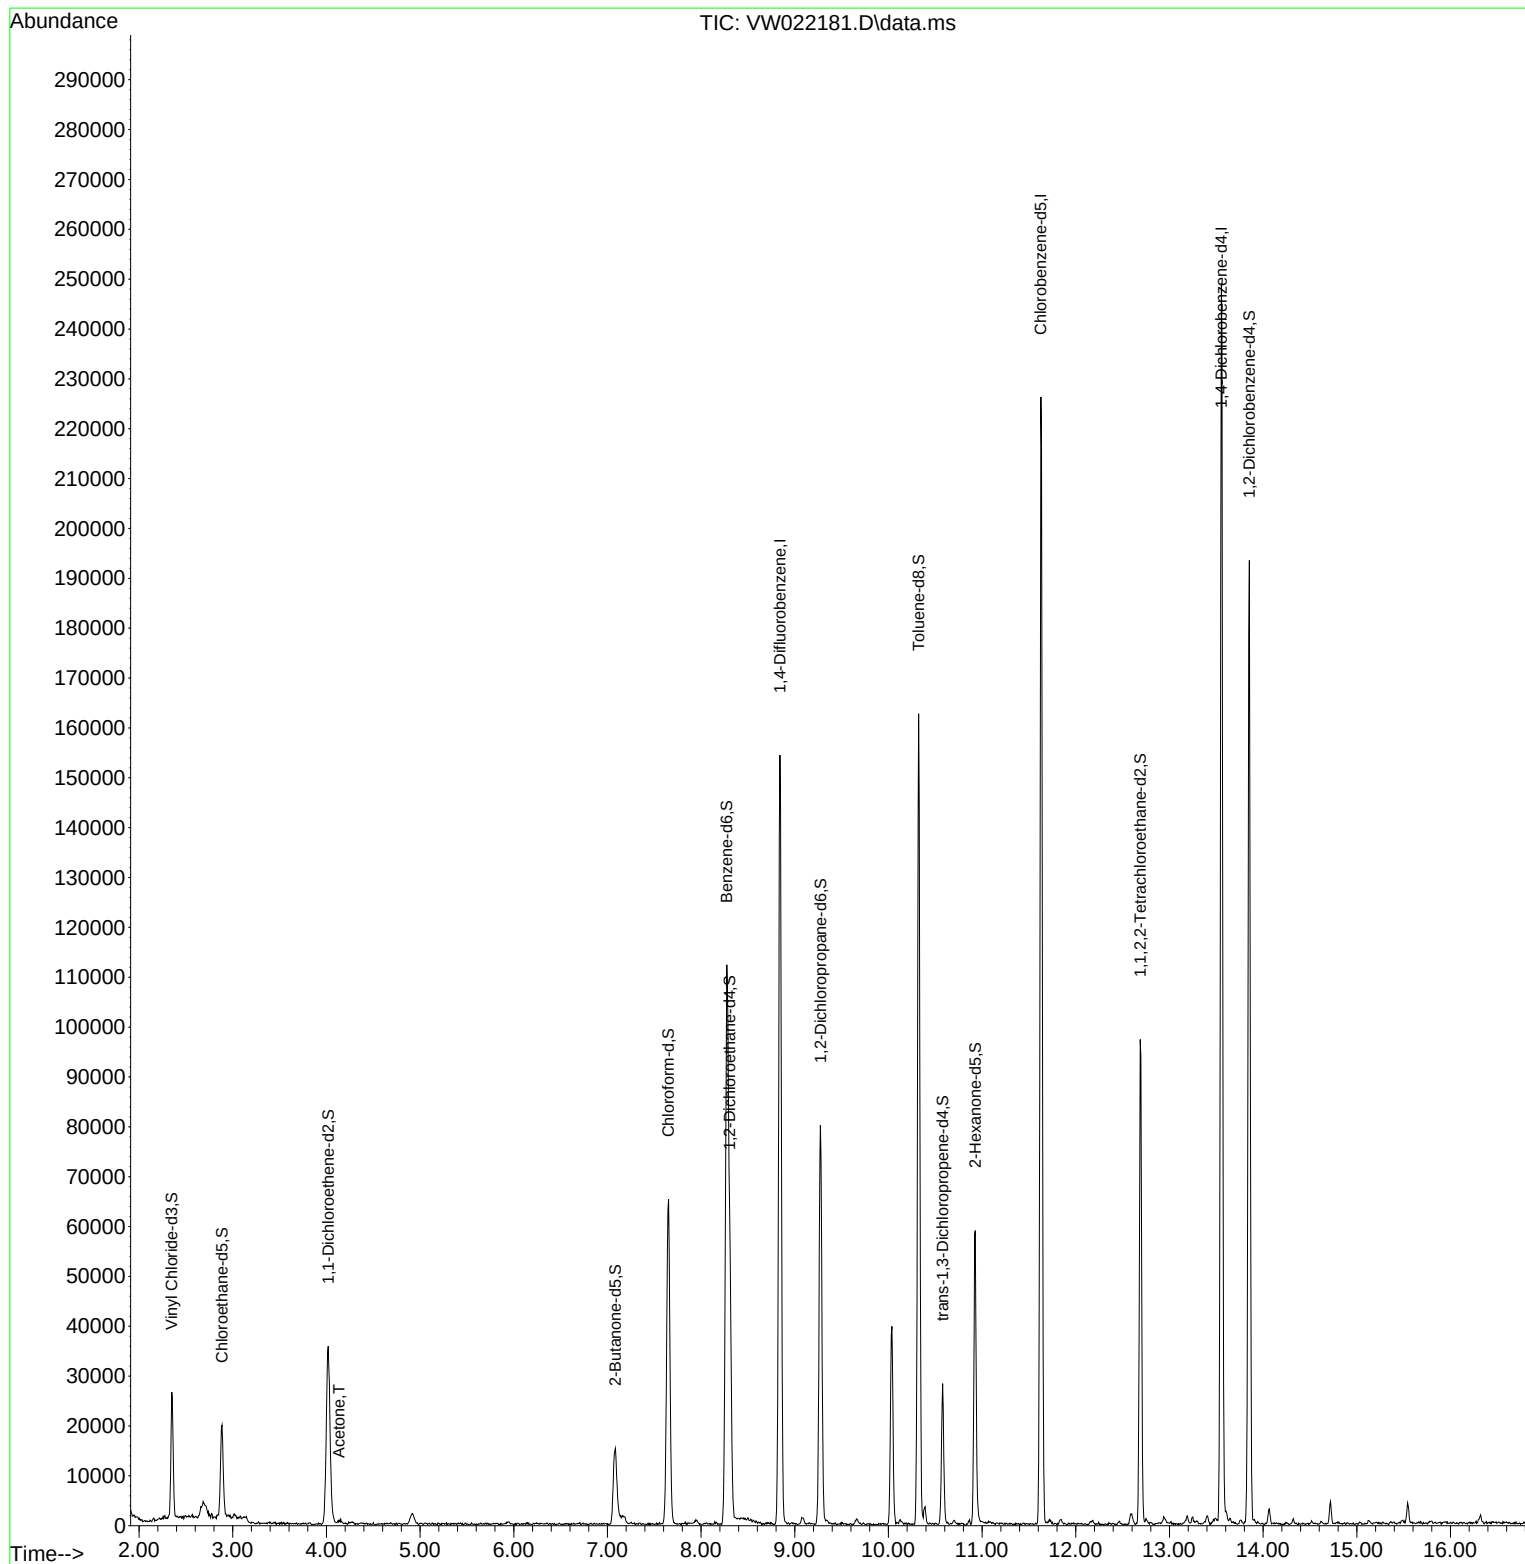

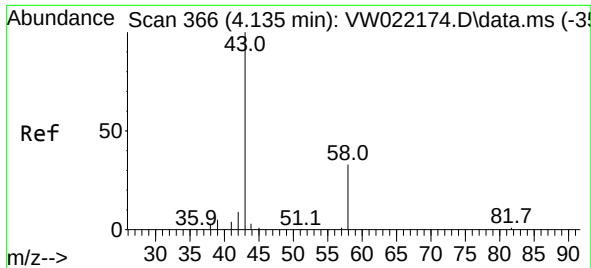

#13
 Acetone
 Concen: 5.182 ug/L m
 RT: 4.135 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW022181.D
 Acq: 04 Mar 2022 15:39

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRU8

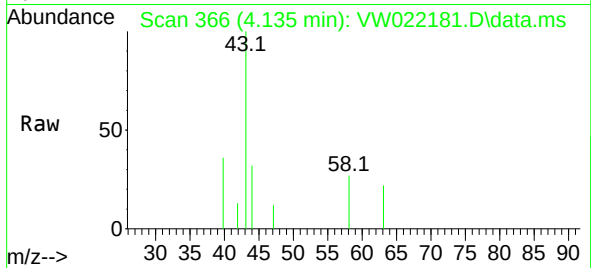

Tgt Ion: 43 Resp: 1250
 Ion Ratio Lower Upper
 43 100
 58 10.6 0.0 69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/05/2022
 Supervised By :Mahesh Dadoda 03/07/2022

