

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
 Data File : VW022183.D
 Acq On : 04 Mar 2022 16:27
 Operator : SY/VA
 Sample : N1733-21
 Misc : 4.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRT9

Quant Time: Mar 05 03:23:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Mar 05 03:21:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	246302	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	224530	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	117617	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	30425	9.471	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	37.880%
7) Chloroethane-d5	2.879	69	27125	10.731	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	42.920%
11) 1,1-Dichloroethene-d2	4.019	63	43008	8.742	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	34.960%#
21) 2-Butanone-d5	7.080	46	17028	31.525	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.060%
24) Chloroform-d	7.647	84	82405	14.995	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	60.000%
26) 1,2-Dichloroethane-d4	8.305	65	39960	13.989	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	55.960%#
32) Benzene-d6	8.275	84	147513	14.117	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	56.480%
36) 1,2-Dichloropropane-d6	9.275	67	43420	14.962	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	59.840%#
41) Toluene-d8	10.323	98	137117	13.199	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	52.800%
43) trans-1,3-Dichloroprop...	10.579	79	15680	12.186	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	48.760%
47) 2-Hexanone-d5	10.921	63	14118	29.579	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.160%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	37689	14.799	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	59.200%
66) 1,2-Dichlorobenzene-d4	13.853	152	57218	15.146	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	60.600%#
Target Compounds					Qvalue	
13) Acetone	4.135	43	2325	5.270	ug/L	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030422\
Data File : VW022183.D
Acq On : 04 Mar 2022 16:27
Operator : SY/VA
Sample : N1733-21
Misc : 4.82g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRT9


Quant Time: Mar 05 03:23:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Mar 05 03:21:21 2022
Response via : Initial Calibration

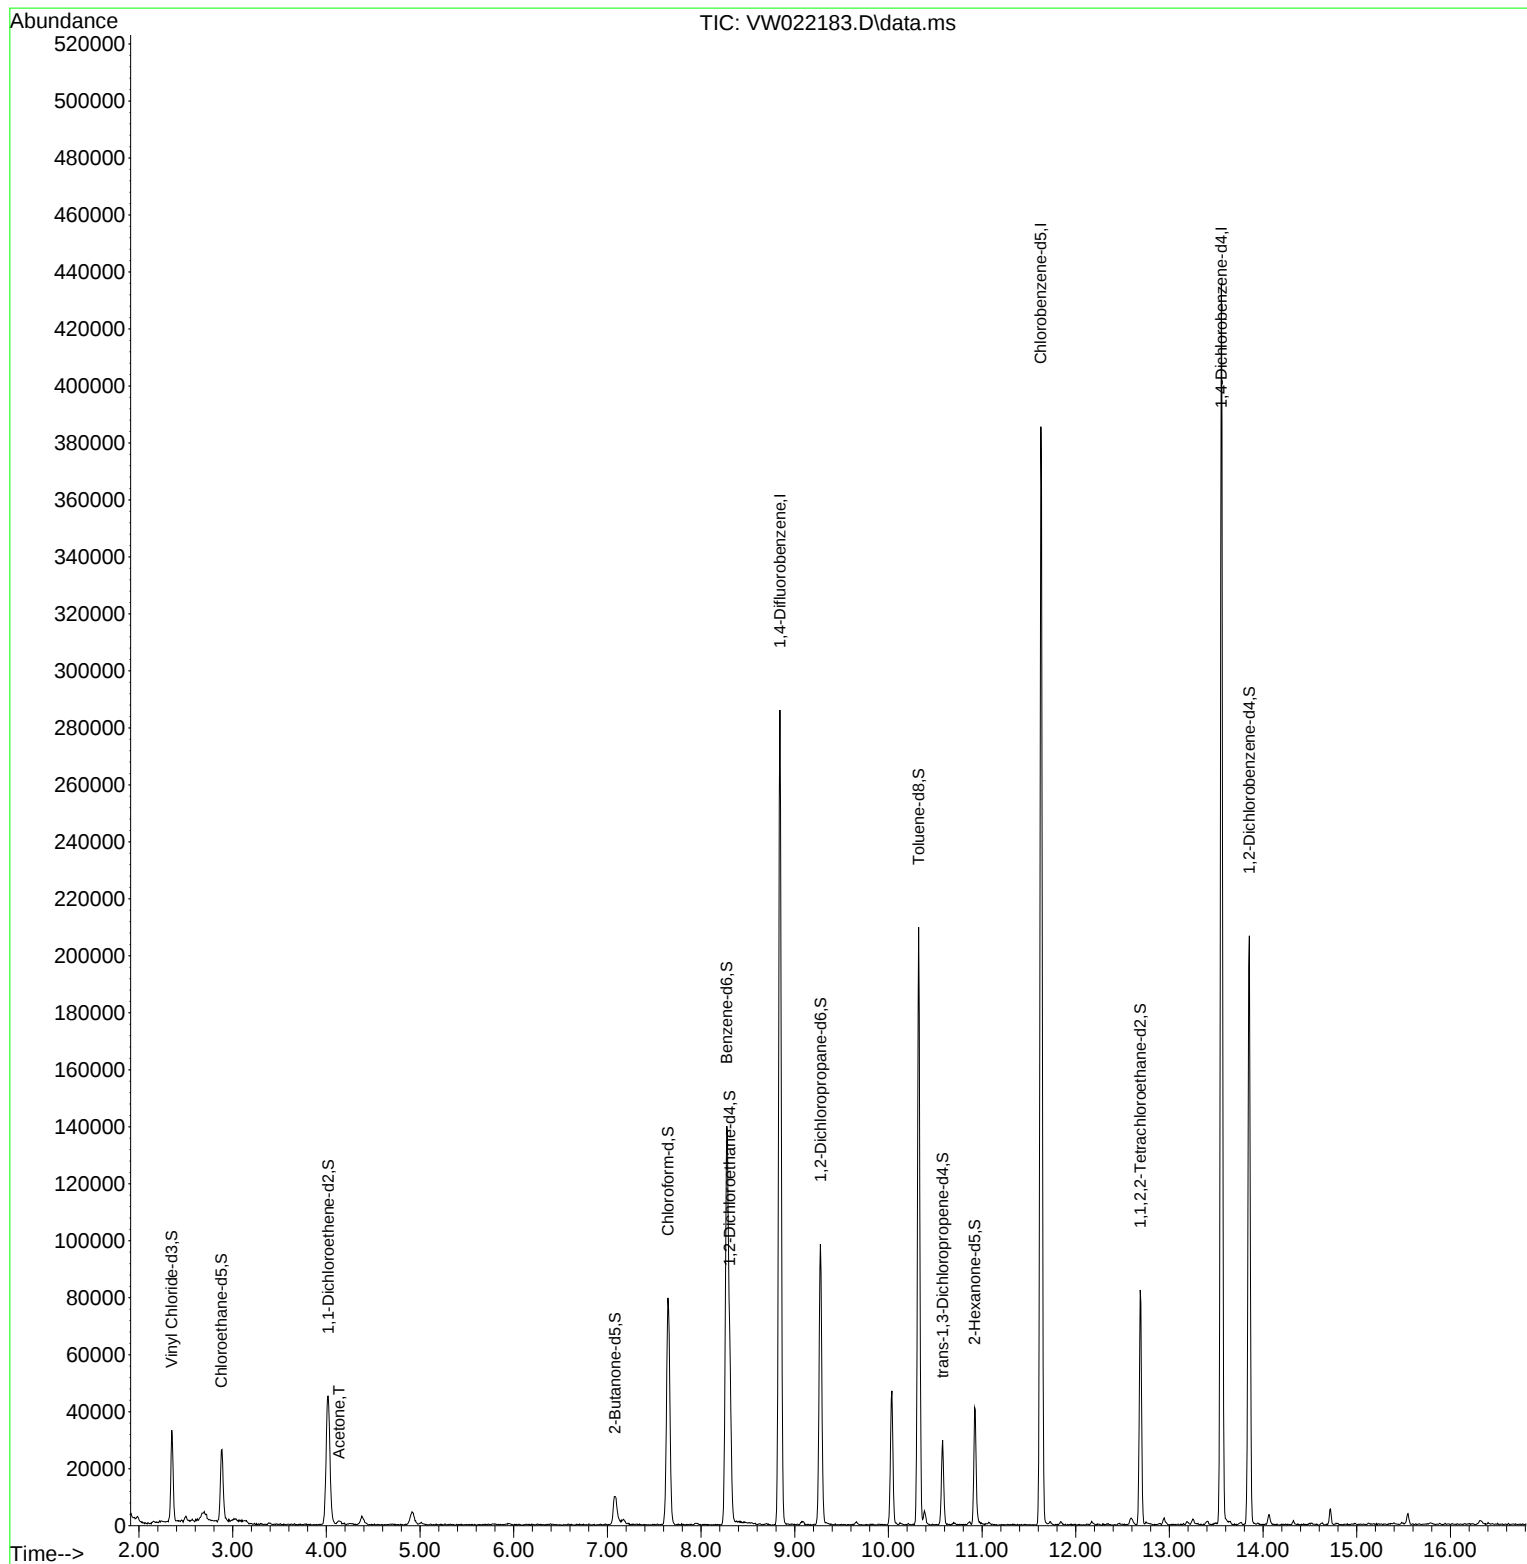

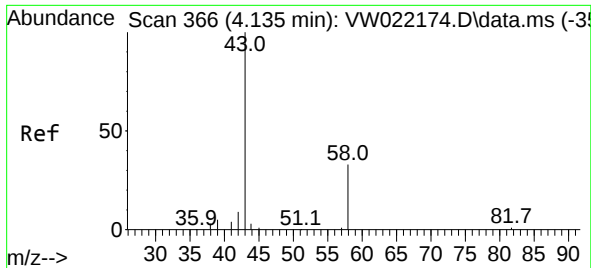

#13
 Acetone
 Concen: 5.270 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW022183.D
 Acq: 04 Mar 2022 16:27

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRT9

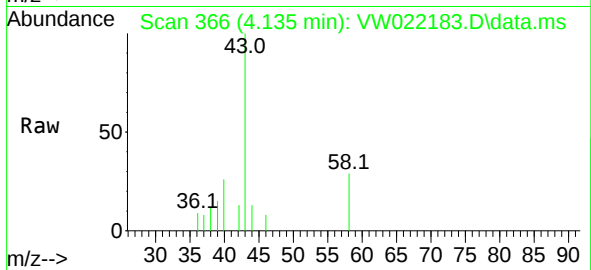

Tgt Ion: 43 Resp: 2325
 Ion Ratio Lower Upper
 43 100
 58 14.2 0.0 69.2

