

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030524\
 Data File : VW028096.D
 Acq On : 05 Mar 2024 16:26
 Operator : SY/MD
 Sample : P1677-09
 Misc : 11.49g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E06Y8

Quant Time: Mar 06 00:00:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 05 23:58:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	418442	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	373753	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.549	152	166466	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.368	65	101412	20.303	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.200%
7) Chloroethane-d5	2.899	69	73261	18.933	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.720%
11) 1,1-Dichloroethene-d2	4.027	65	43964	21.548	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.200%
21) 2-Butanone-d5	7.075	46	36315	50.966	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.940%
24) Chloroform-d	7.648	84	173186	19.541	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.160%
26) 1,2-Dichloroethane-d4	8.306	65	91222	22.116	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.480%
32) Benzene-d6	8.270	84	359012	20.576	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.320%
36) 1,2-Dichloropropane-d6	9.270	67	94341	20.928	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.720%
41) Toluene-d8	10.324	98	343842	20.912	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.640%
43) trans-1,3-Dichloroprop...	10.574	79	42680	21.605	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.440%
47) 2-Hexanone-d5	10.922	63	33856	53.320	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.640%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	81605	22.936	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.760%
66) 1,2-Dichlorobenzene-d4	13.848	152	104152	21.038	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.160%
Target Compounds						
13) Acetone	4.124	43	7077	7.106	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030524\
Data File : VW028096.D
Acq On : 05 Mar 2024 16:26
Operator : SY/MD
Sample : P1677-09
Misc : 11.49g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E06Y8

Quant Time: Mar 06 00:00:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 05 23:58:07 2024
Response via : Initial Calibration

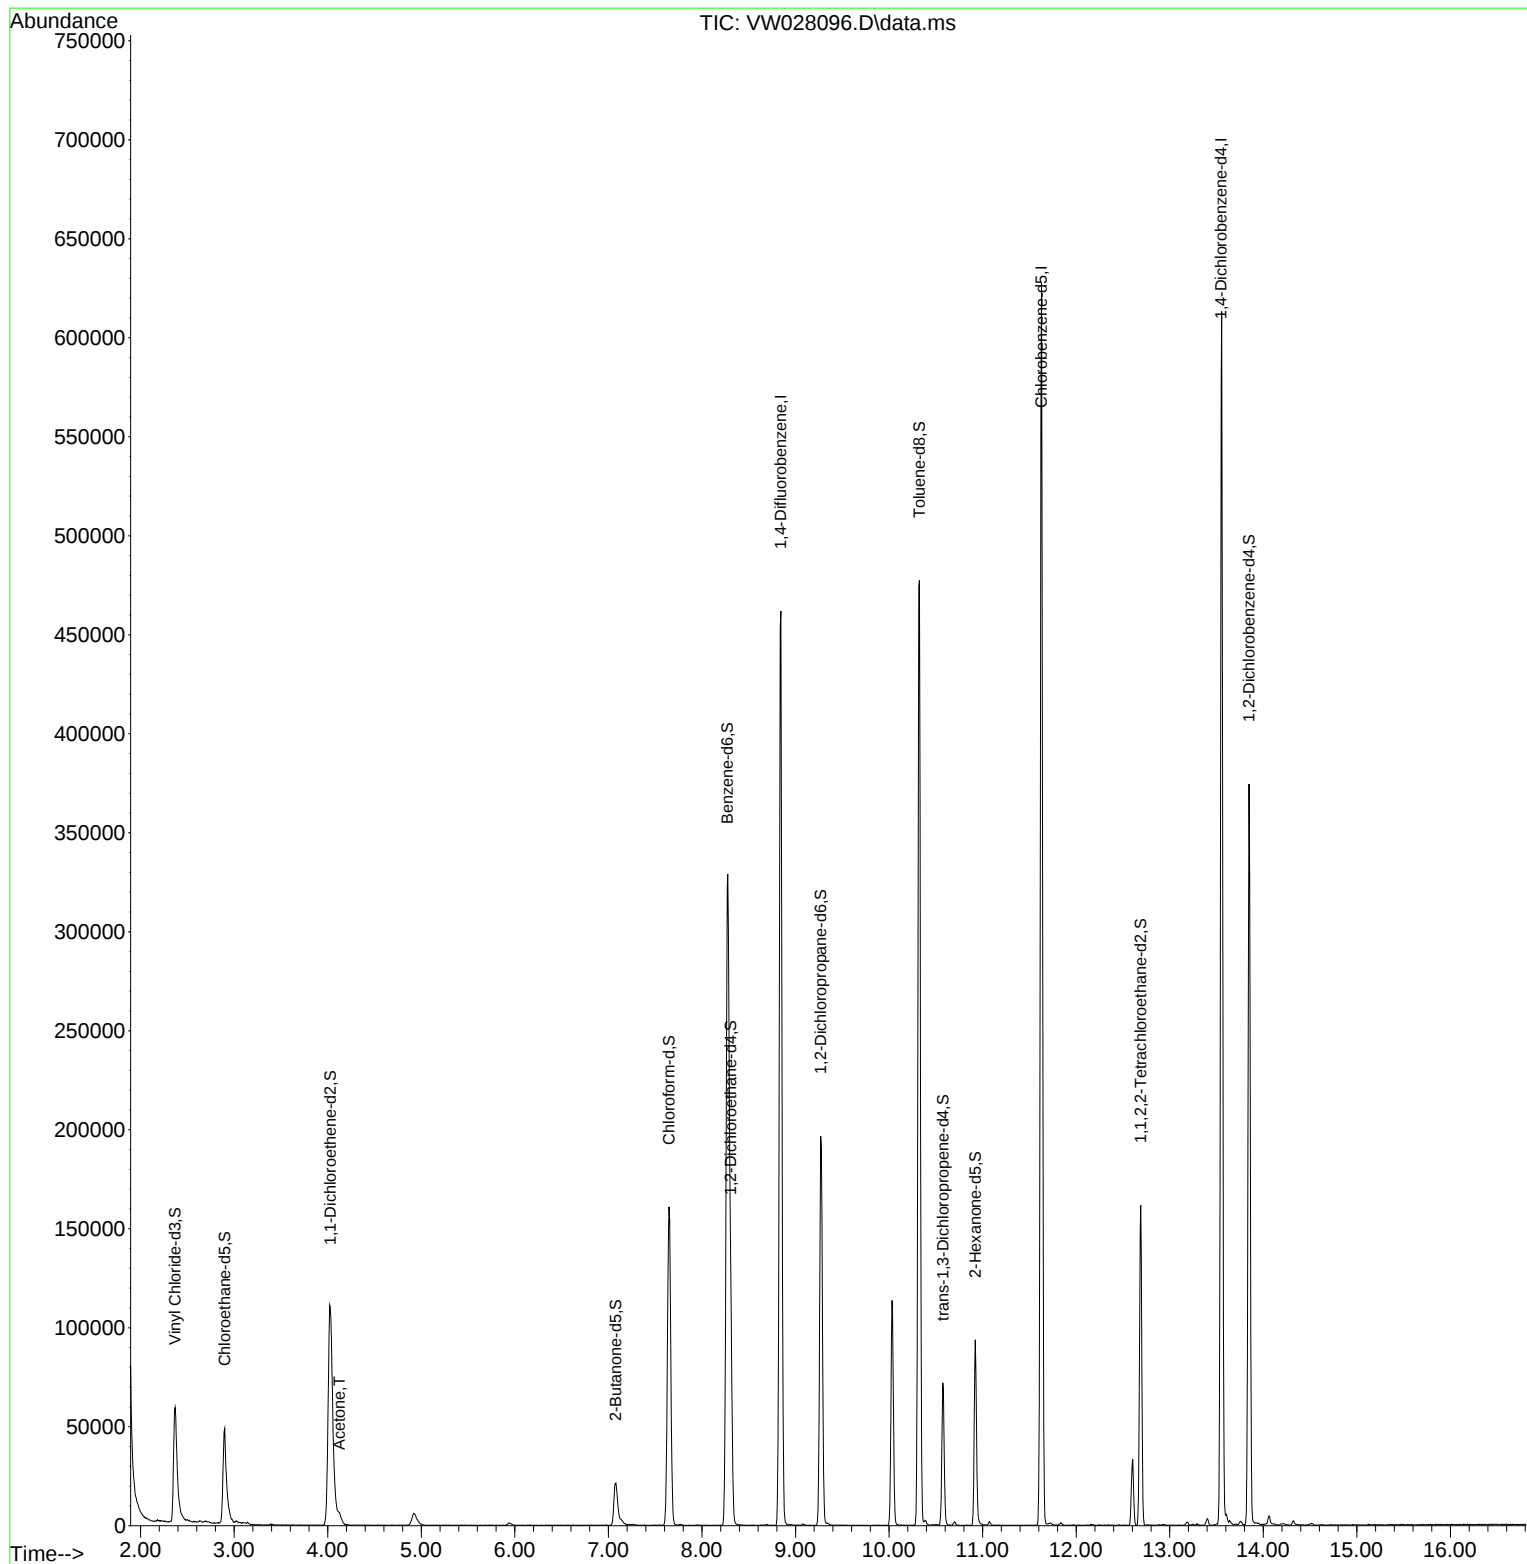

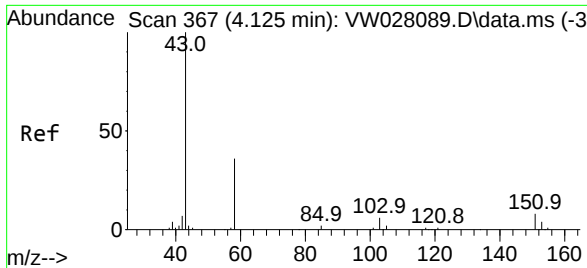

#13
 Acetone
 Concen: 7.106 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW028096.D
 Acq: 05 Mar 2024 16:26

Instrument :
 MSVOA_W
 ClientSampleId :
 E06Y8

Tgt Ion: 43 Resp: 7077
 Ion Ratio Lower Upper
 43 100
 58 32.8 0.0 70.0

