
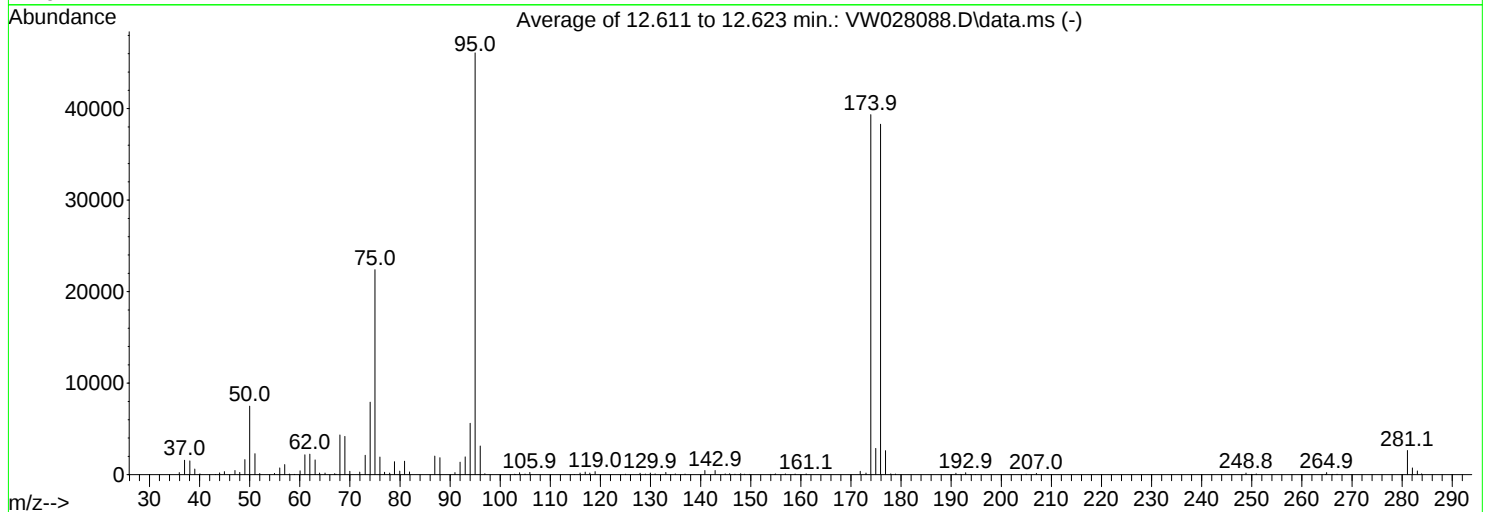


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030524\
Data File : VW028088.D
Acq On : 05 Mar 2024 09:11
Operator : SY/MD
Sample : BFB446
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB446

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Title : SFAM01.0
Last Update : Tue Mar 05 23:58:07 2024

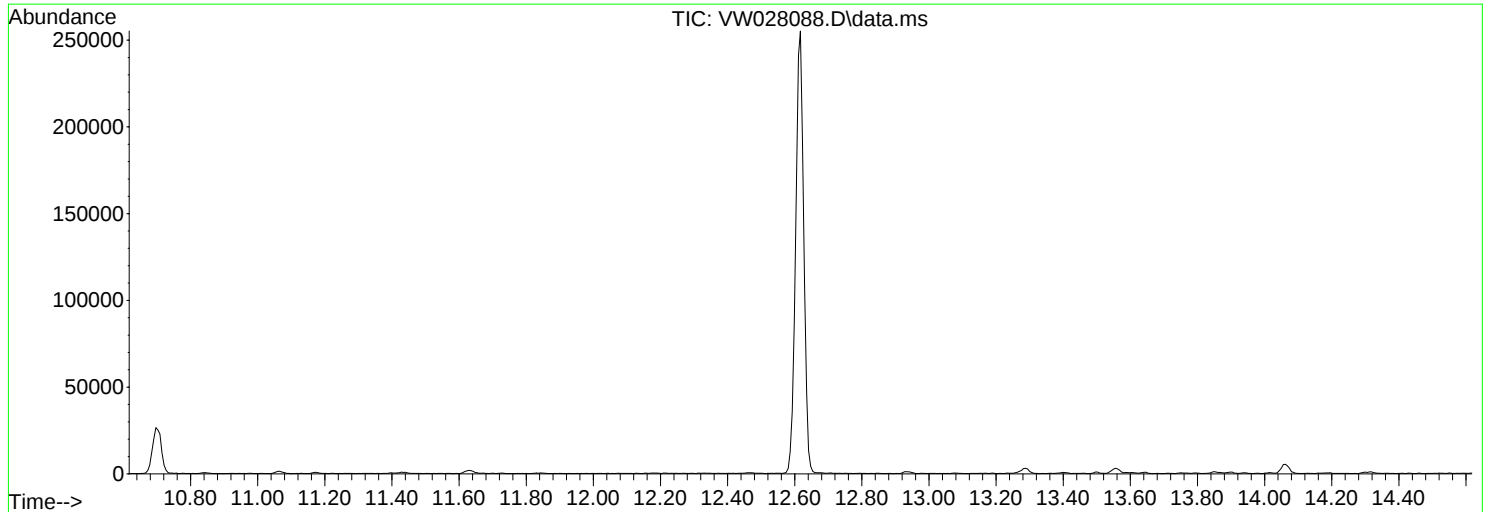

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	7482	PASS
75	95	30	80	48.6	22397	PASS
95	95	100	100	100.0	46096	PASS
96	95	5	9	6.8	3134	PASS
173	174	0.00	2	0.5	178	PASS
174	95	50	120	85.4	39347	PASS
175	174	5	9	7.3	2869	PASS
176	174	95	101	97.3	38291	PASS
177	176	5	9	6.8	2619	PASS

m/z	Abundance
35.90	91.0
40.10	90.0
44.00	86.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

m/z	Abundance
36.00	377.0
37.00	1746.0
38.10	1645.0
39.10	756.0
40.10	175.0
43.20	74.0
44.00	271.0
44.90	407.0
47.10	531.0
48.00	282.0
49.00	1651.0
50.00	8470.0
51.00	2448.0
52.00	95.0
54.90	145.0
56.00	643.0
57.00	1429.0
57.90	107.0
59.00	59.0
60.00	522.0
61.00	2379.0
62.00	2298.0
63.10	1733.0
64.00	149.0
65.10	212.0
67.20	139.0
68.00	4590.0
69.00	4485.0
70.00	373.0
72.00	308.0
73.10	2218.0
74.00	8485.0
75.00	24480.0
76.00	2148.0
76.90	282.0
78.00	227.0
78.90	1463.0
80.00	406.0
80.90	1511.0
81.90	303.0
87.00	2375.0
87.90	1930.0
90.90	283.0
92.00	1353.0
93.00	1928.0
94.00	5800.0
95.00	48488.0
96.00	3307.0
97.00	136.0
102.90	139.0
103.80	256.0
105.90	256.0
114.80	53.0
116.00	154.0
116.90	260.0
117.90	193.0
118.90	317.0
125.10	99.0
127.90	116.0
129.00	122.0
129.90	193.0
130.90	100.0
133.00	453.0
135.00	83.0
136.90	95.0
140.90	482.0
143.00	470.0
144.90	124.0
145.80	82.0
146.80	76.0
147.70	53.0
153.90	60.0
154.90	111.0
156.90	71.0
158.90	76.0
161.00	60.0
171.90	335.0
173.00	535.0
174.00	35256.0
174.90	2757.0
175.90	39672.0
176.90	2524.0
177.90	90.0
178.90	107.0
191.00	291.0
191.90	86.0
192.90	365.0
193.90	50.0
194.80	79.0
205.00	103.0
207.00	209.0
208.10	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

248.80	219.0
250.00	106.0
250.90	148.0
264.90	495.0
266.10	117.0
267.00	65.0
281.10	4997.0
282.00	1332.0
283.10	712.0
283.90	135.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

m/z	Abundance
36.00	377.0
37.00	1659.0
38.10	1605.0
39.00	573.0
40.00	162.0
44.00	311.0
45.00	342.0
47.10	426.0
48.00	289.0
49.10	1987.0
50.00	8013.0
51.00	2691.0
52.10	135.0
55.00	136.0
56.00	940.0
57.00	1095.0
57.90	86.0
58.80	58.0
60.10	444.0
61.00	2368.0
62.00	2526.0
63.10	1749.0
63.90	185.0
64.90	160.0
66.90	195.0
68.00	4850.0
69.00	4735.0
70.00	499.0
72.00	254.0
73.00	2397.0
74.00	8984.0
75.00	24320.0
76.00	2081.0
76.80	246.0
77.90	212.0
78.90	1564.0
79.90	440.0
80.90	1695.0
81.90	338.0
87.00	2148.0
88.00	2019.0
91.00	251.0
92.00	1588.0
93.00	2207.0
94.00	6373.0
95.00	52464.0
96.00	3504.0
96.90	92.0
103.10	71.0
103.90	225.0
104.90	94.0
105.80	284.0
115.90	207.0
117.00	347.0
117.80	191.0
118.90	404.0
124.90	83.0
127.80	212.0
128.90	94.0
129.90	188.0
130.90	102.0
133.10	190.0
134.00	70.0
134.90	104.0
136.90	102.0
140.90	502.0
142.90	491.0
144.90	91.0
145.80	139.0
146.90	68.0
148.00	188.0
148.80	74.0
149.80	57.0
153.90	50.0
155.00	135.0
156.90	95.0
158.80	60.0
161.00	115.0
171.80	453.0
173.90	43120.0
174.90	3125.0
175.90	44544.0
176.90	3007.0
177.90	91.0
178.90	87.0
190.90	185.0
192.90	253.0
204.90	54.0
207.00	110.0
248.90	216.0
250.90	118.0
265.00	185.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

267.00	90.0
280.90	1649.0
282.10	664.0
283.00	363.0
283.90	143.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446

m/z	Abundance
36.10	225.0
37.00	1302.0
38.00	1260.0
39.10	503.0
40.00	193.0
44.00	276.0
45.00	272.0
46.90	391.0
48.00	176.0
49.00	1321.0
50.00	5962.0
51.10	1718.0
51.90	118.0
54.90	143.0
56.00	639.0
57.00	808.0
60.00	272.0
61.00	1748.0
62.00	1877.0
63.00	1343.0
64.00	176.0
65.10	175.0
67.00	102.0
68.00	3577.0
69.00	3333.0
70.00	241.0
71.90	260.0
73.00	1712.0
74.10	6322.0
75.00	18392.0
76.00	1520.0
77.00	283.0
78.00	76.0
78.90	1247.0
79.90	299.0
80.90	1216.0
81.90	238.0
86.90	1577.0
88.00	1625.0
90.90	128.0
92.00	1151.0
93.00	1708.0
94.00	4666.0
95.00	37336.0
96.00	2592.0
97.00	69.0
103.90	154.0
105.00	105.0
106.00	190.0
116.00	160.0
116.90	249.0
118.00	162.0
119.00	256.0
128.00	145.0
130.00	167.0
131.00	51.0
132.90	73.0
135.00	97.0
140.80	381.0
142.80	421.0
144.80	52.0
145.80	90.0
148.00	129.0
148.80	76.0
149.80	75.0
154.70	132.0
156.90	74.0
158.90	75.0
161.10	91.0
171.90	311.0
173.90	39664.0
175.00	2724.0
175.90	30656.0
176.90	2326.0
178.00	81.0
206.90	96.0
248.90	85.0
264.70	108.0
281.00	1266.0
282.00	226.0
283.10	150.0

Instrument :
MSVOA_W
ClientSampleId :
BFB446