

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022191.D
 Acq On : 07 Mar 2022 11:07
 Operator : SY/VA
 Sample : VW0307SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK463

Quant Time: Mar 08 00:22:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	169940	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	157352	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	79446	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	58159	26.239	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.960%
7) Chloroethane-d5	2.891	69	38302	21.962	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.840%
11) 1,1-Dichloroethene-d2	4.019	63	69171	20.378	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.520%
21) 2-Butanone-d5	7.086	46	17491	46.933	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.860%
24) Chloroform-d	7.653	84	100970	26.630	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	106.520%
26) 1,2-Dichloroethane-d4	8.305	65	51739	26.251	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.000%
32) Benzene-d6	8.274	84	199336	27.220	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.880%
36) 1,2-Dichloropropane-d6	9.274	67	54487	26.792	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.160%
41) Toluene-d8	10.323	98	197810	27.170	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.680%
43) trans-1,3-Dichloroprop...	10.579	79	22920	25.418	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.680%
47) 2-Hexanone-d5	10.926	63	14547	43.490	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.980%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	42657	23.900	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	67620	26.500	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.000%
Target Compounds						Qvalue
34) Trichloroethene	8.848	95	5038	2.313	ug/L	# 4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022191.D
Acq On : 07 Mar 2022 11:07
Operator : SY/VA
Sample : VW0307SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK463


Quant Time: Mar 08 00:22:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

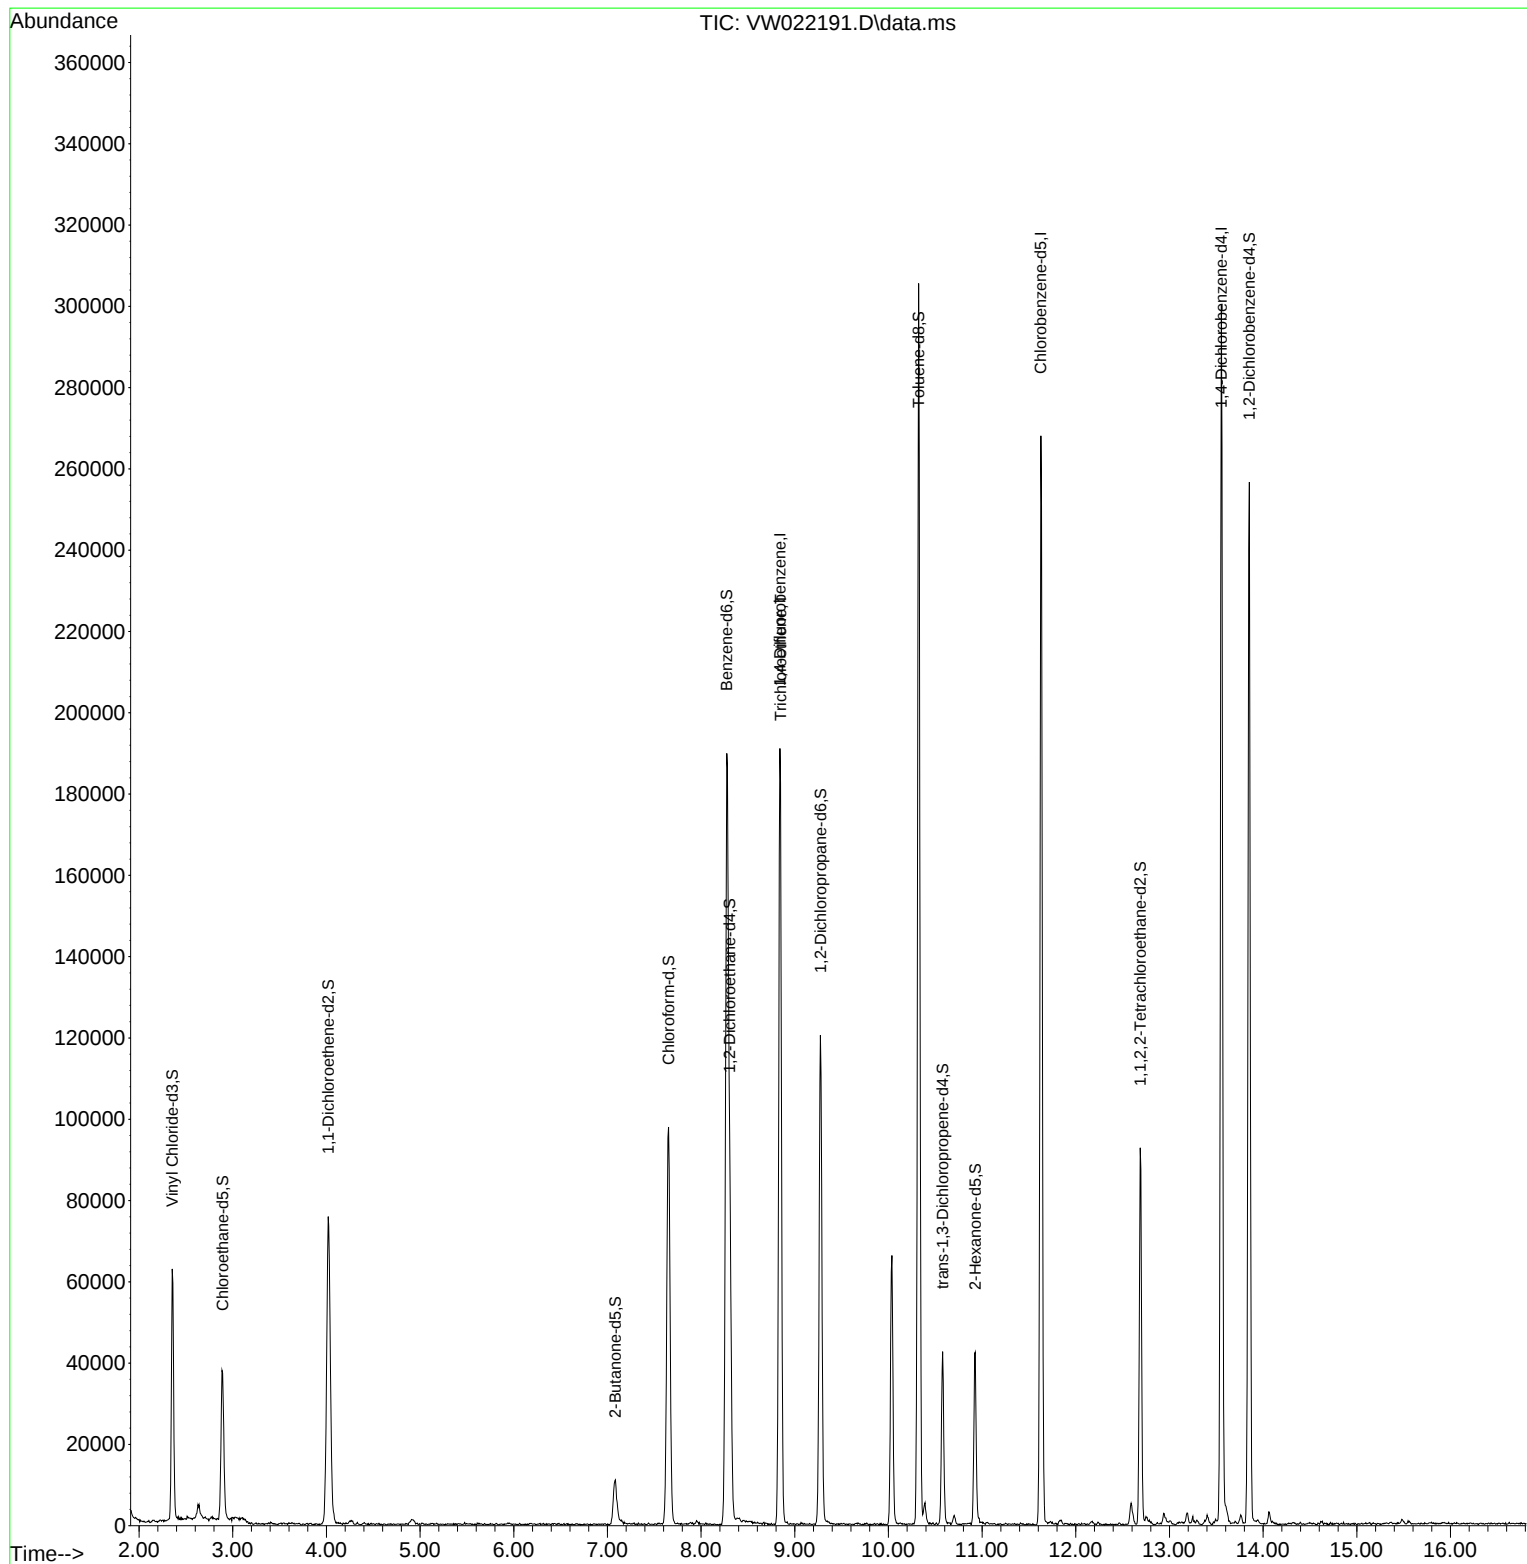

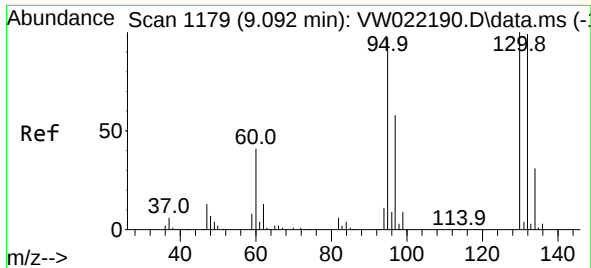

#34
 Trichloroethene
 Concen: 2.313 ug/L
 RT: 8.848 min Scan# 1179
 Delta R.T. -0.244 min
 Lab File: VW022191.D
 Acq: 07 Mar 2022 11:07

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK463

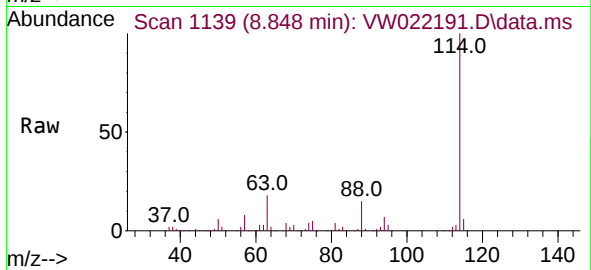

Tgt Ion: 95 Resp: 5038

Ion	Ratio	Lower	Upper
95	100		
97	0.0	44.4	82.4#
132	0.0	71.7	133.1#
130	0.0	71.7	133.1#

