

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022193.D
 Acq On : 07 Mar 2022 11:57
 Operator : SY/VA
 Sample : N1775-12
 Misc : 6.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRU6

Quant Time: Mar 08 00:22:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	176384	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	169094	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	82305	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	30296	13.169	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.680%
7) Chloroethane-d5	2.885	69	27558	15.224	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.880%
11) 1,1-Dichloroethene-d2	4.019	63	41720	11.842	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	47.360%
21) 2-Butanone-d5	7.080	46	20397	52.731	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.460%
24) Chloroform-d	7.653	84	83259	21.157	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.640%
26) 1,2-Dichloroethane-d4	8.305	65	43685	21.355	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	85.440%
32) Benzene-d6	8.275	84	146044	18.558	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.240%
36) 1,2-Dichloropropane-d6	9.275	67	44725	20.465	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.840%
41) Toluene-d8	10.323	98	137343	17.554	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.200%
43) trans-1,3-Dichloroprop...	10.579	79	17051	17.596	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.400%
47) 2-Hexanone-d5	10.927	63	17450	48.547	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.100%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	43054	22.447	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.800%
66) 1,2-Dichlorobenzene-d4	13.853	152	60225	22.782	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.120%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	1630	0.562	ug/L	# 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022193.D
Acq On : 07 Mar 2022 11:57
Operator : SY/VA
Sample : N1775-12
Misc : 6.36g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRU6

Quant Time: Mar 08 00:22:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

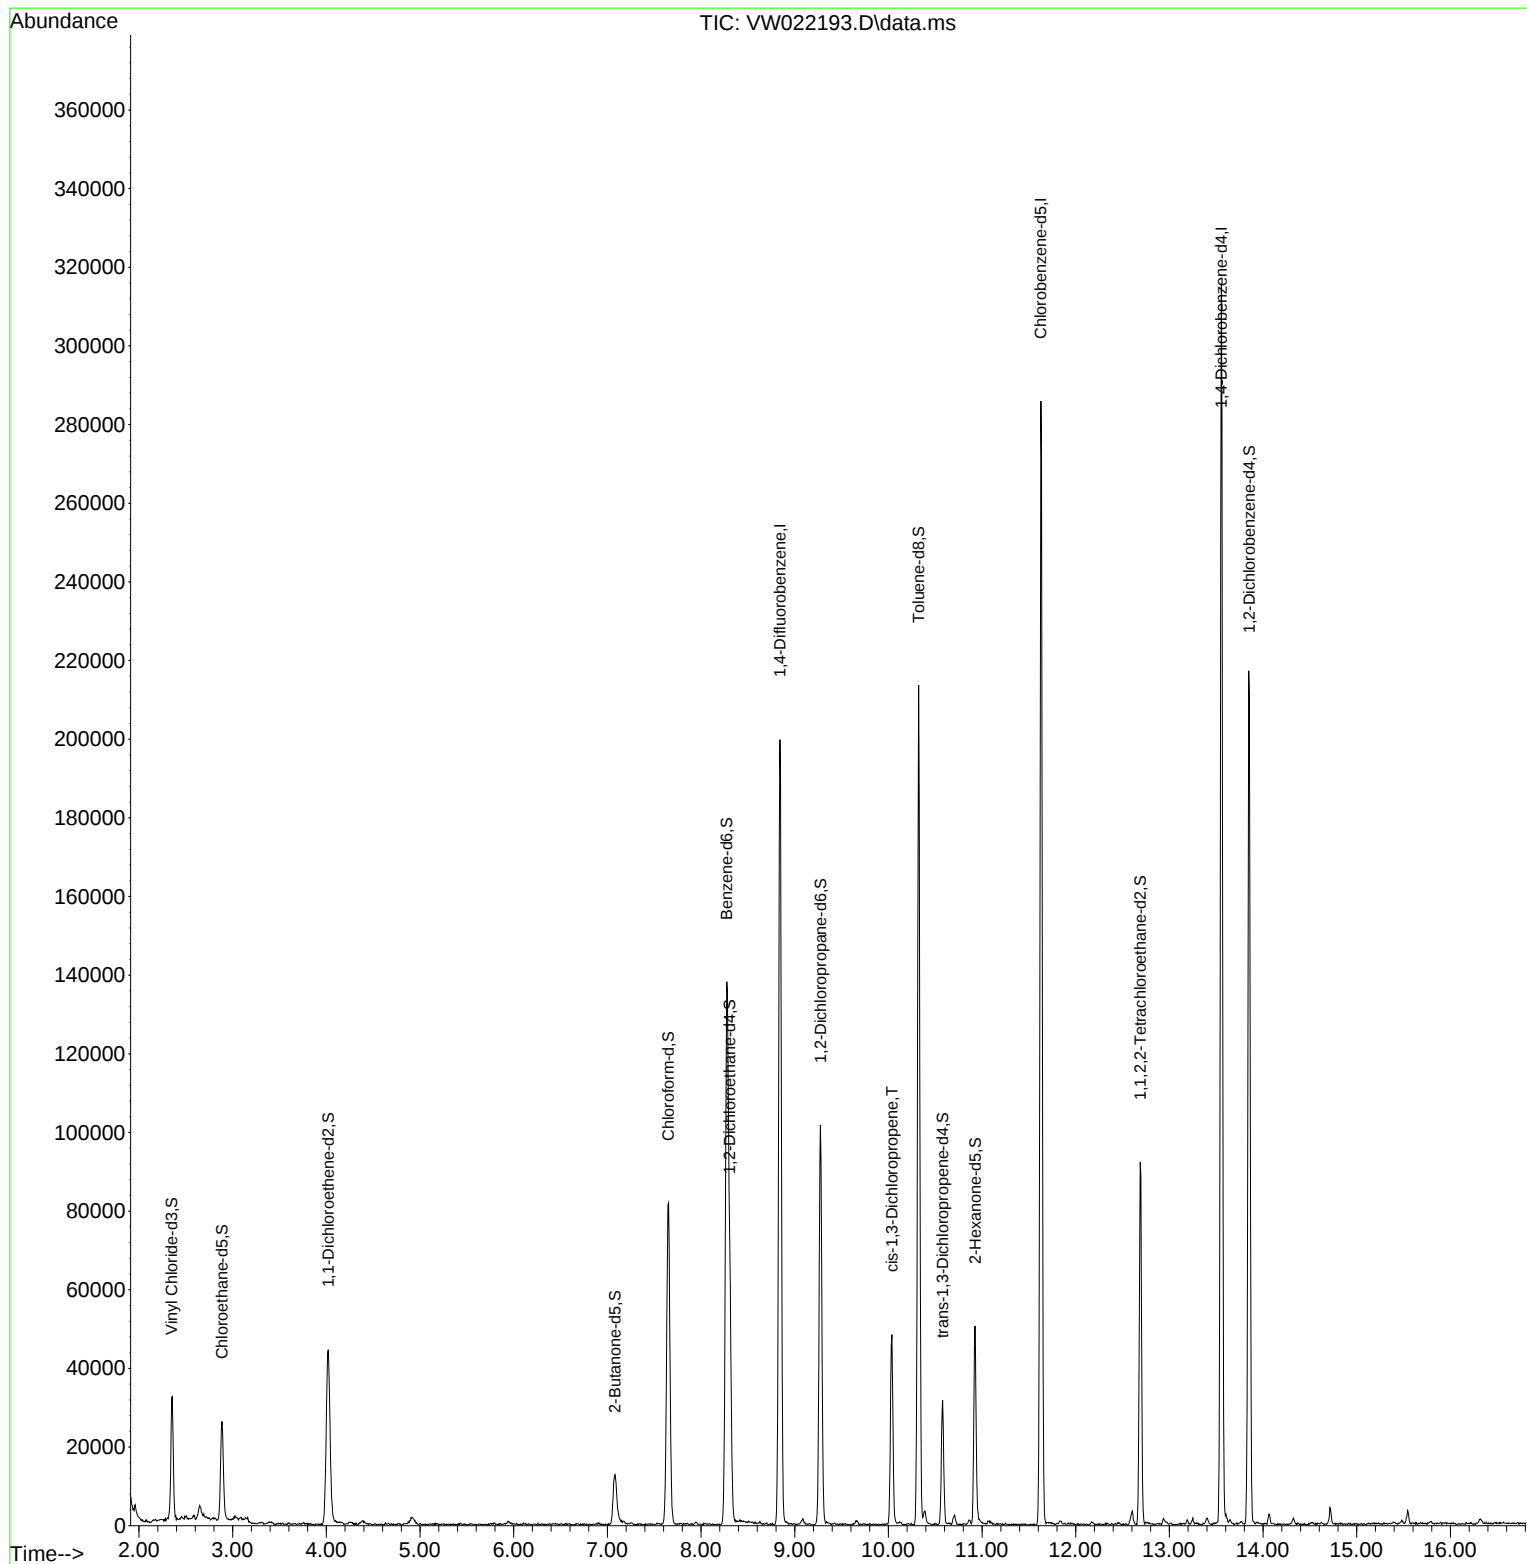

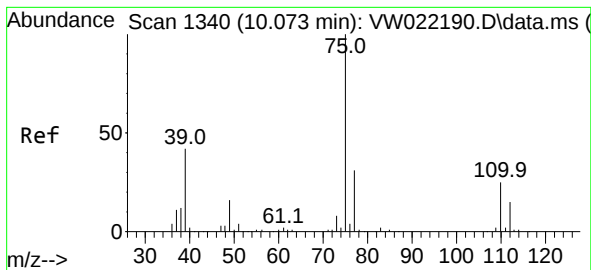

#39
 cis-1,3-Dichloropropene
 Concen: 0.562 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW022193.D
 Acq: 07 Mar 2022 11:57

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRU6

Tgt Ion: 75 Resp: 1630
 Ion Ratio Lower Upper
 75 100
 77 51.6 20.6 38.2#

