

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022197.D
 Acq On : 07 Mar 2022 13:40
 Operator : SY/VA
 Sample : N1775-15
 Misc : 5.51g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB8

Quant Time: Mar 08 00:24:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	155632	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	149835	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	73360	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	49867	24.566	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.280%
7) Chloroethane-d5	2.885	69	34639	21.688	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.760%
11) 1,1-Dichloroethene-d2	4.013	63	58561	18.839	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.360%
21) 2-Butanone-d5	7.080	46	17835	52.256	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.520%
24) Chloroform-d	7.653	84	87668	25.247	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.000%
26) 1,2-Dichloroethane-d4	8.305	65	47884	26.529	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.120%
32) Benzene-d6	8.275	84	177401	25.440	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.760%
36) 1,2-Dichloropropane-d6	9.274	67	49220	25.416	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.680%
41) Toluene-d8	10.323	98	170667	24.618	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.480%
43) trans-1,3-Dichloroprop...	10.579	79	20944	24.392	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.560%
47) 2-Hexanone-d5	10.926	63	14968	46.994	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.980%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	41853	24.626	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.520%
66) 1,2-Dichlorobenzene-d4	13.853	152	60262	25.575	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.320%
Target Compounds						Qvalue
13) Acetone	4.129	43	1143	4.100	ug/L	93
39) cis-1,3-Dichloropropene	10.042	75	2021	0.787	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022197.D
Acq On : 07 Mar 2022 13:40
Operator : SY/VA
Sample : N1775-15
Misc : 5.51g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSB8

Quant Time: Mar 08 00:24:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

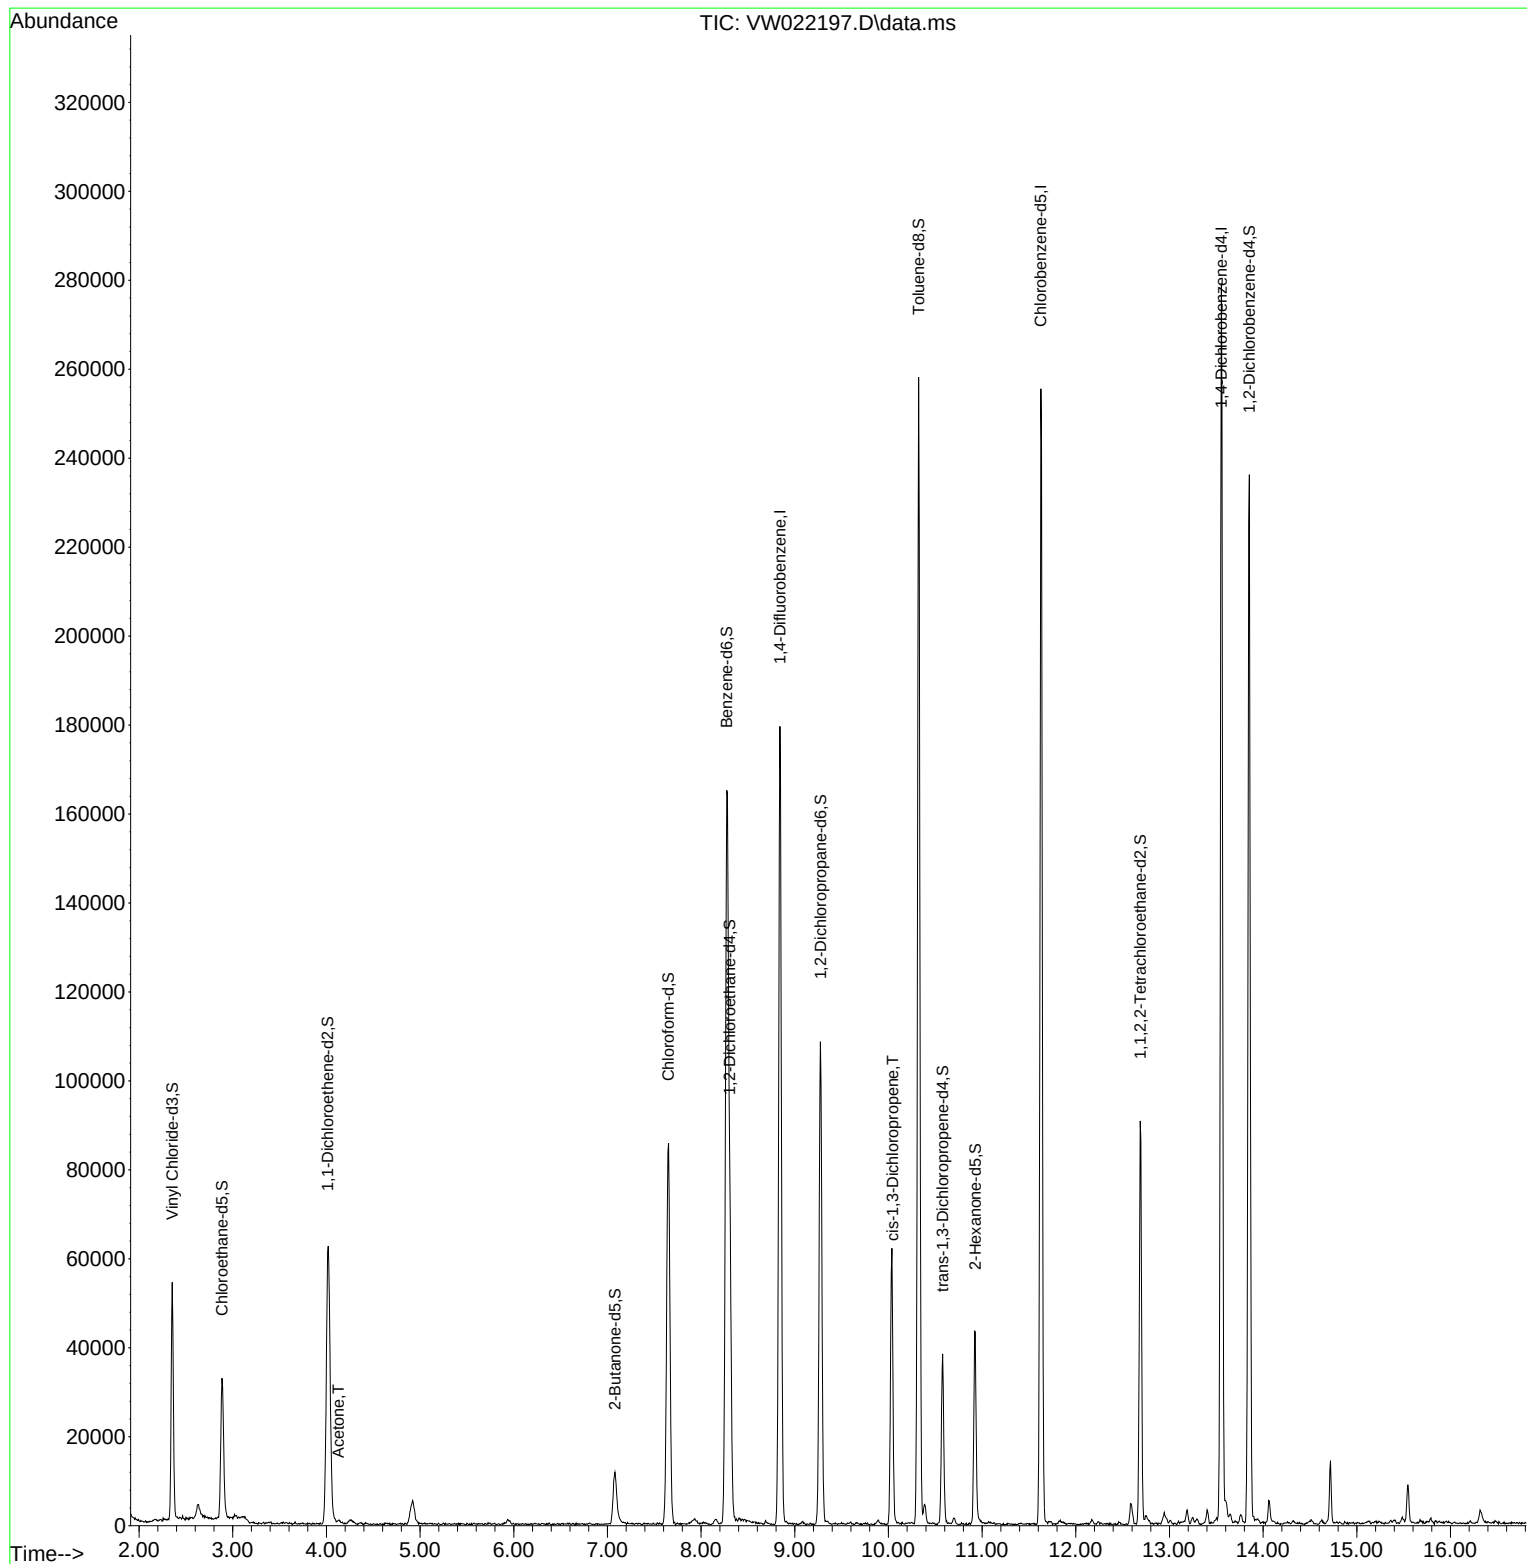

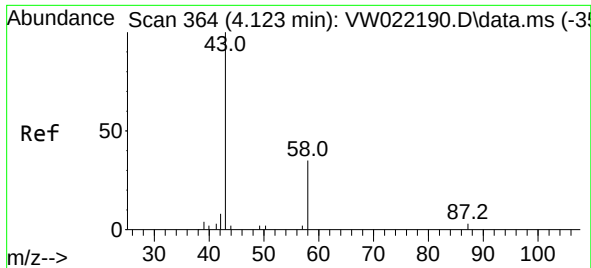

#13

Acetone

Concen: 4.100 ug/L

RT: 4.129 min Scan# 3

Delta R.T. 0.006 min

Lab File: VW022197.D

Acq: 07 Mar 2022 13:40

Instrument :

MSVOA_W

ClientSampleId :





DBSB8

Tgt Ion: 43 Resp: 1143

Ion Ratio Lower Upper

43 100

58 30.6 0.0 69.2

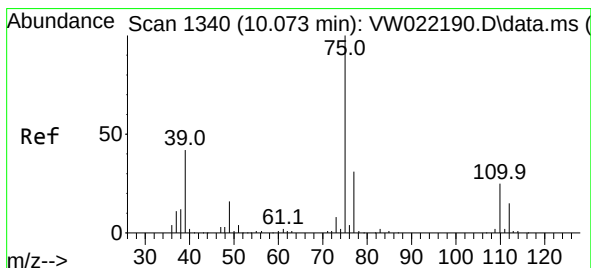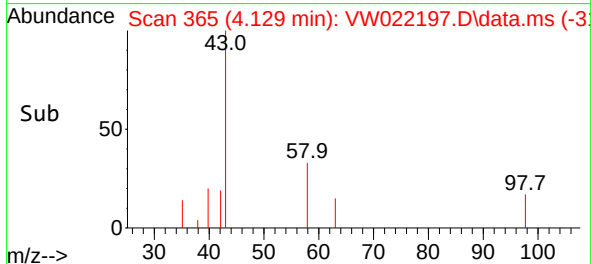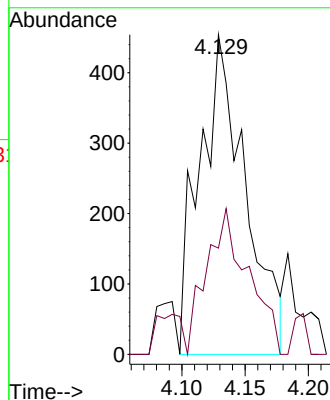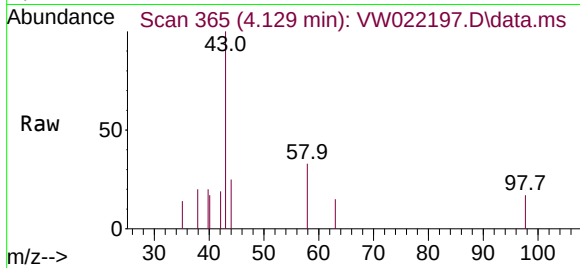

#39

cis-1,3-Dichloropropene

Concen: 0.787 ug/L

RT: 10.042 min Scan# 1335

Delta R.T. -0.031 min

Lab File: VW022197.D

Acq: 07 Mar 2022 13:40

Tgt Ion: 75 Resp: 2021

Ion Ratio Lower Upper

75 100

77 34.4 20.6 38.2

