

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022198.D
 Acq On : 07 Mar 2022 14:04
 Operator : SY/VA
 Sample : N1775-16
 Misc : 5.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB9

Quant Time: Mar 08 00:24:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	170754	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	164536	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	86575	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	50015	22.457	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.840%
7) Chloroethane-d5	2.885	69	35613	20.323	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.280%
11) 1,1-Dichloroethene-d2	4.019	63	59039	17.310	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.240%
21) 2-Butanone-d5	7.074	46	17589	46.971	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.940%
24) Chloroform-d	7.653	84	86622	22.737	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.960%
26) 1,2-Dichloroethane-d4	8.305	65	48141	24.309	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.240%
32) Benzene-d6	8.275	84	178125	23.261	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.040%
36) 1,2-Dichloropropane-d6	9.275	67	48859	22.976	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.920%
41) Toluene-d8	10.323	98	172167	22.615	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.480%
43) trans-1,3-Dichloroprop...	10.579	79	21011	22.284	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.120%
47) 2-Hexanone-d5	10.927	63	13959	39.910	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.820%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	39928	21.394	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	62535	22.489	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.960%
Target Compounds						Qvalue
34) Trichloroethene	8.848	95	5277	2.317	ug/L #	4
39) cis-1,3-Dichloropropene	10.037	75	1871	0.663	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022198.D
Acq On : 07 Mar 2022 14:04
Operator : SY/VA
Sample : N1775-16
Misc : 5.92g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSB9

Quant Time: Mar 08 00:24:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration




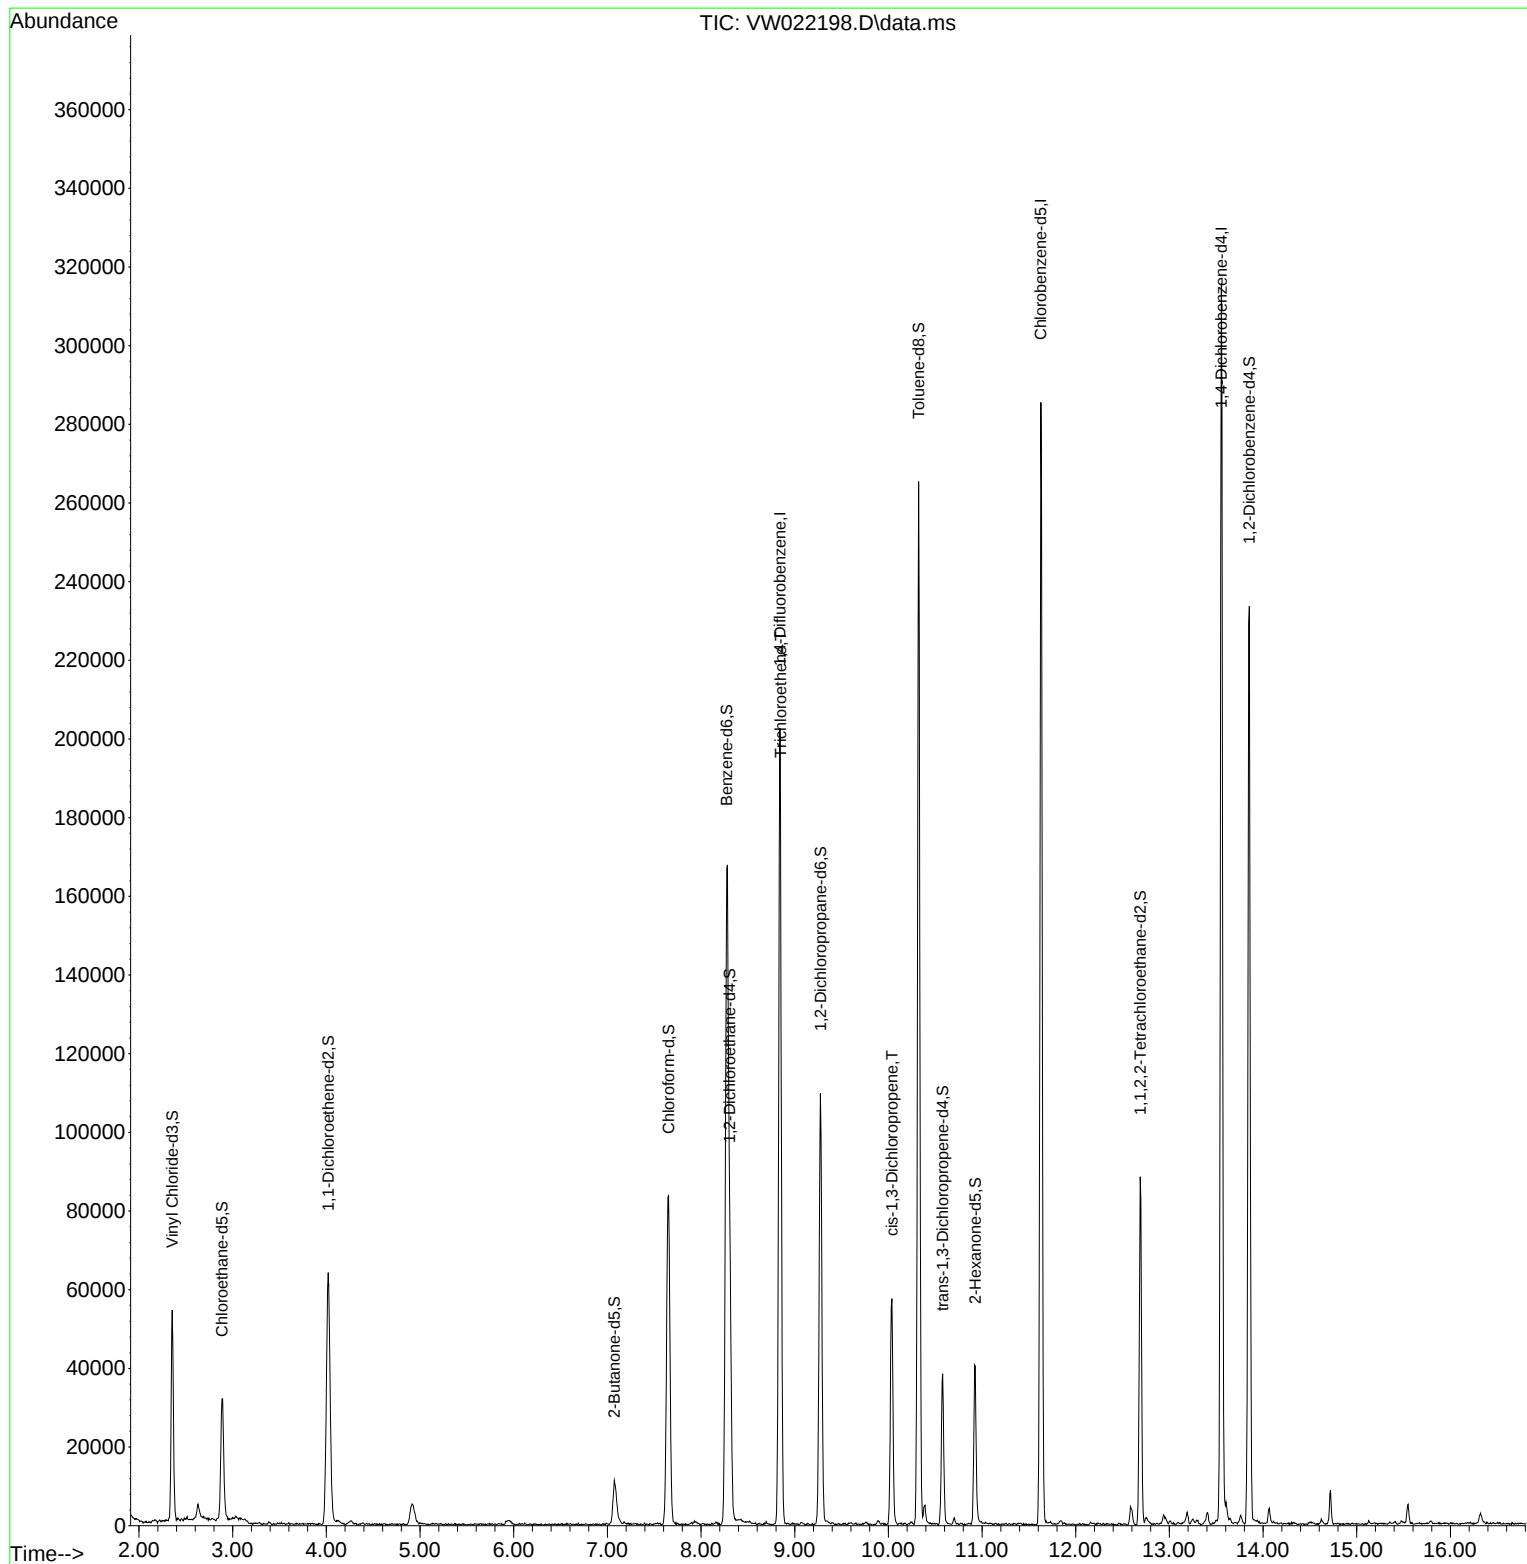


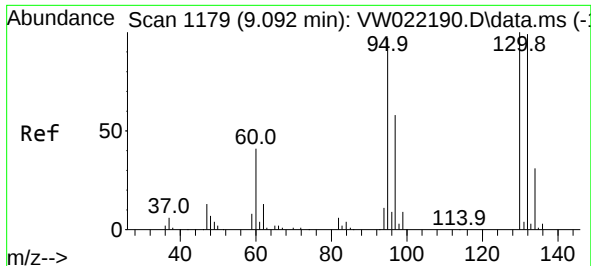

#34
 Trichloroethene
 Concen: 2.317 ug/L
 RT: 8.848 min Scan# 1139
 Delta R.T. -0.244 min
 Lab File: VW022198.D
 Acq: 07 Mar 2022 14:04

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB9

Tgt Ion: 95 Resp: 5277
 Ion Ratio Lower Upper
 95 100
 97 0.0 44.4 82.4#
 132 0.0 71.7 133.1#
 130 0.0 71.7 133.1#

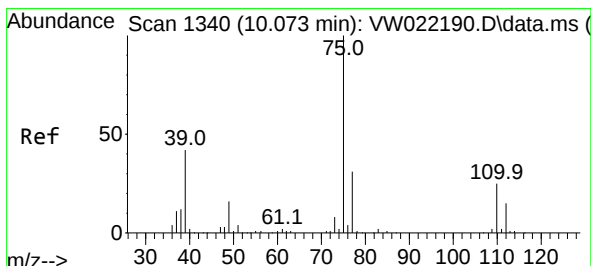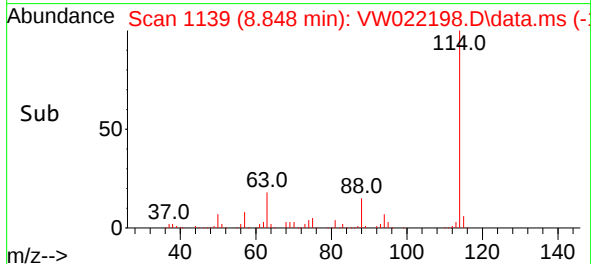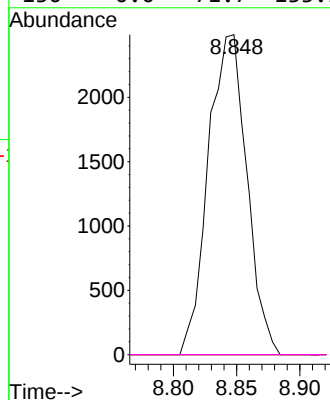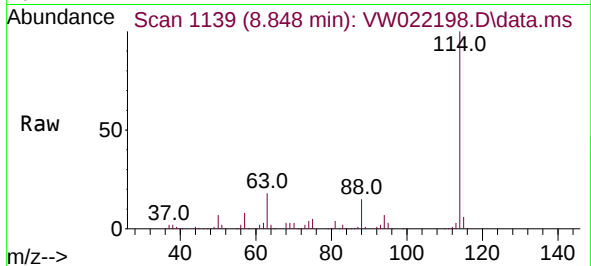

#39
 cis-1,3-Dichloropropene
 Concen: 0.663 ug/L
 RT: 10.037 min Scan# 1334
 Delta R.T. -0.037 min
 Lab File: VW022198.D
 Acq: 07 Mar 2022 14:04

Tgt Ion: 75 Resp: 1871
 Ion Ratio Lower Upper
 75 100
 77 48.5 20.6 38.2#

