

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022205.D
 Acq On : 07 Mar 2022 16:52
 Operator : SY/VA
 Sample : N1775-19
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSC2

Quant Time: Mar 08 00:25:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	121533	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	113726	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	56875	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	22816	14.393	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.560%
7) Chloroethane-d5	2.879	69	20443	16.391	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.560%
11) 1,1-Dichloroethene-d2	4.019	63	30298	12.481	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.920%
21) 2-Butanone-d5	7.080	46	22947	86.098	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	172.200%#
24) Chloroform-d	7.647	84	63061	23.256	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.040%
26) 1,2-Dichloroethane-d4	8.305	65	36676	26.021	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.080%
32) Benzene-d6	8.275	84	108812	20.558	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.240%
36) 1,2-Dichloropropane-d6	9.274	67	34641	23.567	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.280%
41) Toluene-d8	10.323	98	99963	18.997	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.000%
43) trans-1,3-Dichloroprop...	10.579	79	14127	21.676	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.720%
47) 2-Hexanone-d5	10.920	63	18473	76.413	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	152.820%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	42531	32.970	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	131.880%#
66) 1,2-Dichlorobenzene-d4	13.853	152	47491	25.997	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.000%
Target Compounds					Qvalue	
13) Acetone	4.129	43	2766	12.707	ug/L	60
61) 1,2,3-Trichloropropane	13.554	75	6695	7.458	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022205.D
Acq On : 07 Mar 2022 16:52
Operator : SY/VA
Sample : N1775-19
Misc : 6.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSC2

Quant Time: Mar 08 00:25:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration




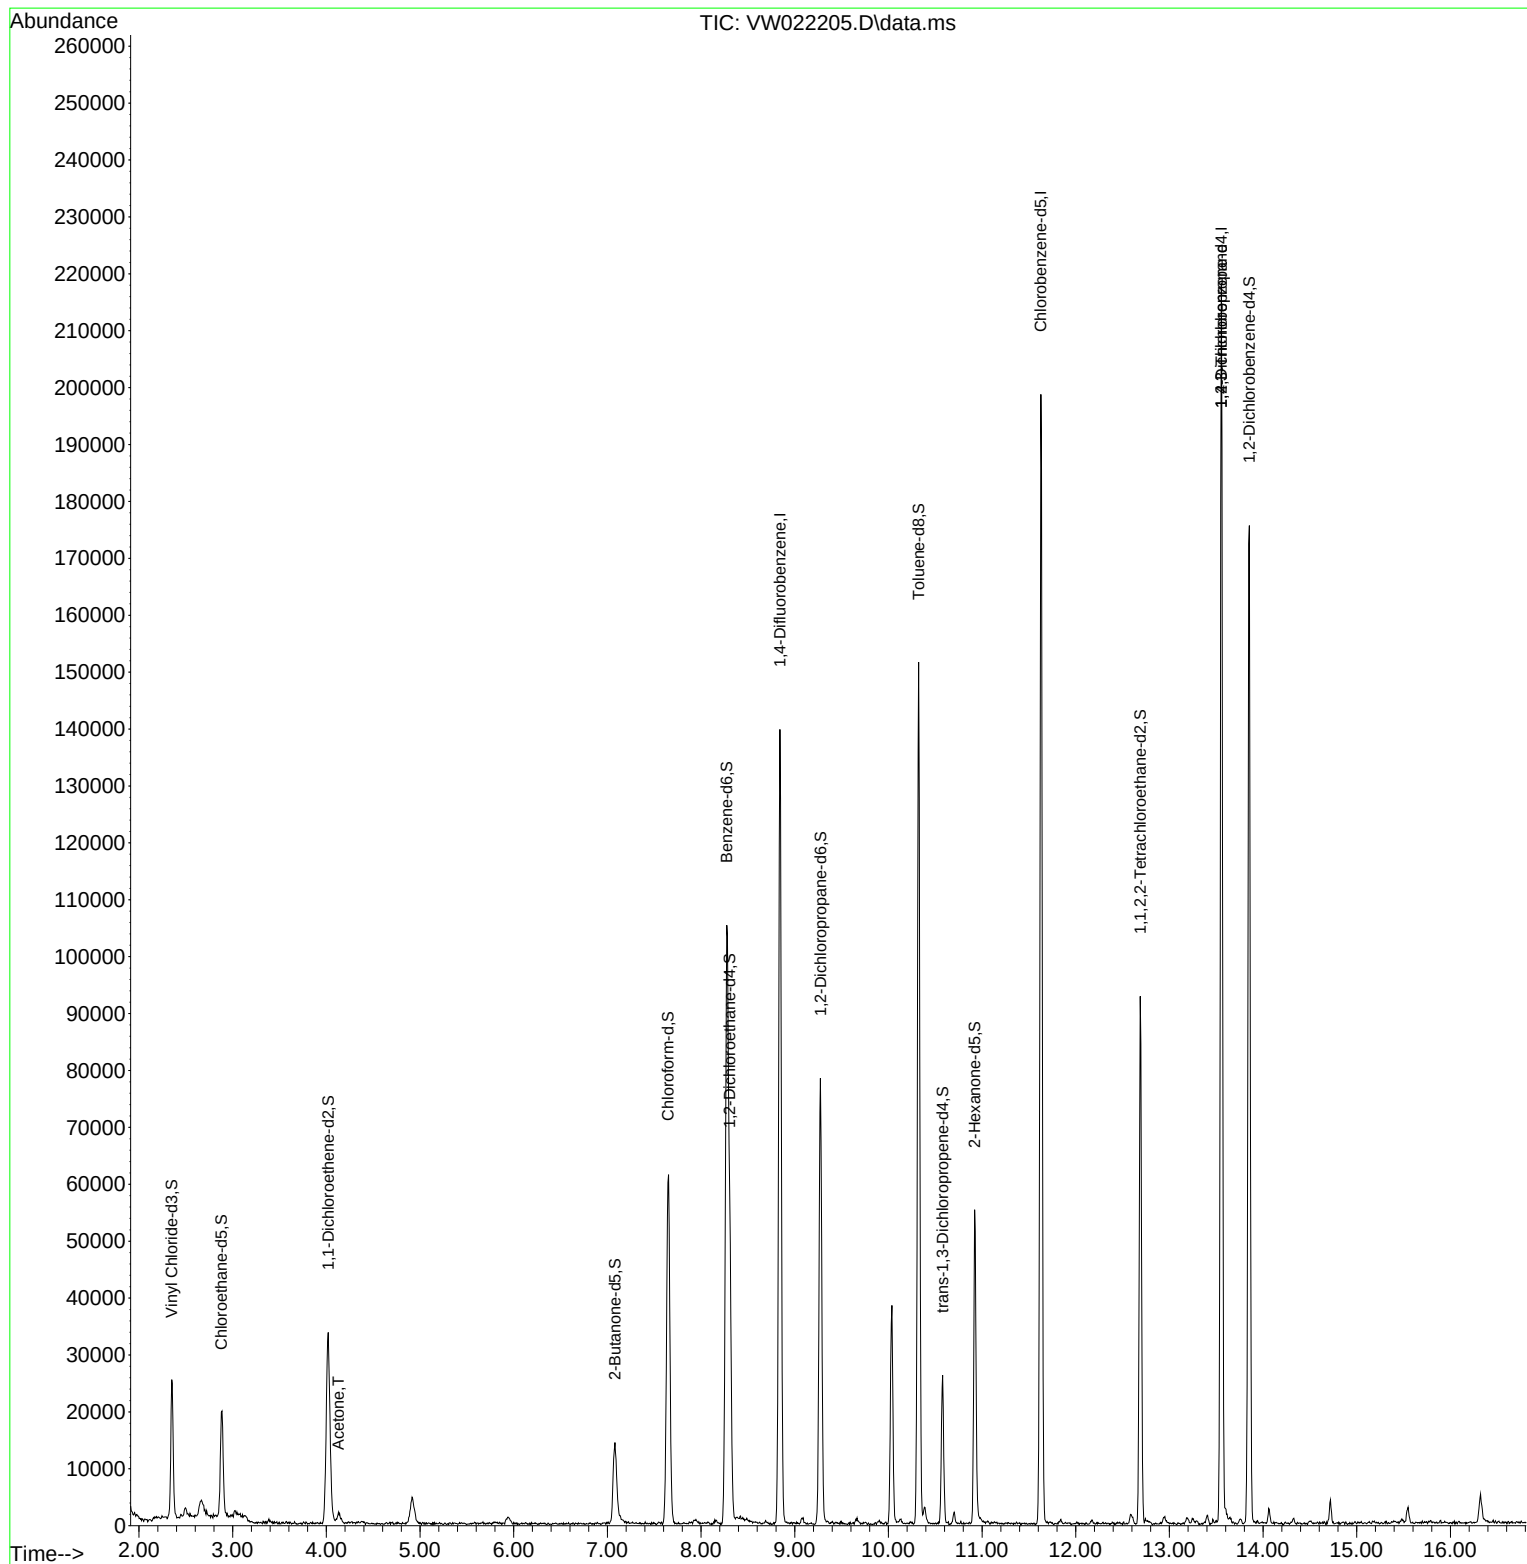


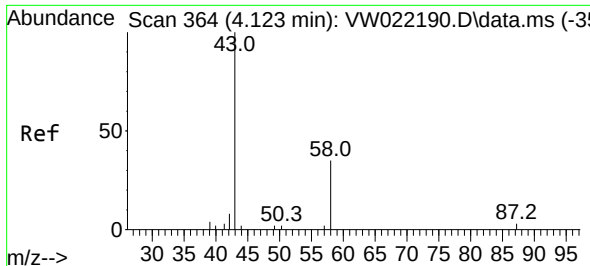

#13
Acetone
Concen: 12.707 ug/L
RT: 4.129 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW022205.D
Acq: 07 Mar 2022 16:52

Instrument :
MSVOA_W
ClientSampleId :
DBSC2

Tgt Ion: 43 Resp: 2766
Ion Ratio Lower Upper
43 100
58 11.5 0.0 69.2

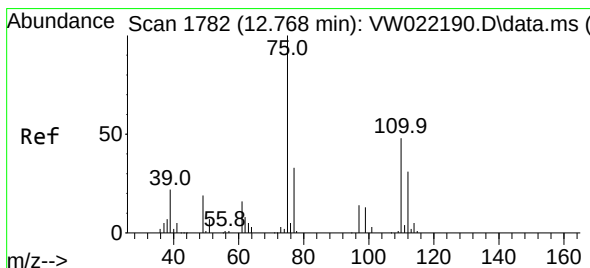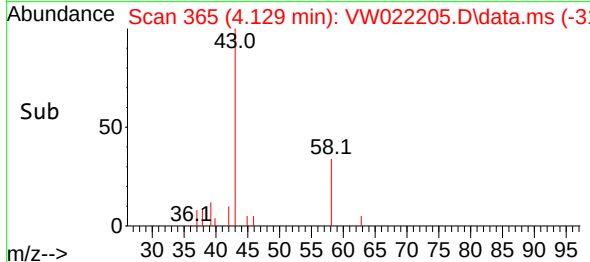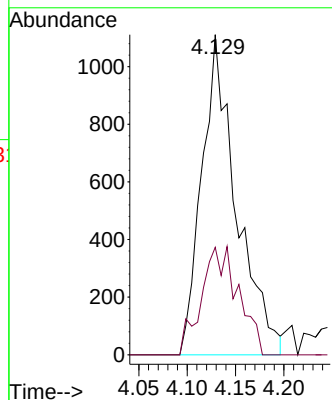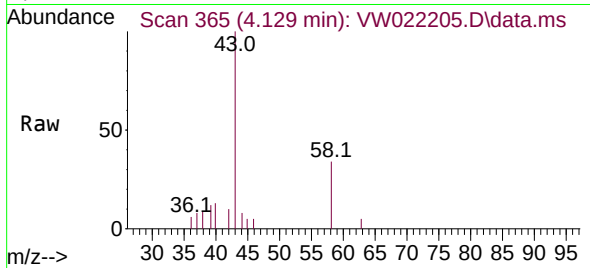

#61
1,2,3-Trichloropropane
Concen: 7.458 ug/L
RT: 13.554 min Scan# 1911
Delta R.T. 0.786 min
Lab File: VW022205.D
Acq: 07 Mar 2022 16:52

Tgt Ion: 75 Resp: 6695
Ion Ratio Lower Upper
75 100
77 34.7 27.1 40.7
110 5.8 36.7 55.1#

