

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022206.D
 Acq On : 07 Mar 2022 17:16
 Operator : SY/VA
 Sample : N1775-23
 Misc : 4.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSC6

Quant Time: Mar 08 00:25:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	141217	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	130488	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	65457	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	25919	14.072	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.280%
7) Chloroethane-d5	2.885	69	22778	15.717	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.880%
11) 1,1-Dichloroethene-d2	4.013	63	37381	13.253	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.000%
21) 2-Butanone-d5	7.074	46	24559	79.302	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	158.600%#
24) Chloroform-d	7.653	84	74471	23.636	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.560%
26) 1,2-Dichloroethane-d4	8.305	65	41312	25.224	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.880%
32) Benzene-d6	8.275	84	133270	21.945	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.760%
36) 1,2-Dichloropropane-d6	9.275	67	41916	24.854	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.400%
41) Toluene-d8	10.323	98	122162	20.234	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.920%
43) trans-1,3-Dichloroprop...	10.579	79	15759	21.074	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.280%
47) 2-Hexanone-d5	10.921	63	20113	72.510	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	145.020%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	45639	30.835	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	123.320%#
66) 1,2-Dichlorobenzene-d4	13.853	152	53391	25.395	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.600%
Target Compounds						
					Qvalue	
14) Carbon disulfide	4.385	76	8760	2.316	ug/L	99
37) 1,2-Dichloropropane	9.268	63	5011	3.405	ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022206.D
Acq On : 07 Mar 2022 17:16
Operator : SY/VA
Sample : N1775-23
Misc : 4.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSC6

Quant Time: Mar 08 00:25:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration




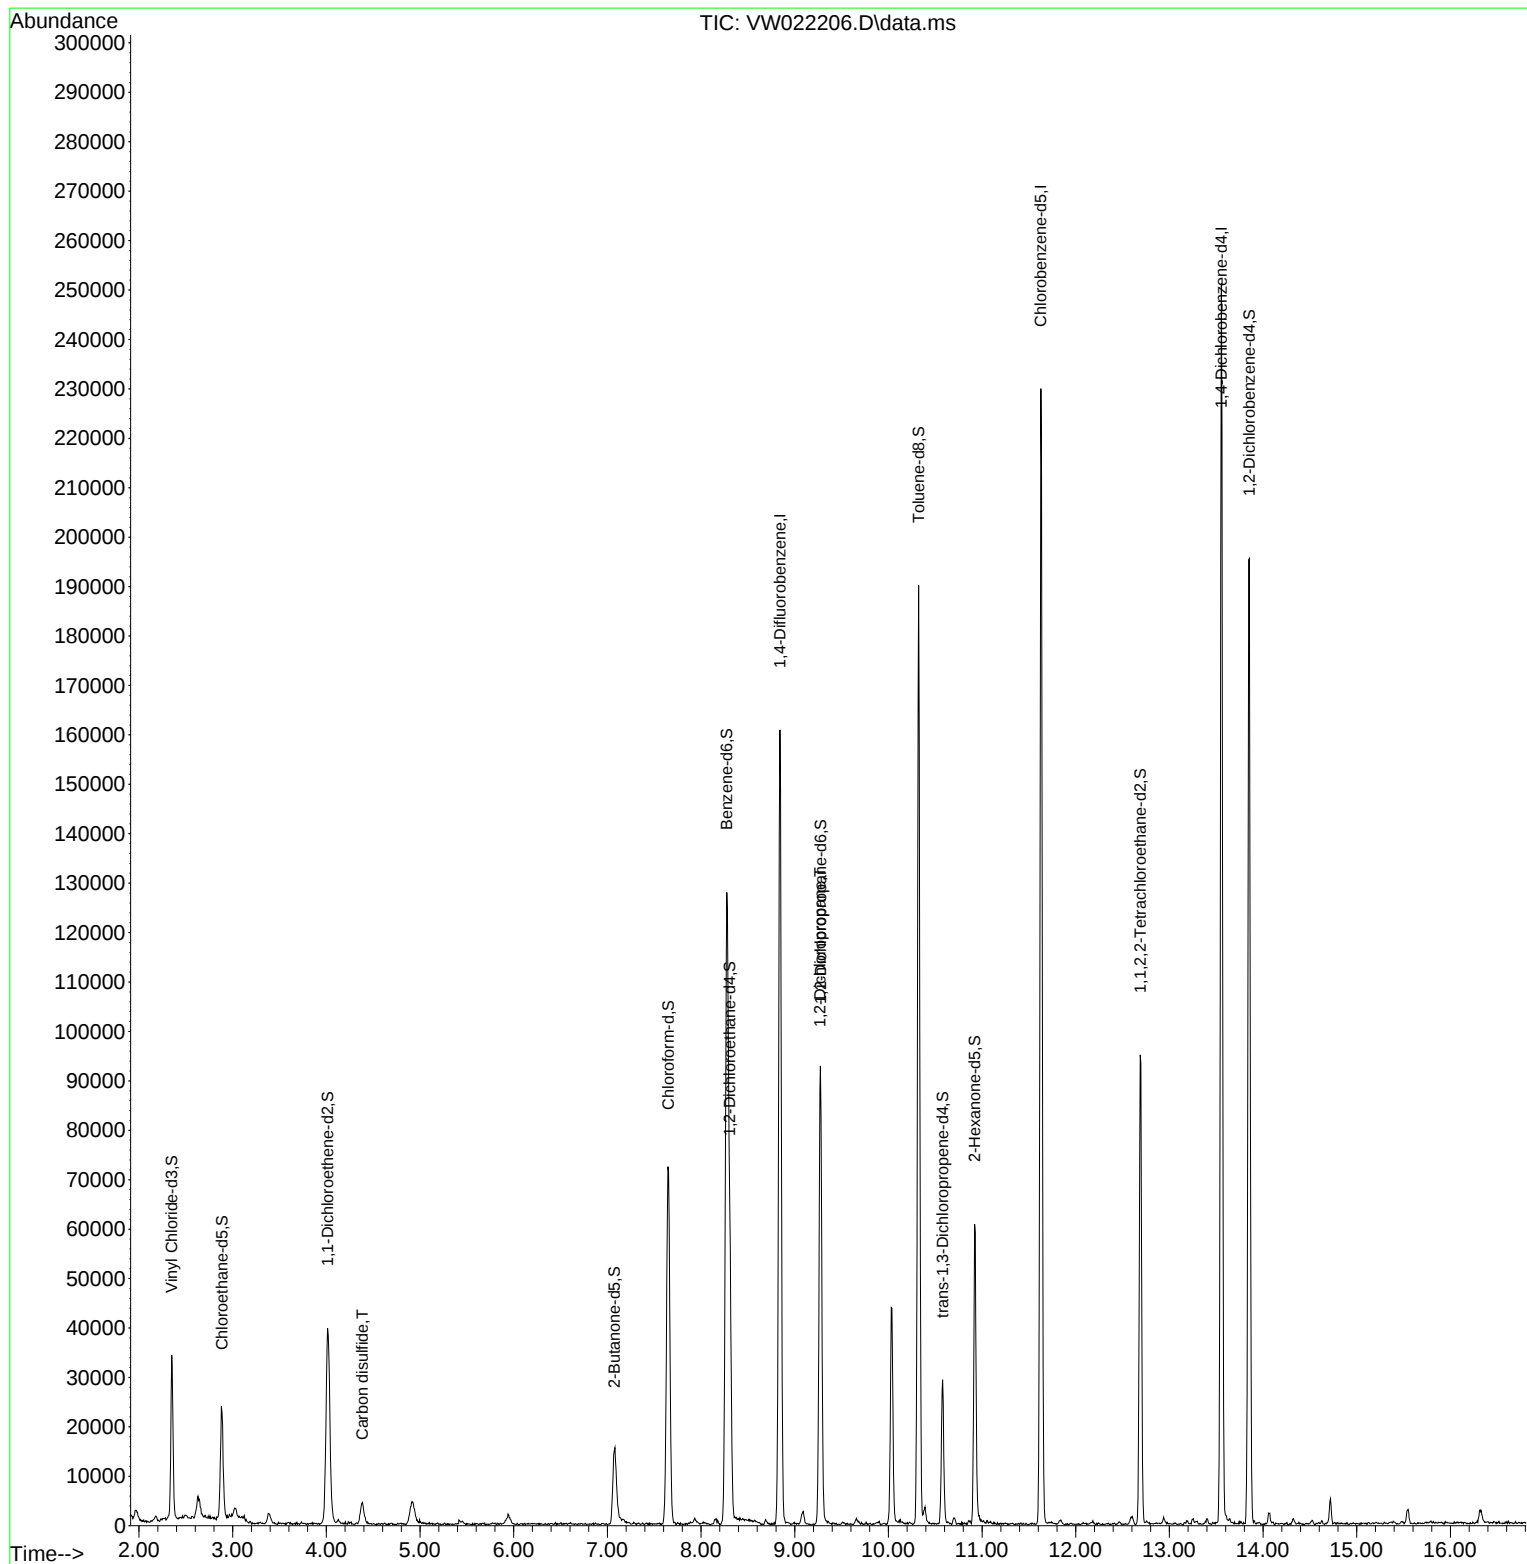


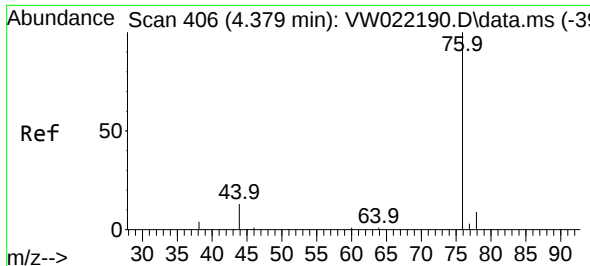

#14
Carbon disulfide
Concen: 2.316 ug/L
RT: 4.385 min Scan# 406
Delta R.T. 0.006 min
Lab File: VW022206.D
Acq: 07 Mar 2022 17:16

Instrument :
MSVOA_W
ClientSampleId :
DBSC6

Tgt Ion: 76 Resp: 8760
Ion Ratio Lower Upper
76 100
78 10.2 7.8 11.8

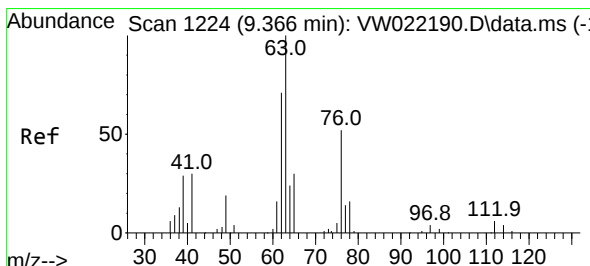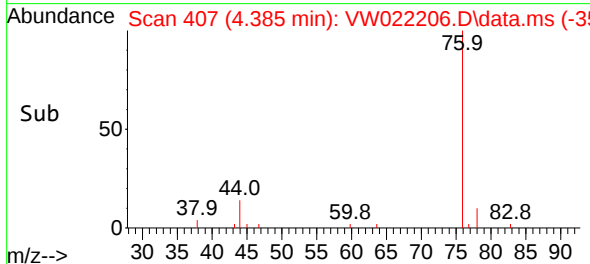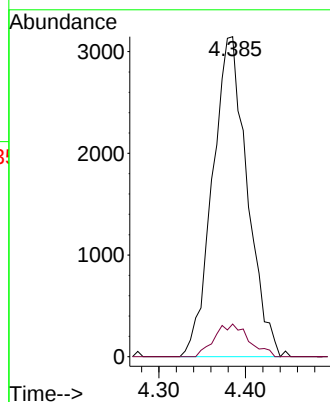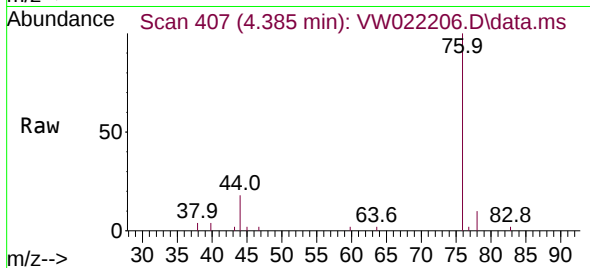

#37
1,2-Dichloropropane
Concen: 3.405 ug/L
RT: 9.268 min Scan# 1208
Delta R.T. -0.098 min
Lab File: VW022206.D
Acq: 07 Mar 2022 17:16

Tgt Ion: 63 Resp: 5011
Ion Ratio Lower Upper
63 100
112 0.0 4.1 6.1#

