




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022198.D
 Acq On : 07 Mar 2022 14:04
 Operator : SY/VA
 Sample : N1775-16
 Misc : 5.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB9

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:24:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

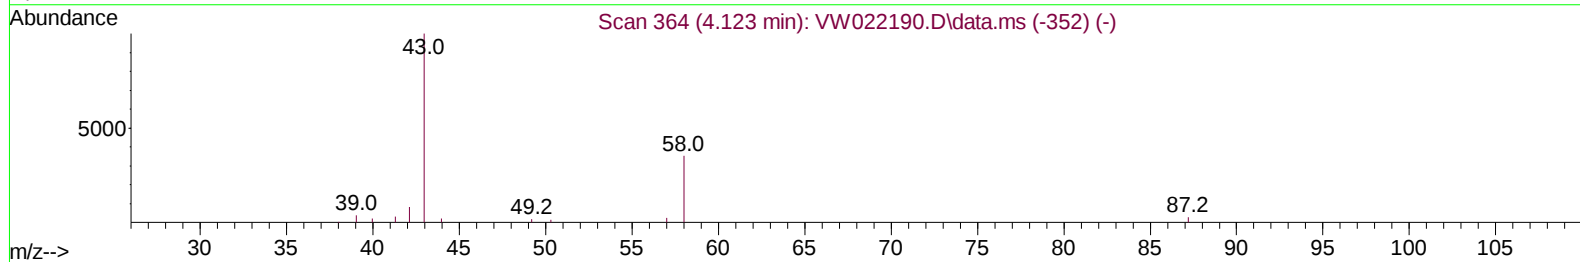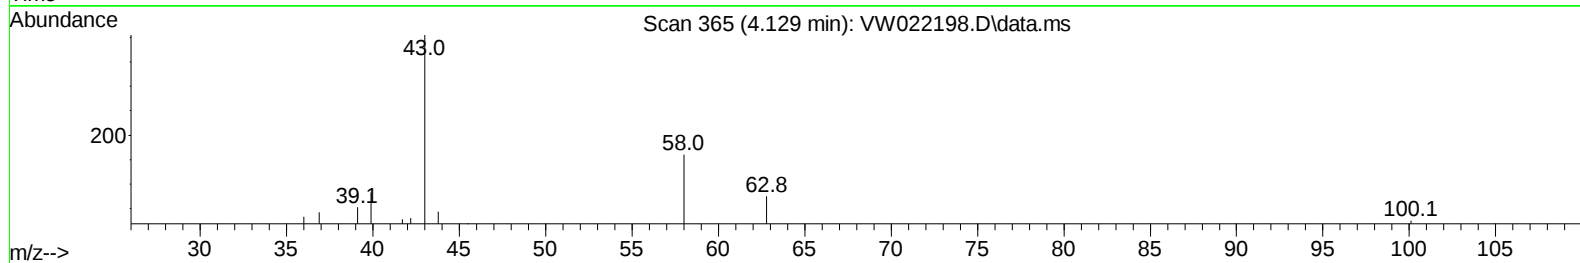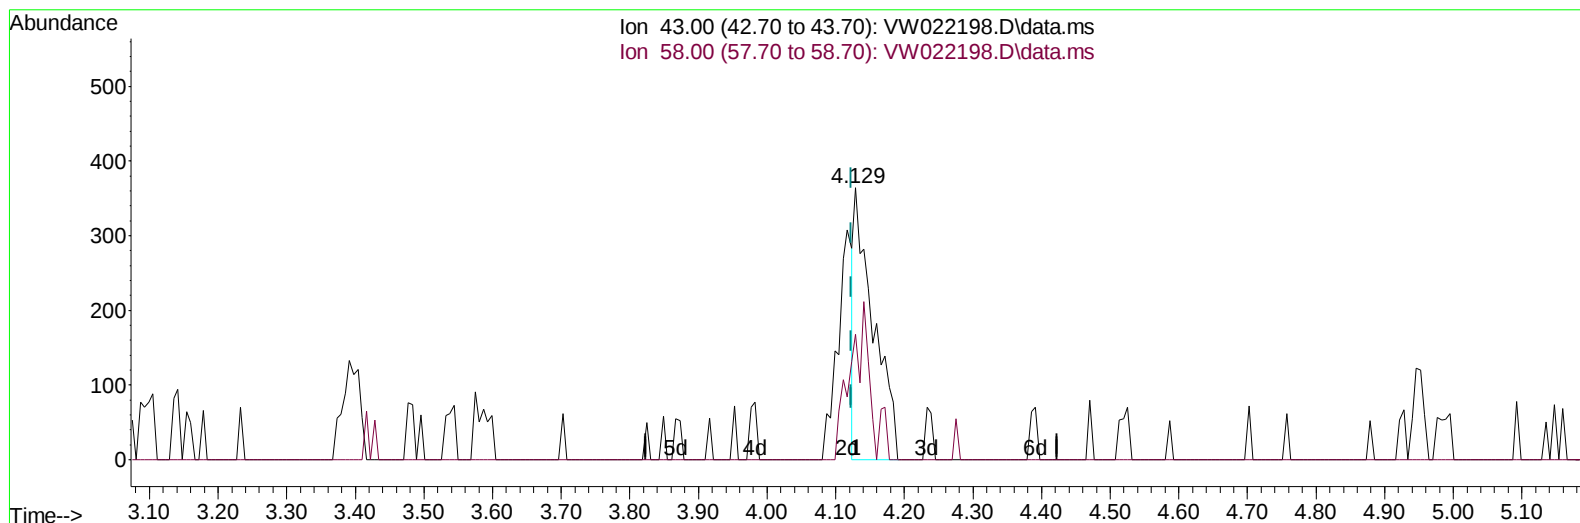

TIC: VW022198.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 2.31 ug/L

response 706

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	34.14
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022198.D
Acq On : 07 Mar 2022 14:04
Operator : SY/VA
Sample : N1775-16
Misc : 5.92g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSB9

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:24:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
Supervised By :Mahesh Dadoda 03/08/2022

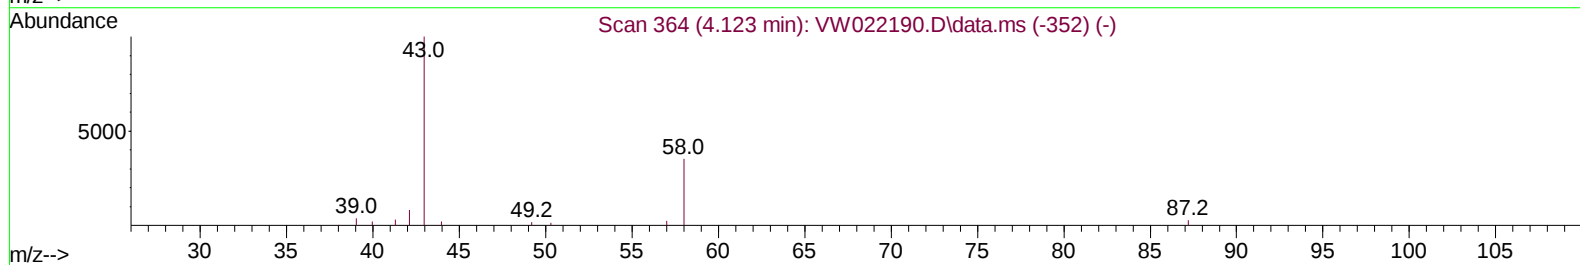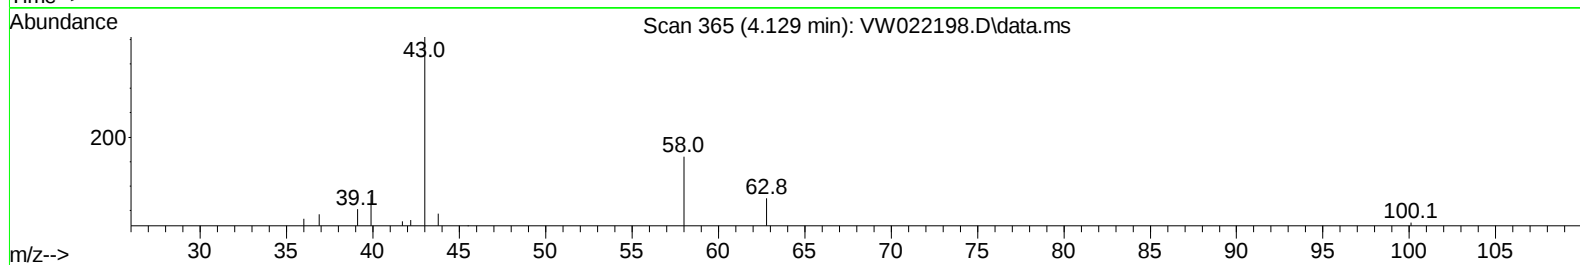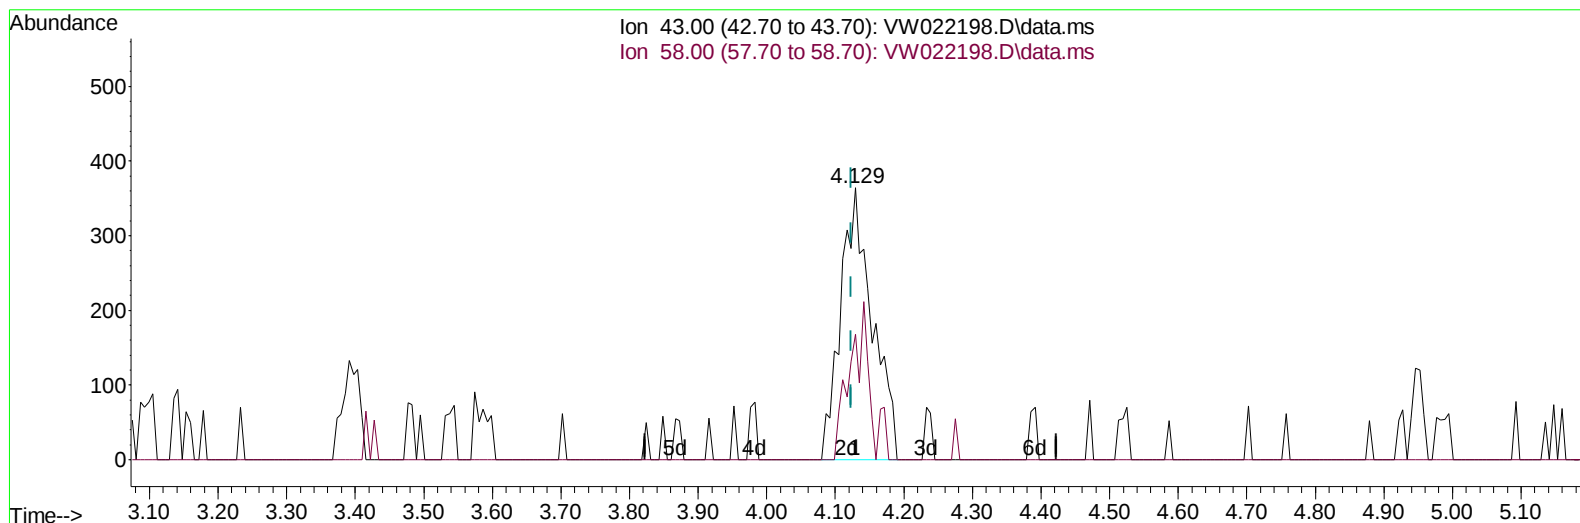

TIC: VW022198.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 3.82 ug/L m

response 1169

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	20.62
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022198.D
 Acq On : 07 Mar 2022 14:04
 Operator : SY/VA
 Sample : N1775-16
 Misc : 5.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSB9

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:24:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	170754	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	164536	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	86575	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	50015	22.457	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.840%		
7) Chloroethane-d5	2.885	69	35613	20.323	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.280%		
11) 1,1-Dichloroethene-d2	4.019	63	59039	17.310	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	69.240%		
21) 2-Butanone-d5	7.074	46	17589	46.971	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.940%		
24) Chloroform-d	7.653	84	86622	22.737	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.960%		
26) 1,2-Dichloroethane-d4	8.305	65	48141	24.309	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	97.240%		
32) Benzene-d6	8.275	84	178125	23.261	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	93.040%		
36) 1,2-Dichloropropane-d6	9.275	67	48859	22.976	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.920%		
41) Toluene-d8	10.323	98	172167	22.615	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	90.480%		
43) trans-1,3-Dichloroprop...	10.579	79	21011	22.284	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	89.120%		
47) 2-Hexanone-d5	10.927	63	13959	39.910	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.820%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	39928	21.394	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.560%		
66) 1,2-Dichlorobenzene-d4	13.853	152	62535	22.489	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.960%		
Target Compounds						
13) Acetone	4.129	43	1169m	3.822	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022198.D
Acq On : 07 Mar 2022 14:04
Operator : SY/VA
Sample : N1775-16
Misc : 5.92g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSB9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/08/2022
Supervised By :Mahesh Dadoda 03/08/2022

Quant Time: Mar 08 00:24:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

