




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022200.D
 Acq On : 07 Mar 2022 14:52
 Operator : SY/VA
 Sample : N1775-21
 Misc : 5.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSC4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

Quant Time: Mar 08 00:24:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

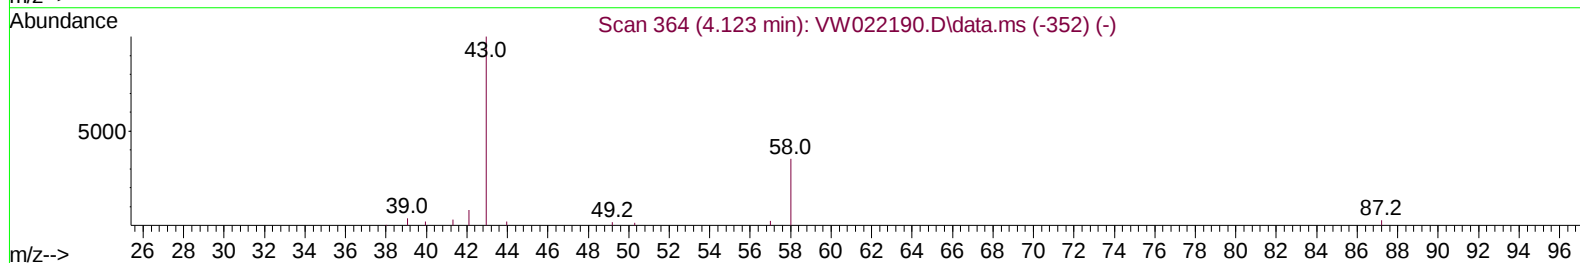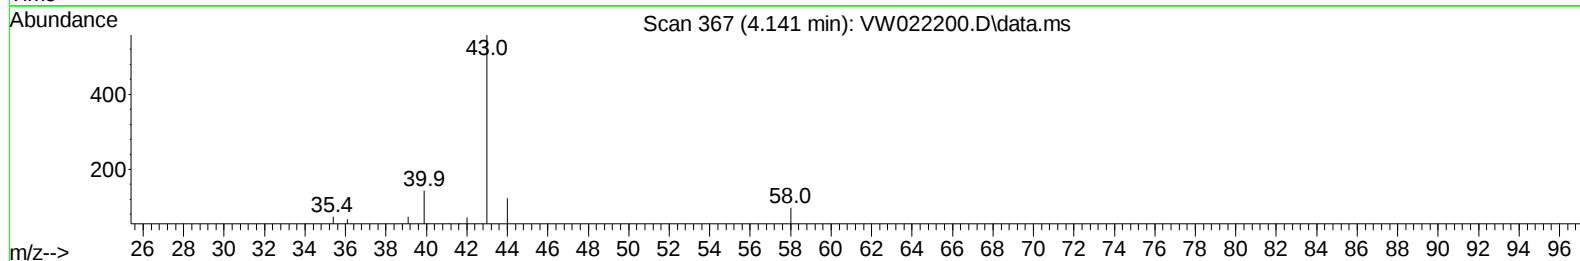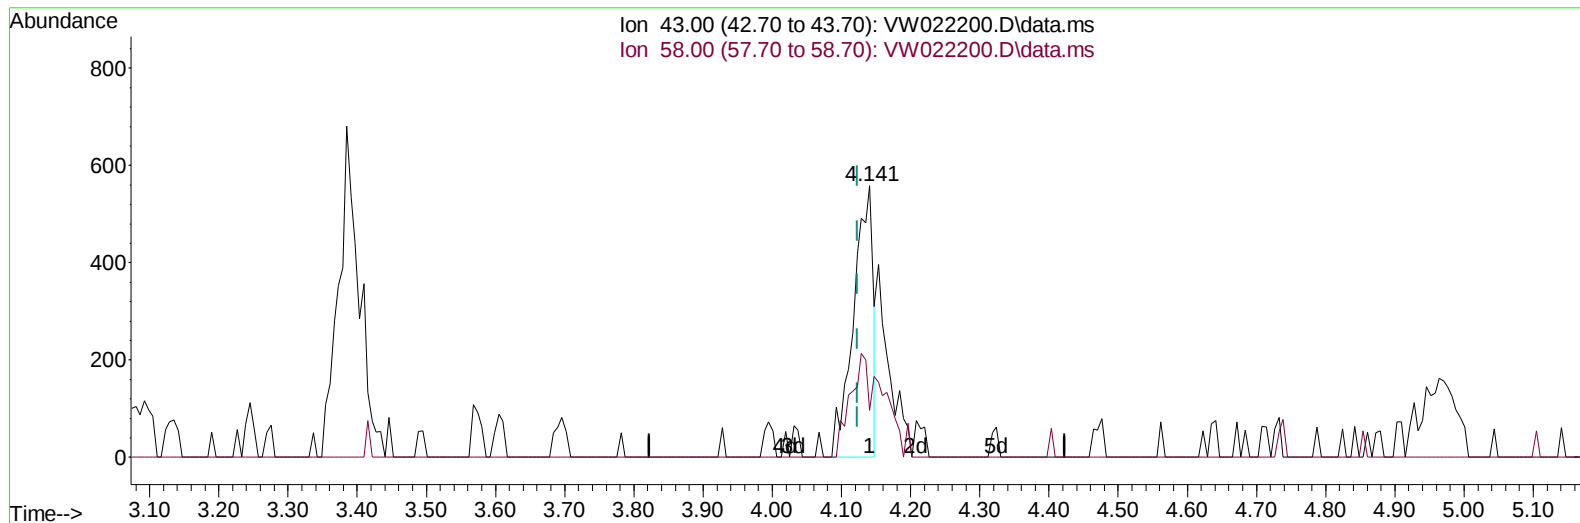

TIC: VW022200.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 3.67 ug/L

response 1100

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	27.45
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022200.D
 Acq On : 07 Mar 2022 14:52
 Operator : SY/VA
 Sample : N1775-21
 Misc : 5.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSC4

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:24:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

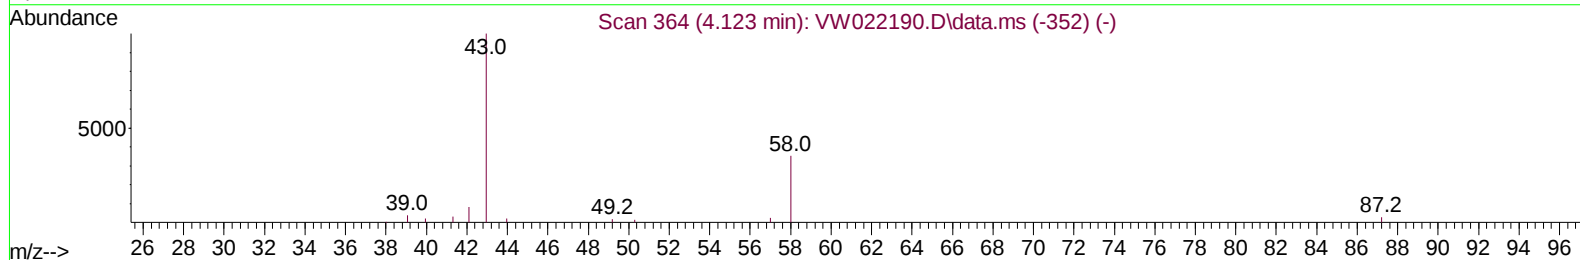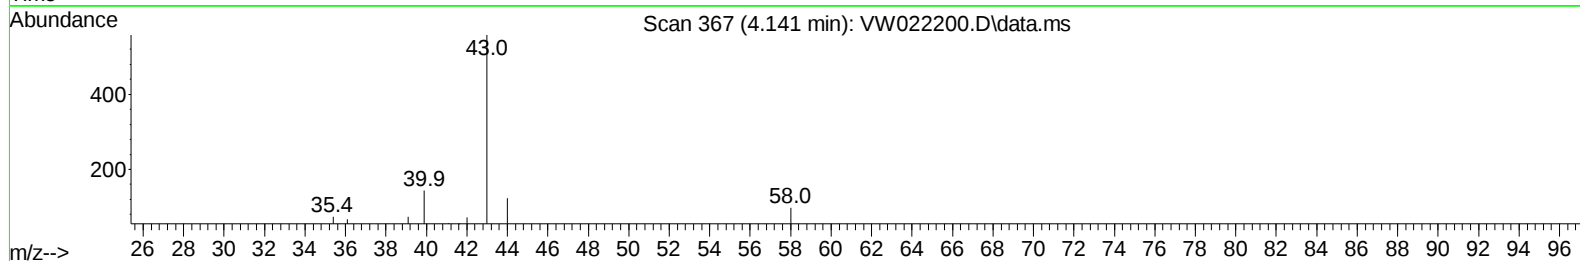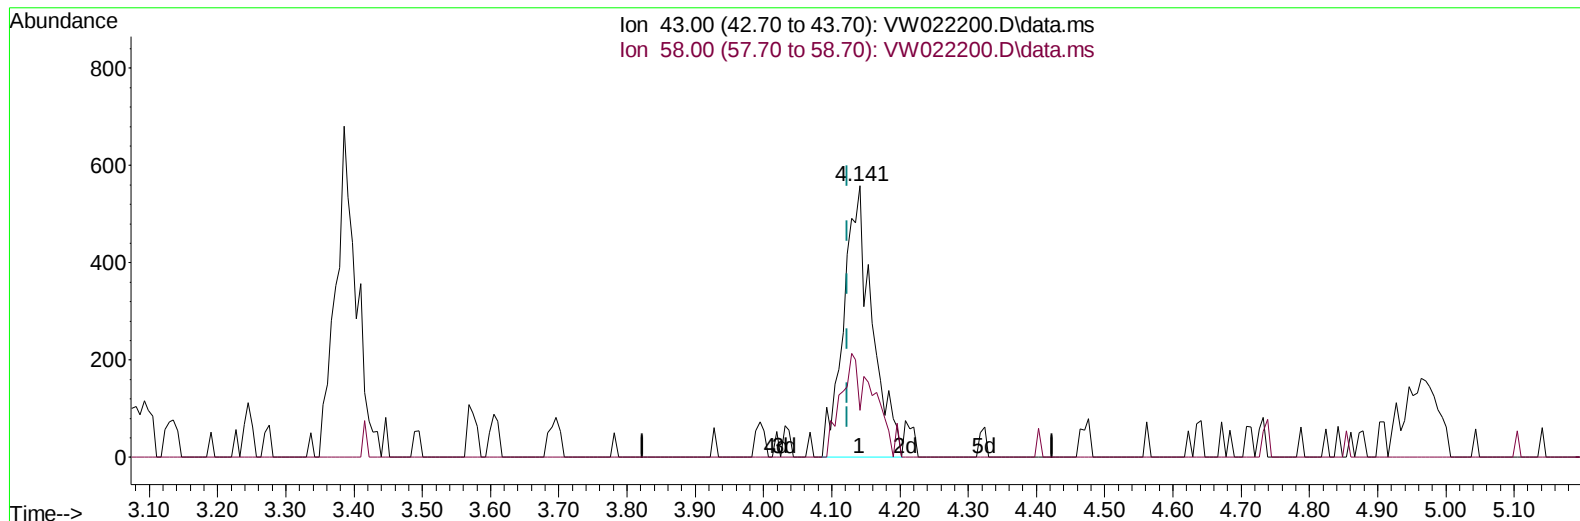

TIC: VW022200.D\data.ms

(13) Acetone (T)

4.141min (+ 0.018) 5.39 ug/L m

response 1616

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	18.69
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022200.D
 Acq On : 07 Mar 2022 14:52
 Operator : SY/VA
 Sample : N1775-21
 Misc : 5.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSC4

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:24:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	167417	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	156418	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	78231	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	29923	13.703	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	54.800%	
7) Chloroethane-d5	2.885	69	28319	16.483	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	65.920%	
11) 1,1-Dichloroethene-d2	4.013	63	42726	12.777	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110	Recovery	=	51.120%	
21) 2-Butanone-d5	7.086	46	16519	44.993	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	89.980%	
24) Chloroform-d	7.647	84	85169	22.801	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.200%	
26) 1,2-Dichloroethane-d4	8.311	65	41196	21.217	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	84.880%	
32) Benzene-d6	8.274	84	150384	20.658	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	82.640%	
36) 1,2-Dichloropropane-d6	9.274	67	45967	22.737	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	90.960%	
41) Toluene-d8	10.323	98	140604	19.428	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	77.720%	
43) trans-1,3-Dichloroprop...	10.579	79	16019	17.871	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.480%	
47) 2-Hexanone-d5	10.926	63	13996	42.093	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	84.180%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	37859	21.338	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	85.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	57398	22.843	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	91.360%	
Target Compounds						
13) Acetone	4.141	43	1616m	5.389	ug/L	
14) Carbon disulfide	4.391	76	8665	1.933	ug/L #	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022200.D
Acq On : 07 Mar 2022 14:52
Operator : SY/VA
Sample : N1775-21
Misc : 5.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSC4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/08/2022
Supervised By :Mahesh Dadoda 03/08/2022

Quant Time: Mar 08 00:24:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

