




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022204.D
Acq On : 07 Mar 2022 16:28
Operator : SY/VA
Sample : N1775-20
Misc : 6.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSC3

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:25:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
Supervised By :Mahesh Dadoda 03/08/2022

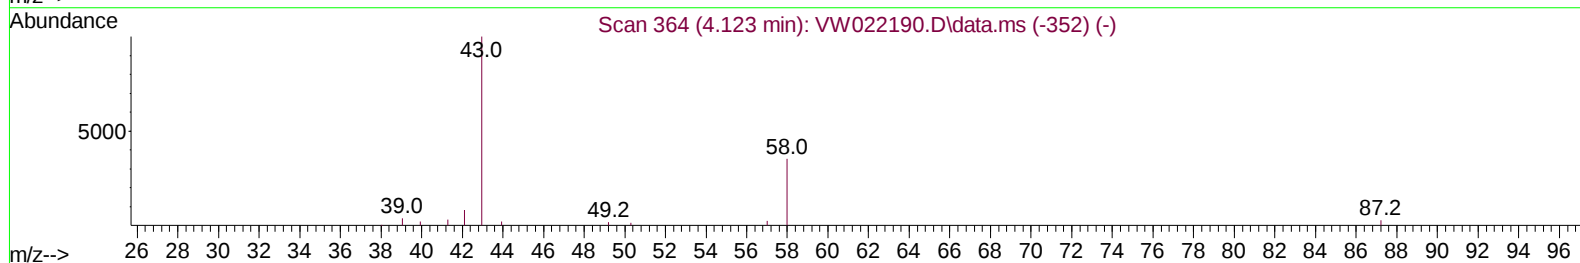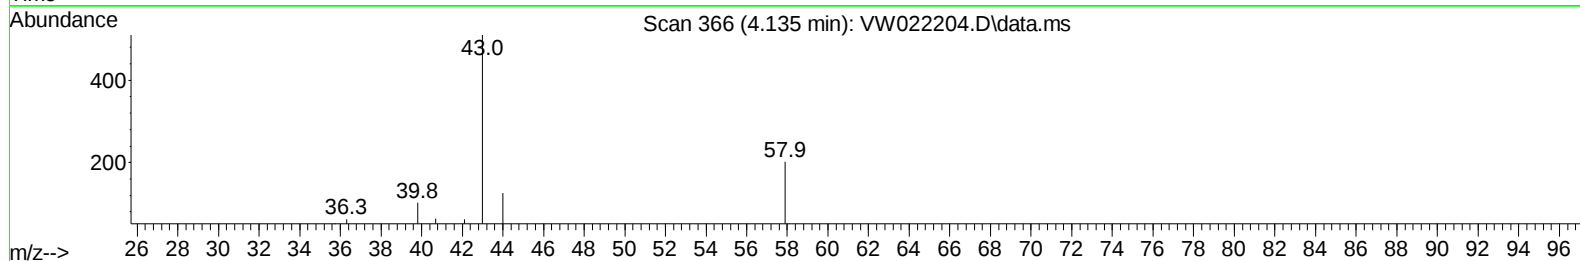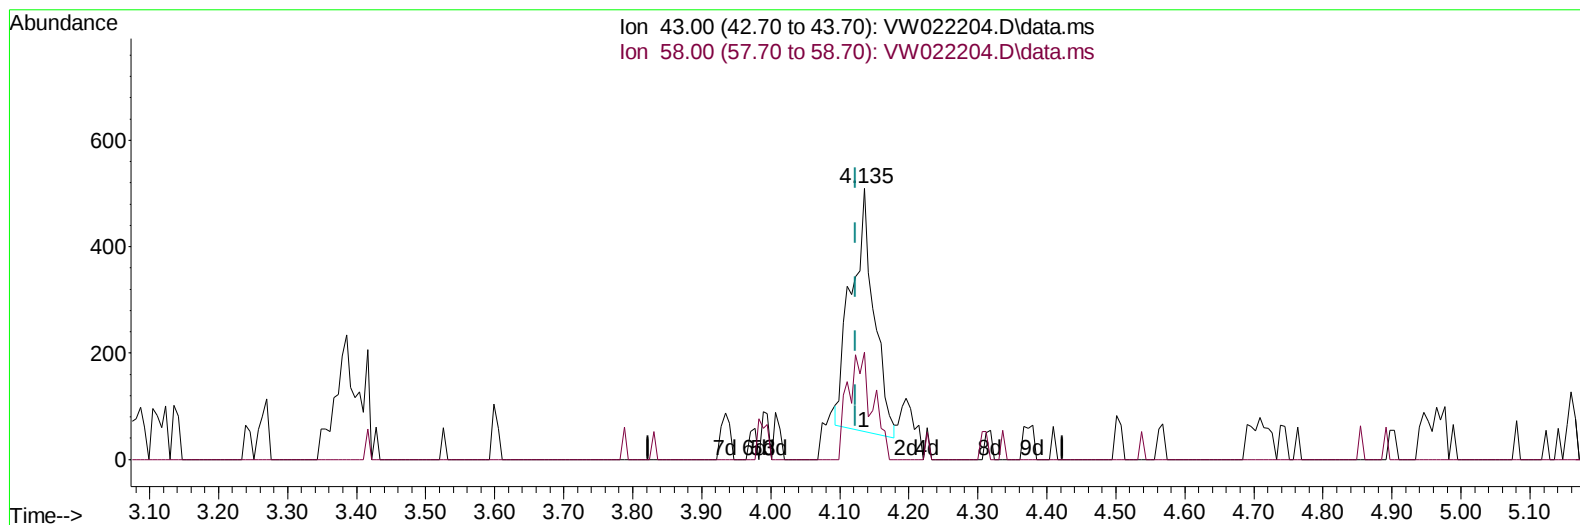

TIC: VW022204.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 4.37 ug/L

response 1040

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	22.50
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022204.D
 Acq On : 07 Mar 2022 16:28
 Operator : SY/VA
 Sample : N1775-20
 Misc : 6.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSC3

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:25:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

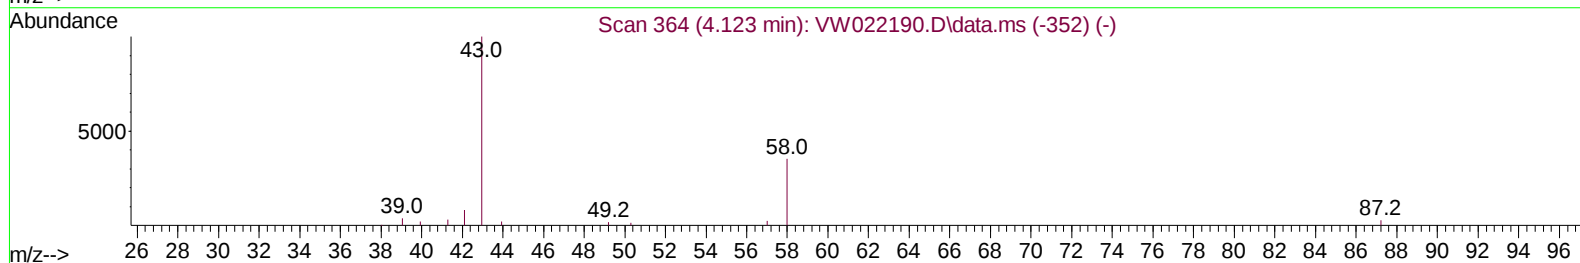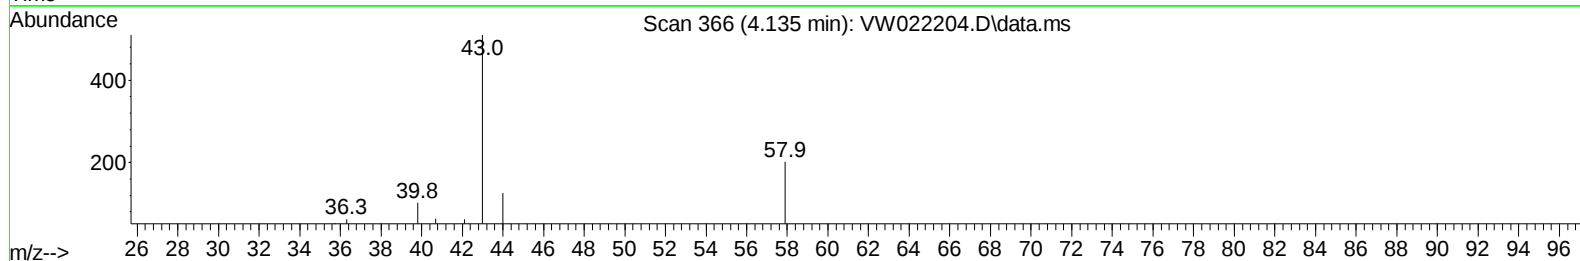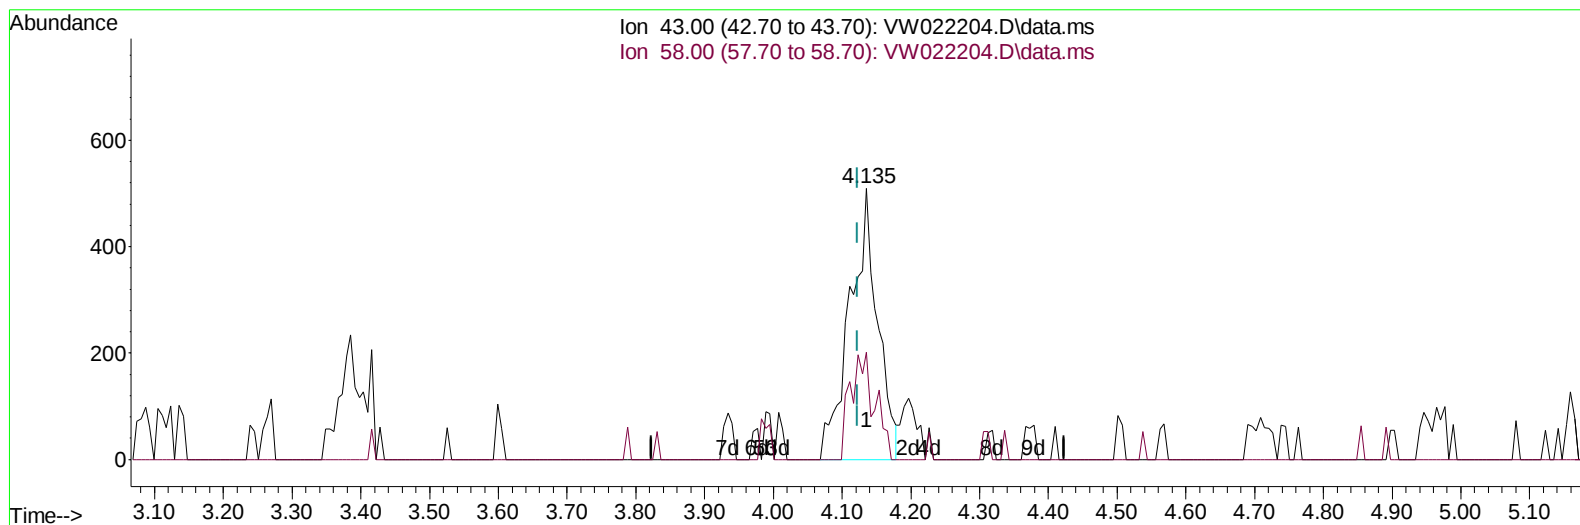

TIC: VW022204.D\data.ms

(13) Acetone (T)

4.135min (+ 0.012) 5.99 ug/L m

response 1424

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	16.43
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022204.D
 Acq On : 07 Mar 2022 16:28
 Operator : SY/VA
 Sample : N1775-20
 Misc : 6.52g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSC3

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:25:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	132742	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	129370	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	67673	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	21916	12.658	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	50.640%	
7) Chloroethane-d5	2.885	69	19887	14.599	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	58.400%	
11) 1,1-Dichloroethene-d2	4.019	63	31359	11.827	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	47.320%	
21) 2-Butanone-d5	7.074	46	22973	78.917	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	157.840%#	
24) Chloroform-d	7.647	84	65528	22.125	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.520%	
26) 1,2-Dichloroethane-d4	8.311	65	37616	24.434	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.720%	
32) Benzene-d6	8.275	84	112368	18.663	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	74.640%	
36) 1,2-Dichloropropane-d6	9.275	67	36505	21.832	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	87.320%	
41) Toluene-d8	10.323	98	104052	17.383	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	69.520%	
43) trans-1,3-Dichloroprop...	10.579	79	14284	19.267	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.080%	
47) 2-Hexanone-d5	10.921	63	18769	68.249	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	136.500%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	42591	29.024	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	116.080%	
66) 1,2-Dichlorobenzene-d4	13.853	152	49972	22.990	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	91.960%	
Target Compounds						
13) Acetone	4.135	43	1424m	5.989	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022204.D
Acq On : 07 Mar 2022 16:28
Operator : SY/VA
Sample : N1775-20
Misc : 6.52g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSC3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/08/2022
Supervised By :Mahesh Dadoda 03/08/2022

Quant Time: Mar 08 00:25:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

