




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022209.D
 Acq On : 07 Mar 2022 18:28
 Operator : SY/VA
 Sample : N1816-04
 Misc : 5.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD1

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:26:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

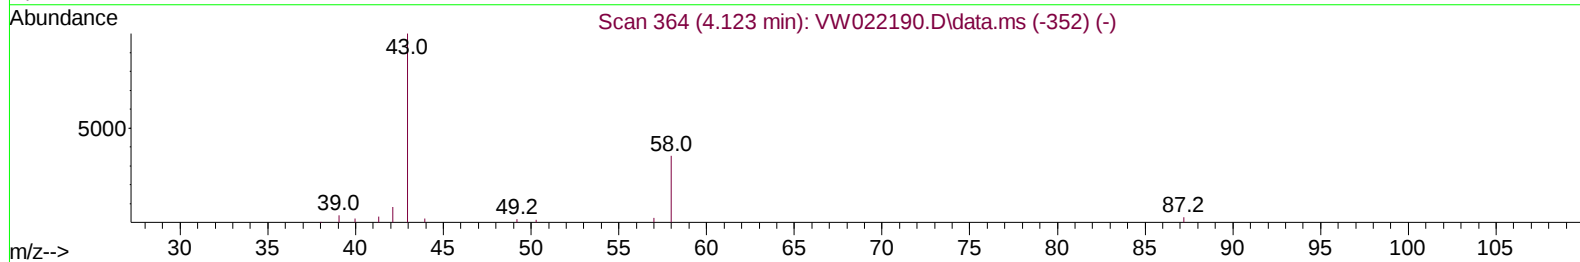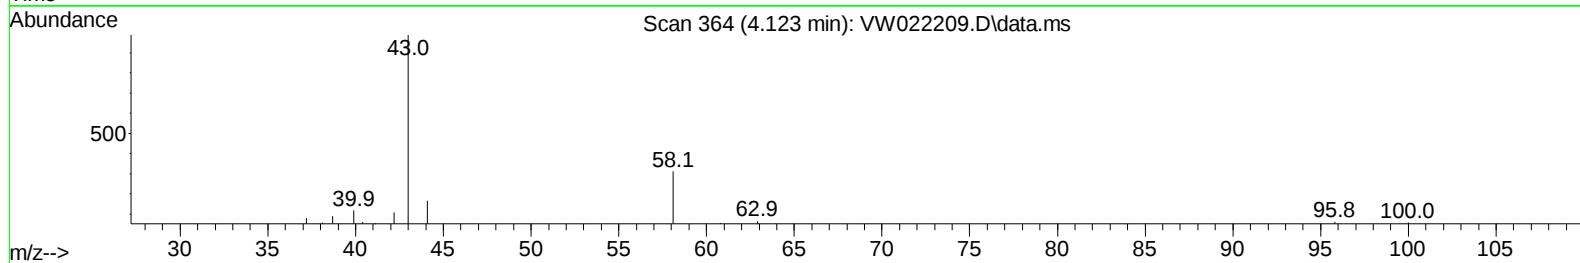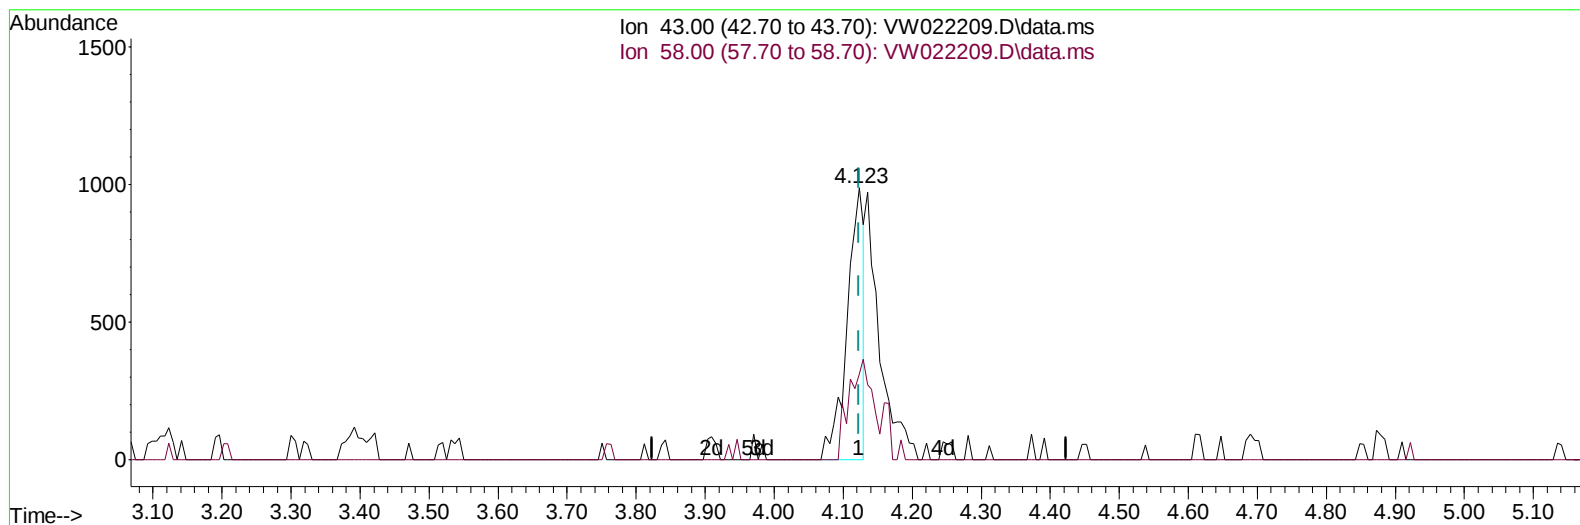

TIC: VW022209.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 5.65 ug/L

response 1663

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	32.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022209.D
 Acq On : 07 Mar 2022 18:28
 Operator : SY/VA
 Sample : N1816-04
 Misc : 5.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD1

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:26:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

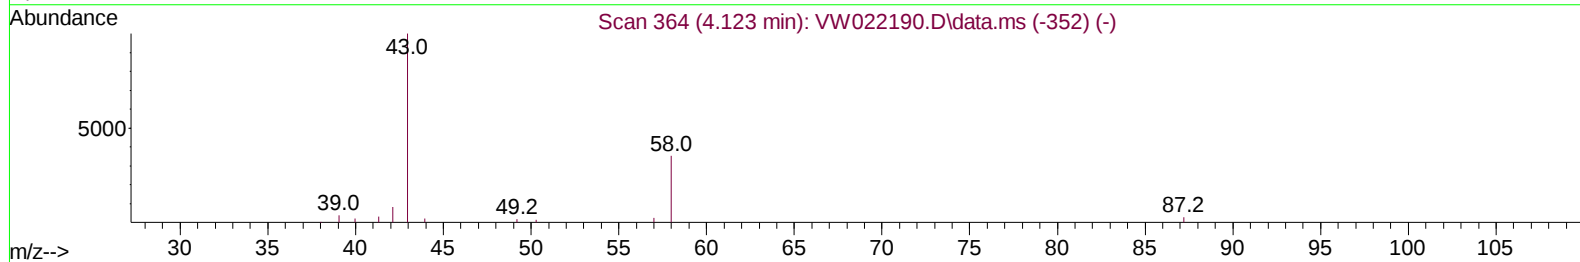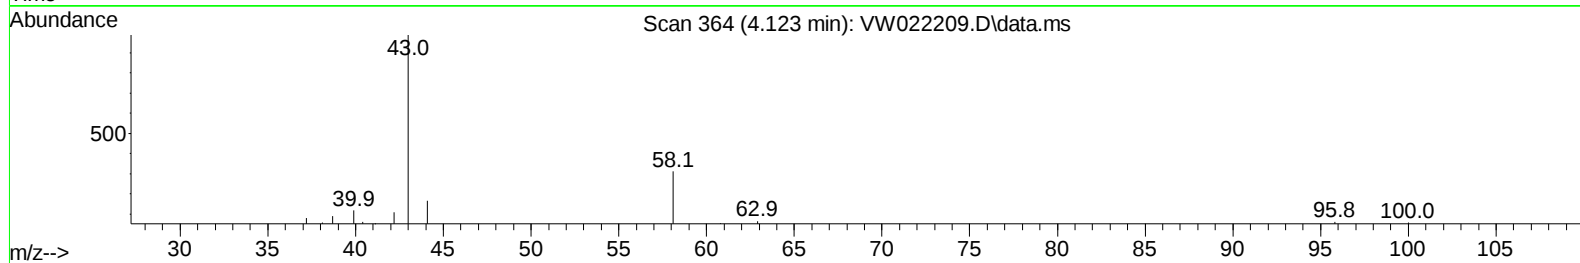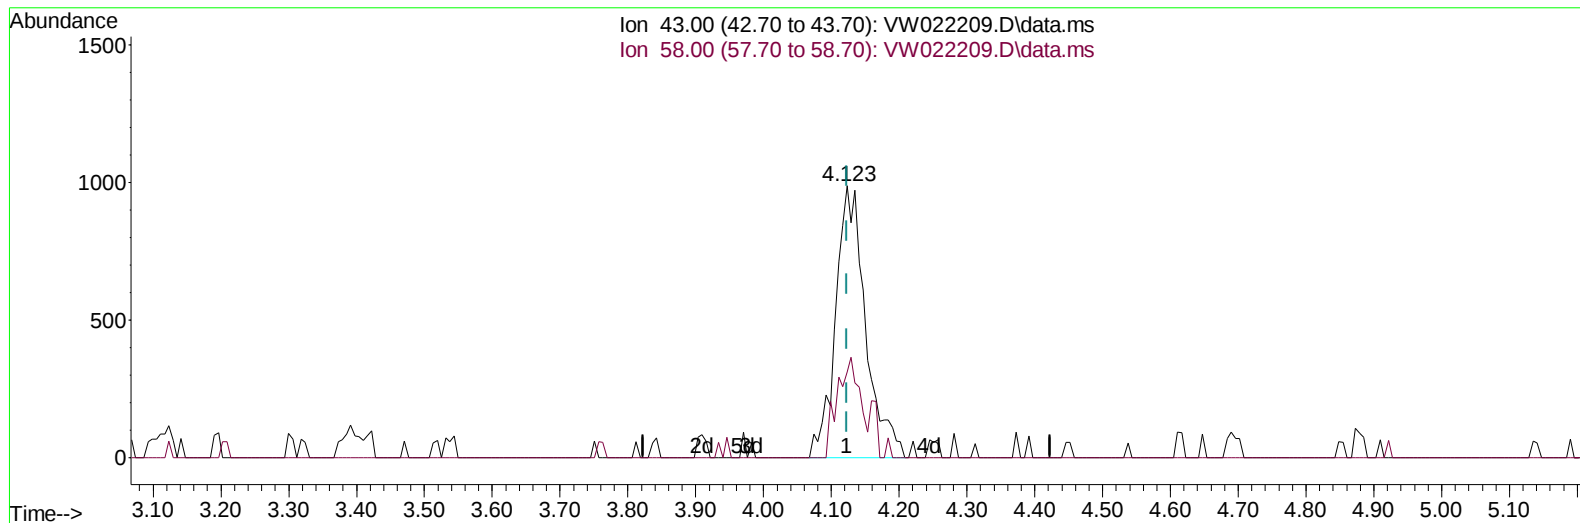

TIC: VW022209.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 10.33 ug/L m

response 3041

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	17.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022209.D
 Acq On : 07 Mar 2022 18:28
 Operator : SY/VA
 Sample : N1816-04
 Misc : 5.12g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD1

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:26:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	164375	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	161267	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81784	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	28988	13.521	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	54.080%	
7) Chloroethane-d5	2.885	69	27372	16.226	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	64.920%	
11) 1,1-Dichloroethene-d2	4.019	63	41113	12.522	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	50.080%	
21) 2-Butanone-d5	7.080	46	22479	62.359	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	124.720%	
24) Chloroform-d	7.653	84	83696	22.821	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.280%	
26) 1,2-Dichloroethane-d4	8.305	65	43922	23.040	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	92.160%	
32) Benzene-d6	8.275	84	148105	19.733	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	78.920%	
36) 1,2-Dichloropropane-d6	9.274	67	45769	21.959	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	87.840%	
41) Toluene-d8	10.323	98	139270	18.665	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	74.640%	
43) trans-1,3-Dichloroprop...	10.579	79	17009	18.405	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	73.600%	
47) 2-Hexanone-d5	10.927	63	19003	55.433	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	110.860%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	45209	24.715	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	98.840%	
66) 1,2-Dichlorobenzene-d4	13.853	152	58911	22.427	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.720%	
Target Compounds						
13) Acetone	4.123	43	3041m	10.329	ug/L	
14) Carbon disulfide	4.385	76	96251	21.864	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022209.D
Acq On : 07 Mar 2022 18:28
Operator : SY/VA
Sample : N1816-04
Misc : 5.12g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSD1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/08/2022
Supervised By :Mahesh Dadoda 03/08/2022

Quant Time: Mar 08 00:26:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

