




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022210.D
 Acq On : 07 Mar 2022 18:52
 Operator : SY/VA
 Sample : N1816-05
 Misc : 6.66g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD2

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:26:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

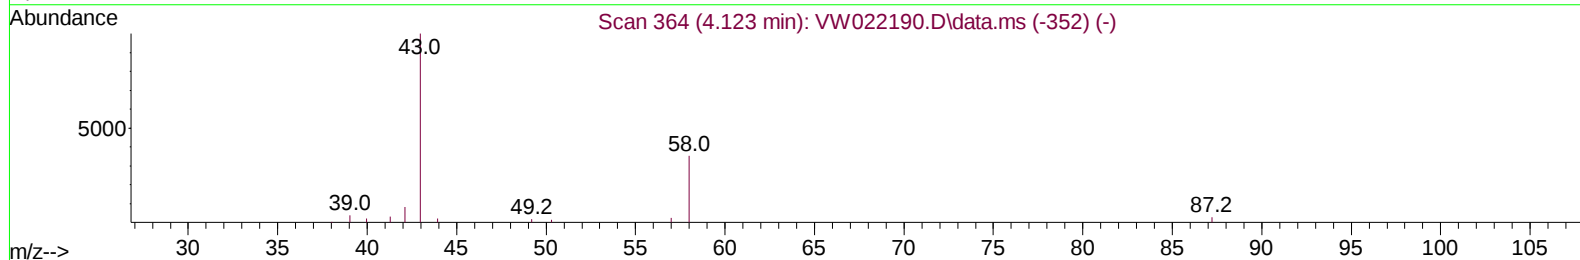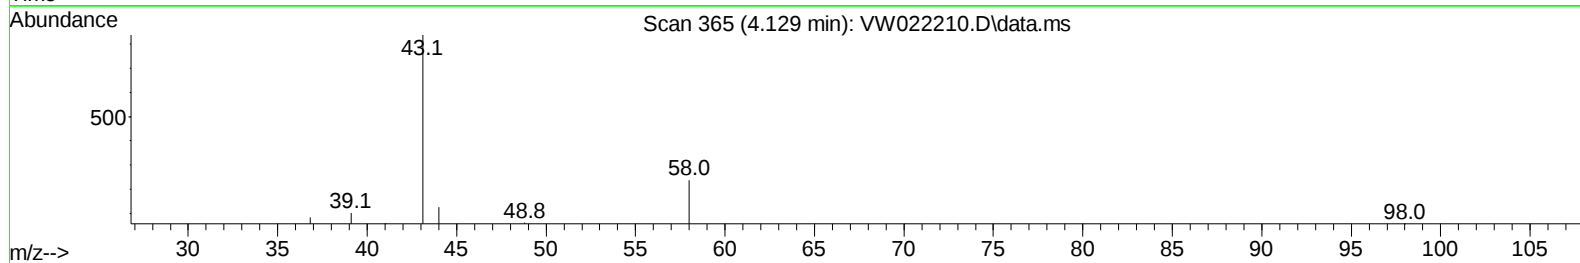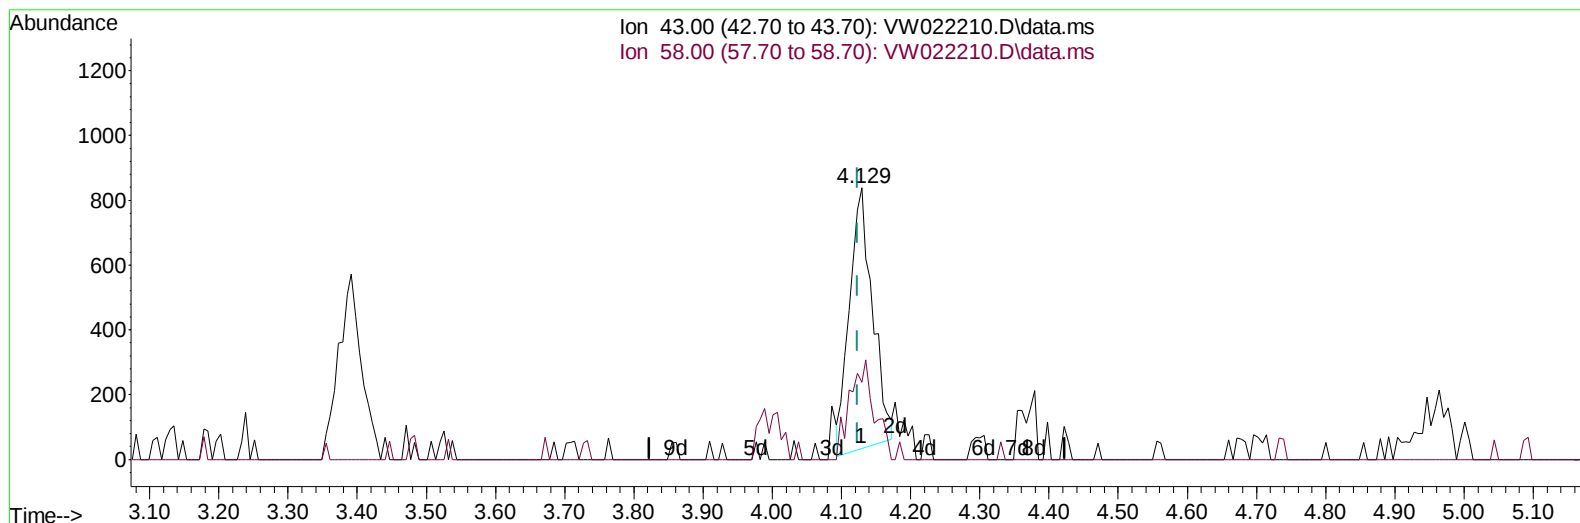

TIC: VW022210.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 6.79 ug/L

response 1862

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	34.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022210.D
 Acq On : 07 Mar 2022 18:52
 Operator : SY/VA
 Sample : N1816-05
 Misc : 6.66g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD2

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:26:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

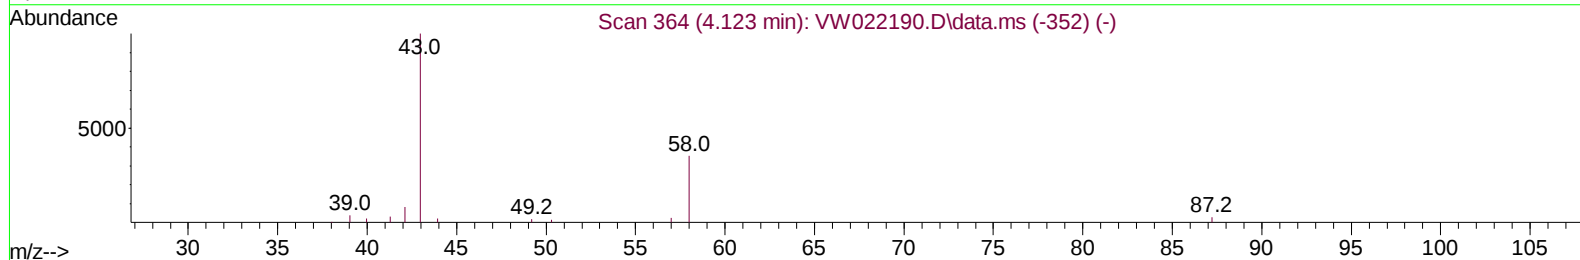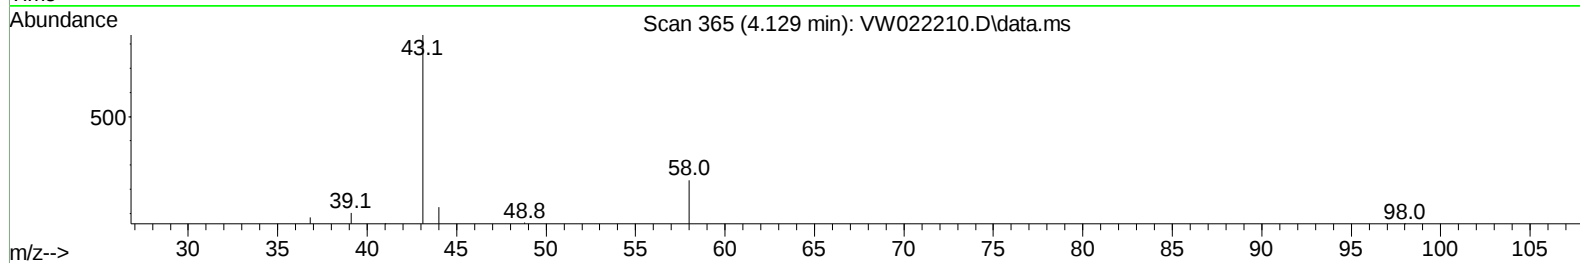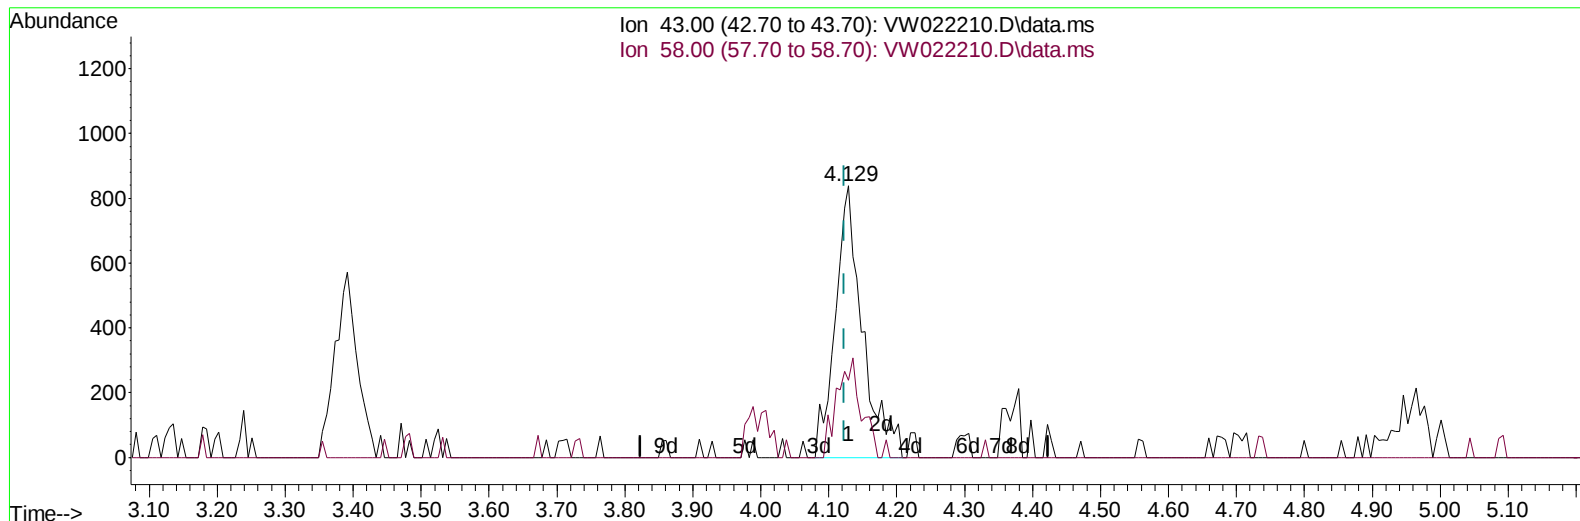

TIC: VW022210.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 8.50 ug/L m

response 2329

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	27.22
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022210.D
 Acq On : 07 Mar 2022 18:52
 Operator : SY/VA
 Sample : N1816-05
 Misc : 6.66g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD2

Manual IntegrationsAPPROVED

Quant Time: Mar 08 00:26:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/08/2022
 Supervised By :Mahesh Dadoda 03/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	153035	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	134455	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	57053	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	28477	14.267	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	57.080%	
7) Chloroethane-d5	2.886	69	27026	17.208	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	68.840%	
11) 1,1-Dichloroethene-d2	4.019	63	40588	13.278	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	53.120%	
21) 2-Butanone-d5	7.080	46	25207	75.109	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	150.220%#	
24) Chloroform-d	7.647	84	82186	24.070	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.280%	
26) 1,2-Dichloroethane-d4	8.305	65	43007	24.231	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	96.920%	
32) Benzene-d6	8.275	84	144162	23.038	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	92.160%	
36) 1,2-Dichloropropane-d6	9.275	67	44331	25.510	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	102.040%	
41) Toluene-d8	10.323	98	126772	20.378	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	81.520%	
43) trans-1,3-Dichloroprop...	10.579	79	16041	20.819	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	83.280%	
47) 2-Hexanone-d5	10.921	63	19664	68.800	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	137.600%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	46882	30.740	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	122.960%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	46162	25.191	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.760%	
Target Compounds						
13) Acetone	4.129	43	2329m	8.497	ug/L	
14) Carbon disulfide	4.385	76	848134	206.935	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022210.D
Acq On : 07 Mar 2022 18:52
Operator : SY/VA
Sample : N1816-05
Misc : 6.66g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSD2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/08/2022
Supervised By :Mahesh Dadoda 03/08/2022

Quant Time: Mar 08 00:26:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

