

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022211.D
 Acq On : 07 Mar 2022 19:16
 Operator : SY/VA
 Sample : N1816-03
 Misc : 6.91g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD0

Quant Time: Mar 08 00:26:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 08 00:21:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	121924	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	118630	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	58340	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	19906	12.517	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	50.080%
7) Chloroethane-d5	2.885	69	19699	15.744	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.960%
11) 1,1-Dichloroethene-d2	4.019	63	28366	11.648	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.600%
21) 2-Butanone-d5	7.080	46	21392	80.006	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	160.020%#
24) Chloroform-d	7.647	84	59672	21.936	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.760%
26) 1,2-Dichloroethane-d4	8.305	65	34906	24.685	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.760%
32) Benzene-d6	8.275	84	105589	19.125	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.480%
36) 1,2-Dichloropropane-d6	9.275	67	33263	21.694	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.760%
41) Toluene-d8	10.323	98	94082	17.140	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	68.560%
43) trans-1,3-Dichloroprop...	10.579	79	13215	19.439	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.760%
47) 2-Hexanone-d5	10.921	63	17134	67.945	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	135.880%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	39649	29.466	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	117.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	43156	23.031	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.120%
Target Compounds					Qvalue	
13) Acetone	4.123	43	1420	6.502	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
Data File : VW022211.D
Acq On : 07 Mar 2022 19:16
Operator : SY/VA
Sample : N1816-03
Misc : 6.91g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSD0

Quant Time: Mar 08 00:26:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 08 00:21:43 2022
Response via : Initial Calibration

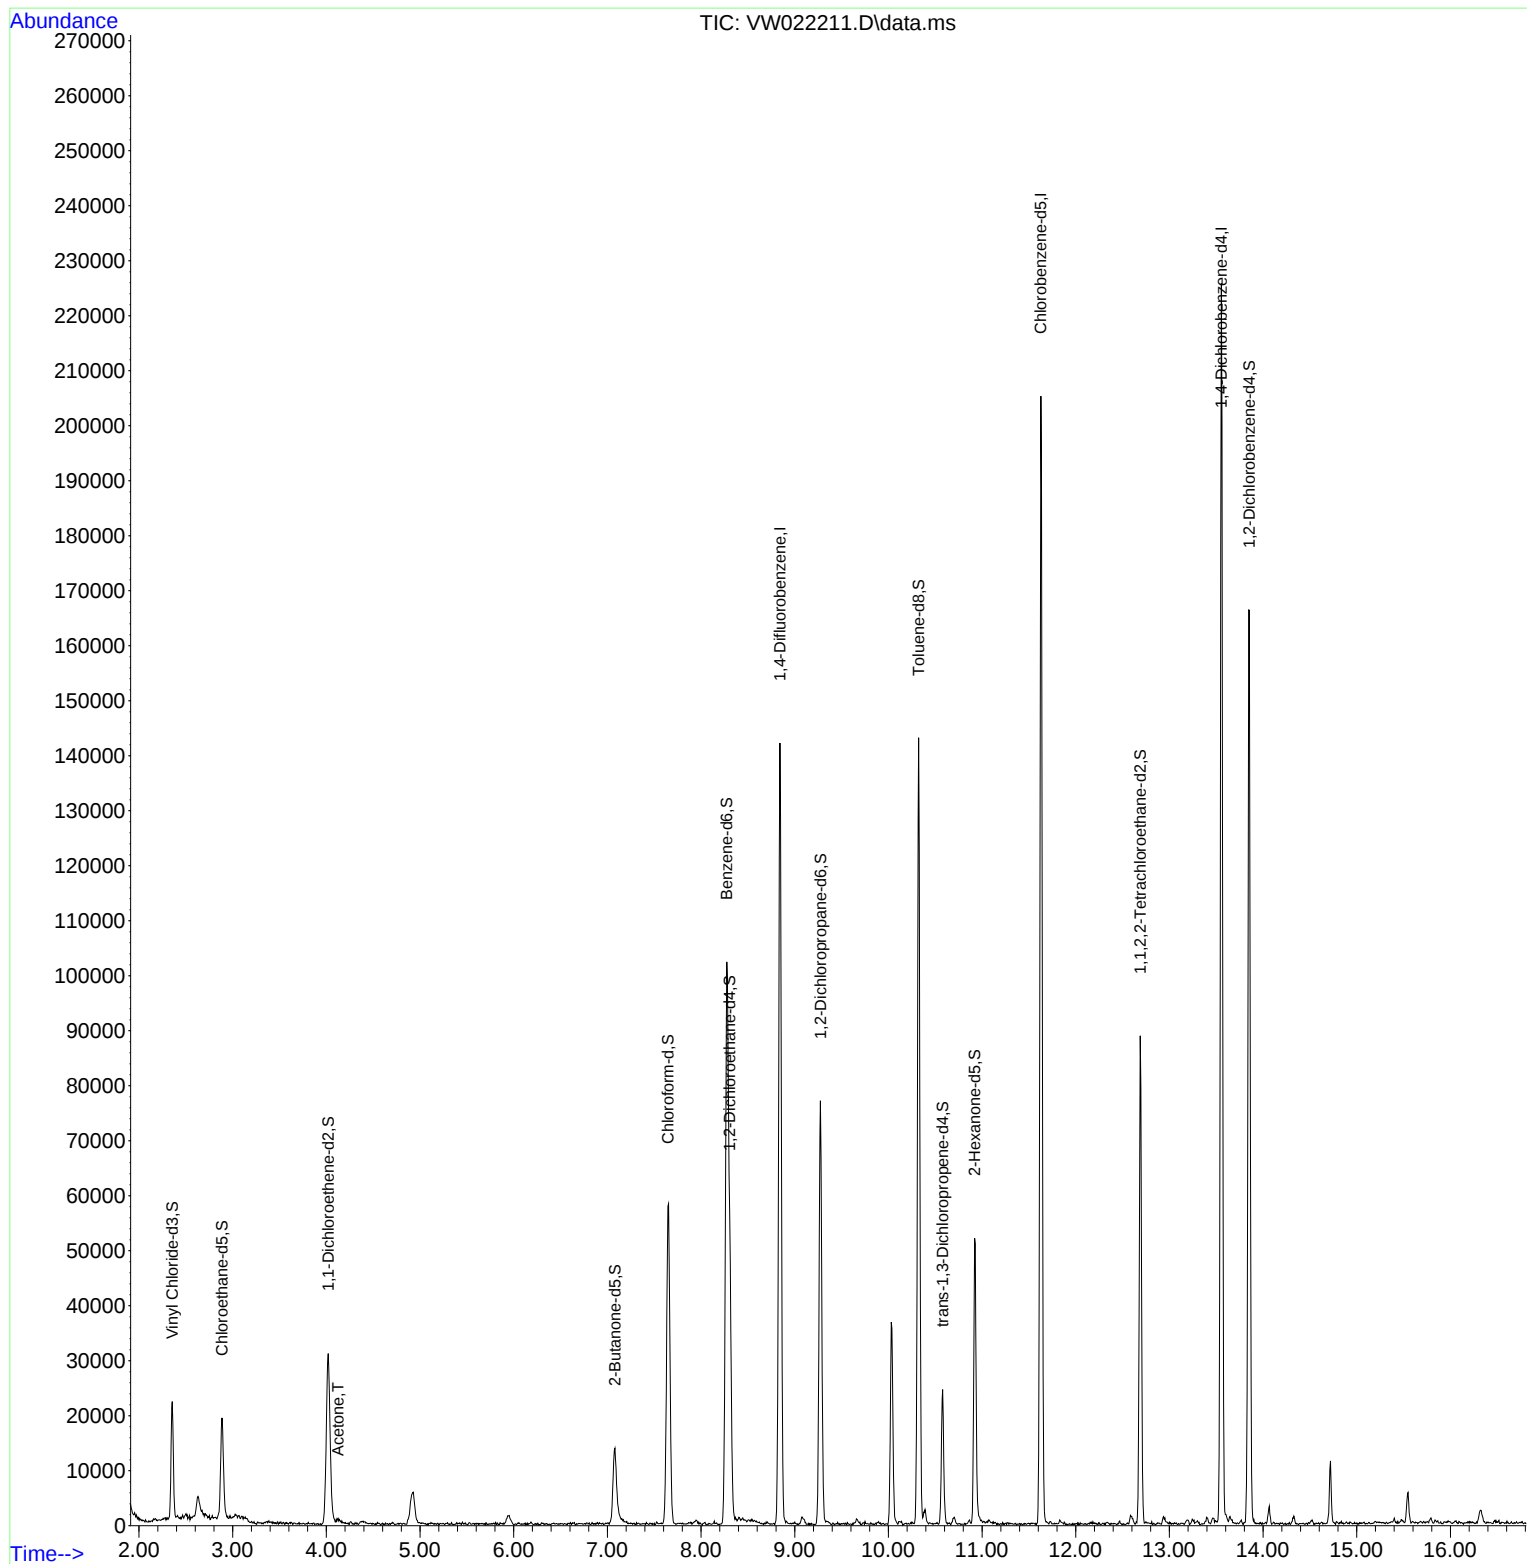

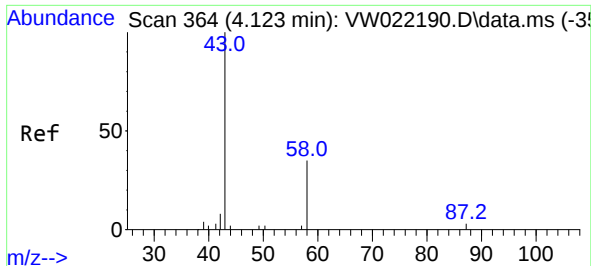

#13
 Acetone
 Concen: 6.502 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW022211.D
 Acq: 07 Mar 2022 19:16

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD0

Tgt Ion: 43 Resp: 1420
 Ion Ratio Lower Upper
 43 100
 58 41.3 0.0 69.2

