
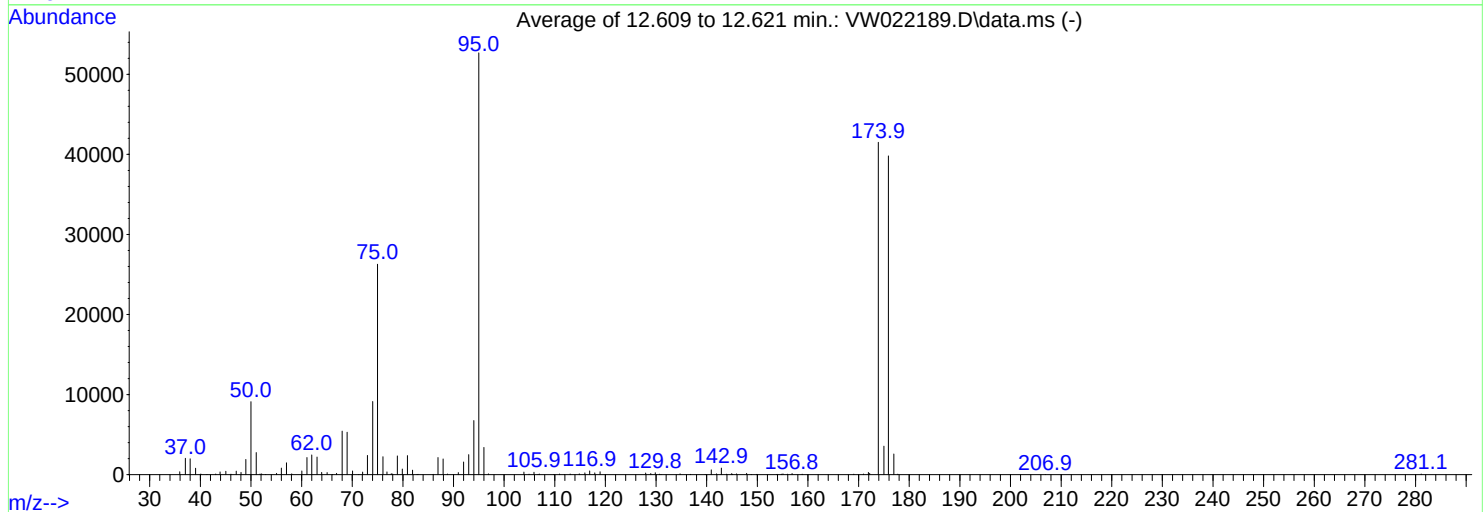


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030722\
 Data File : VW022189.D
 Acq On : 07 Mar 2022 09:34
 Operator : SY/VA
 Sample : BFB517
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB517

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Title : SFAM01.0
 Last Update : Tue Mar 08 00:21:43 2022

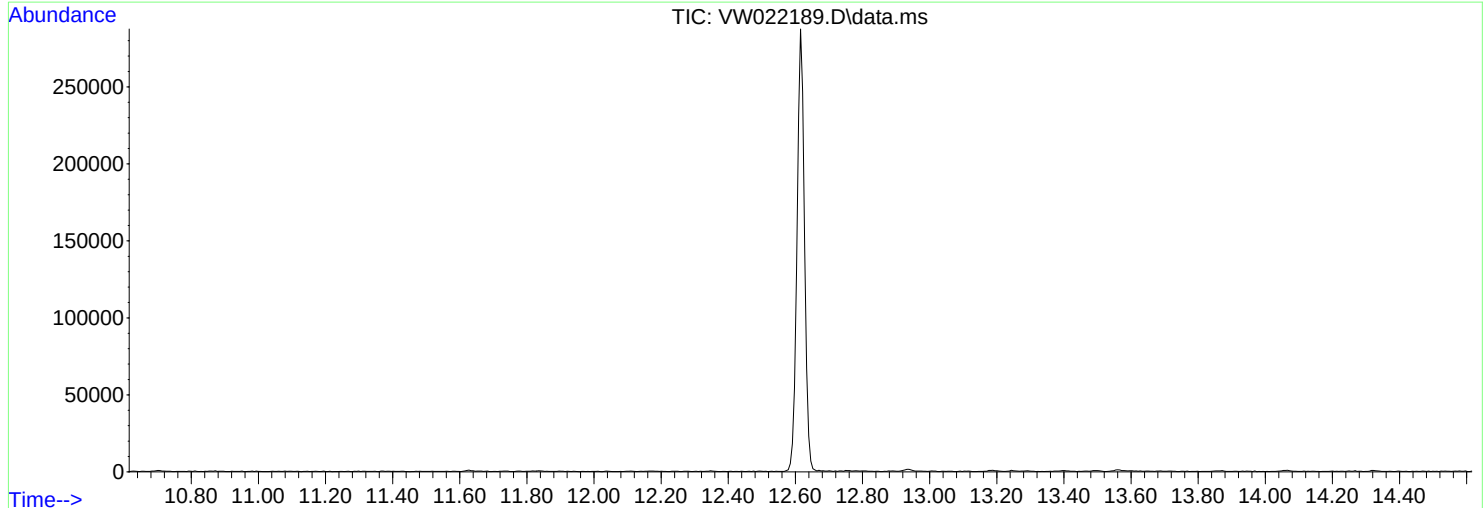

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	9117	PASS
75	95	30	80	49.9	26280	PASS
95	95	100	100	100.0	52683	PASS
96	95	5	9	6.5	3404	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.8	41499	PASS
175	174	5	9	8.6	3561	PASS
176	174	95	105	95.9	39811	PASS
177	176	5	10	6.5	2576	PASS

m/z	Abundance
39.90	131.0
41.00	56.0
42.50	73.0
44.00	91.0

Instrument :
MSVOA_W
ClientSampleId :
BFB517

m/z	Abundance
36.00	339.0
37.00	2160.0
38.00	1964.0
39.10	701.0
39.90	114.0
41.10	50.0
43.00	69.0
43.90	342.0
45.00	414.0
46.10	85.0
47.10	393.0
48.10	263.0
49.00	1887.0
50.00	8881.0
51.10	2734.0
52.10	183.0
52.90	75.0
55.10	173.0
56.00	744.0
57.00	1605.0
58.00	127.0
60.00	448.0
61.00	2213.0
62.00	2488.0
63.10	2172.0
64.00	283.0
65.10	351.0
66.10	54.0
66.90	153.0
68.00	5426.0
69.00	4690.0
70.10	460.0
71.30	58.0
72.20	279.0
73.00	2309.0
74.10	8587.0
75.00	24968.0
76.00	2082.0
76.80	274.0
78.00	273.0
78.90	2356.0
79.90	635.0
80.90	2308.0
81.90	628.0
87.00	1912.0
87.90	1790.0
88.80	86.0
90.90	297.0
92.00	1593.0
93.00	2378.0
94.00	6274.0
95.00	48704.0
96.00	3079.0
96.90	110.0
103.90	333.0
104.90	77.0
106.00	284.0
106.70	65.0
107.00	69.0
109.80	52.0
111.00	73.0
113.10	87.0
114.90	75.0
115.90	215.0
117.00	392.0
118.00	214.0
118.90	241.0
128.00	231.0
129.10	152.0
129.90	164.0
130.70	87.0
134.80	67.0
139.70	52.0
140.90	514.0
141.90	111.0
143.00	806.0
144.90	231.0
145.90	59.0
148.10	127.0
148.80	58.0
153.90	74.0
154.70	77.0
155.90	59.0
156.90	126.0
158.80	50.0
170.90	74.0
171.90	422.0
173.90	34984.0
175.00	3068.0
175.90	32216.0
177.00	2100.0
177.80	89.0

Instrument :
MSVOA_W
ClientSampleId :
BFB517

206.9076.0

281.20125.0

Instrument :
MSVOA_W
ClientSampleId :
BFB517

m/z	Abundance
36.00	424.0
37.10	2145.0
38.00	2241.0
39.10	878.0
40.10	121.0
41.30	54.0
43.10	110.0
43.80	498.0
45.10	464.0
47.10	558.0
48.10	363.0
49.00	2190.0
50.00	10366.0
51.00	2928.0
51.80	229.0
54.90	140.0
56.00	914.0
57.00	1622.0
58.10	82.0
60.10	425.0
61.10	2330.0
62.00	2501.0
63.00	2514.0
63.90	375.0
65.00	201.0
66.90	145.0
68.00	5936.0
69.00	6025.0
70.10	511.0
72.00	338.0
73.00	2675.0
74.00	10165.0
75.00	29120.0
76.10	2462.0
76.90	380.0
77.70	158.0
78.90	2424.0
79.90	736.0
80.90	2738.0
81.90	656.0
82.80	89.0
86.10	81.0
86.90	2703.0
88.00	2329.0
88.80	104.0
90.90	261.0
92.00	1838.0
93.00	2735.0
94.00	7506.0
95.00	59600.0
96.00	3963.0
96.90	143.0
104.00	311.0
105.00	60.0
105.90	342.0
106.90	100.0
111.00	85.0
111.90	67.0
113.10	67.0
114.90	124.0
116.00	243.0
116.90	518.0
117.90	287.0
118.90	515.0
127.80	199.0
128.90	122.0
129.80	334.0
130.70	124.0
134.80	151.0
141.00	713.0
142.00	109.0
142.80	899.0
144.00	94.0
145.10	161.0
145.90	129.0
147.90	213.0
149.90	66.0
153.90	53.0
155.00	192.0
156.00	66.0
156.80	161.0
158.90	65.0
169.10	54.0
170.90	83.0
172.20	459.0
173.90	46680.0
175.00	4187.0
175.90	45920.0
176.90	2924.0
177.70	110.0
281.00	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB517

m/z	Abundance
35.90	296.0
37.00	1794.0
38.00	1751.0
39.00	803.0
40.10	145.0
43.00	85.0
44.00	436.0
45.00	398.0
46.00	84.0
47.10	353.0
47.90	235.0
49.00	1602.0
50.00	8104.0
51.00	2621.0
52.10	146.0
55.10	173.0
56.00	800.0
57.00	1237.0
58.00	93.0
60.00	518.0
61.00	1860.0
62.00	2386.0
63.10	1926.0
63.90	162.0
65.00	245.0
66.90	197.0
68.00	4950.0
69.00	5173.0
70.00	414.0
72.00	348.0
73.00	2219.0
74.00	8672.0
75.00	24752.0
76.10	2162.0
76.90	350.0
77.70	194.0
78.90	2209.0
79.90	738.0
80.90	2074.0
81.90	402.0
83.00	97.0
85.90	73.0
87.00	1778.0
88.00	1783.0
88.80	56.0
91.00	224.0
92.00	1325.0
93.00	2392.0
94.00	6500.0
95.00	49744.0
96.00	3171.0
97.00	73.0
103.80	311.0
104.80	76.0
105.80	300.0
107.00	82.0
110.80	74.0
112.90	61.0
114.80	95.0
115.90	230.0
116.80	495.0
117.80	150.0
119.00	343.0
128.00	178.0
128.90	160.0
129.80	230.0
131.00	82.0
134.70	84.0
136.80	128.0
140.80	591.0
142.00	108.0
142.90	766.0
143.90	116.0
144.90	122.0
145.90	88.0
147.80	165.0
149.90	50.0
154.80	136.0
155.10	142.0
156.00	67.0
156.90	127.0
158.90	56.0
169.00	103.0
171.00	72.0
172.00	401.0
173.90	42832.0
175.00	3428.0
175.90	41296.0
176.90	2703.0

Instrument :
MSVOA_W
ClientSampleId :
BFB517