
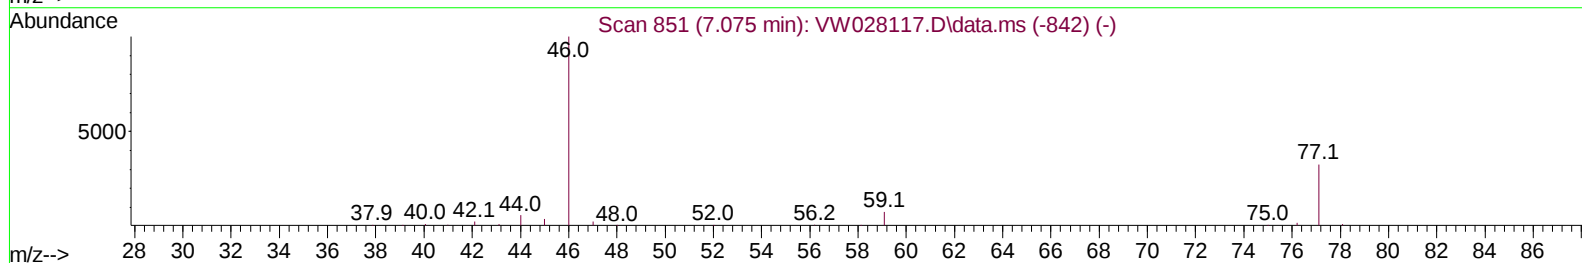
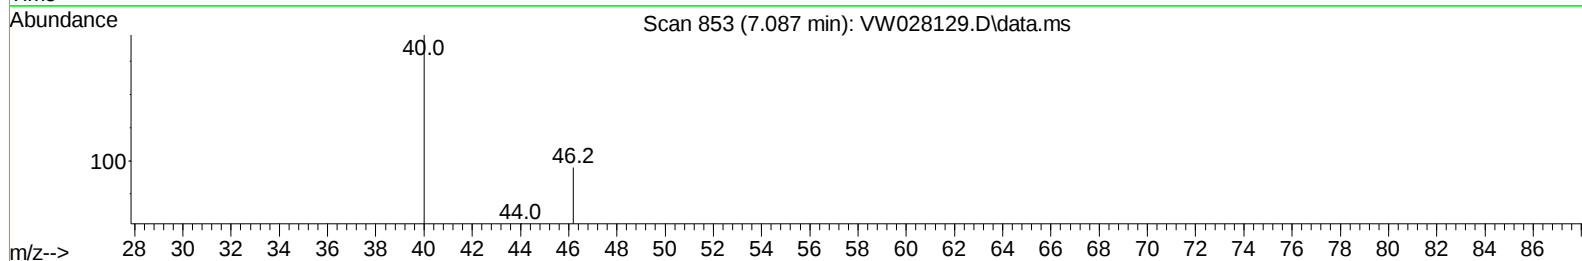


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030724\
Data File : VW028129.D
Acq On : 07 Mar 2024 16:08
Operator : SY/MD
Sample : P1638-08
Misc : 5.06g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 00:20:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 08 00:16:11 2024
Response via : Initial Calibration

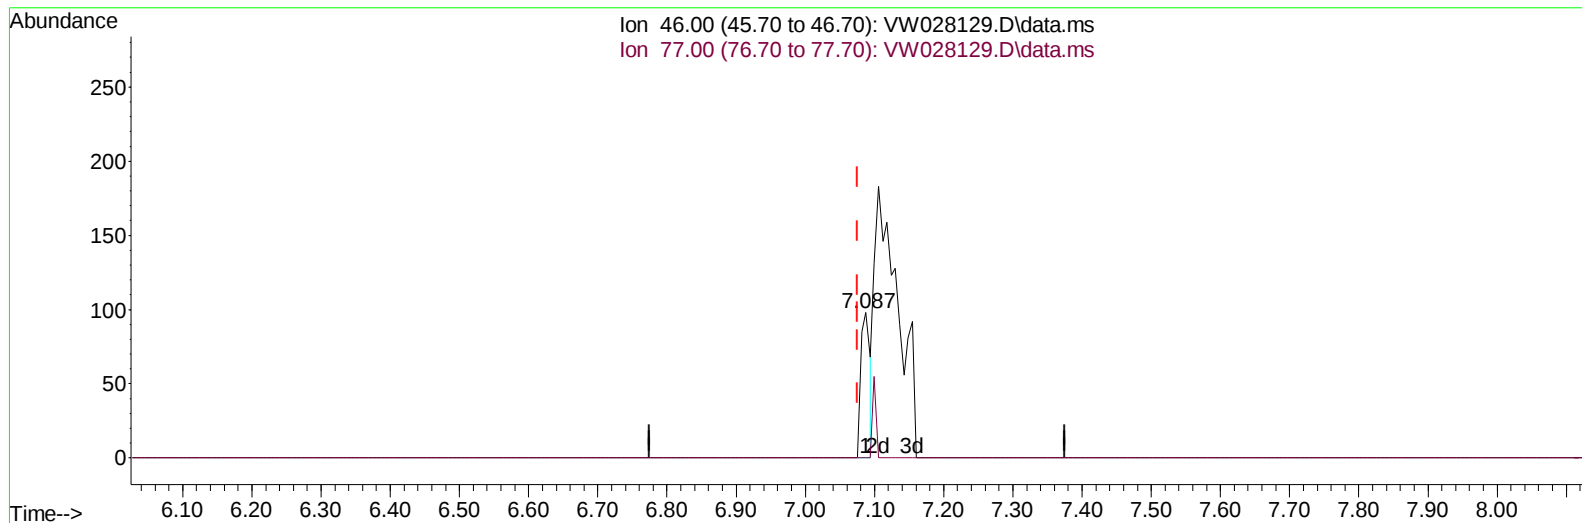

TIC: VW028129.D\data.ms

(21) 2-Butanone-d5 (S)




7.087min (+ 0.012) 2.18 ug/L

response 92

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	32.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030724\
Data File : VW028129.D
Acq On : 07 Mar 2024 16:08
Operator : SY/MD
Sample : P1638-08
Misc : 5.06g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 00:20:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 08 00:16:11 2024
Response via : Initial Calibration

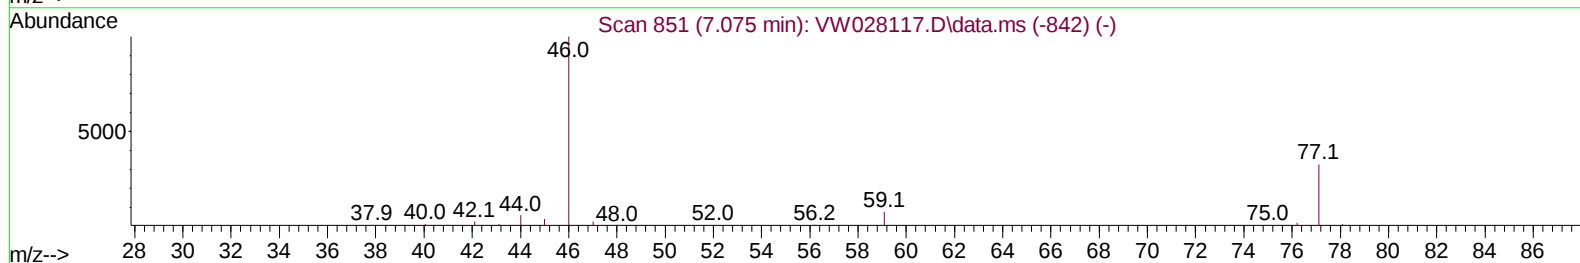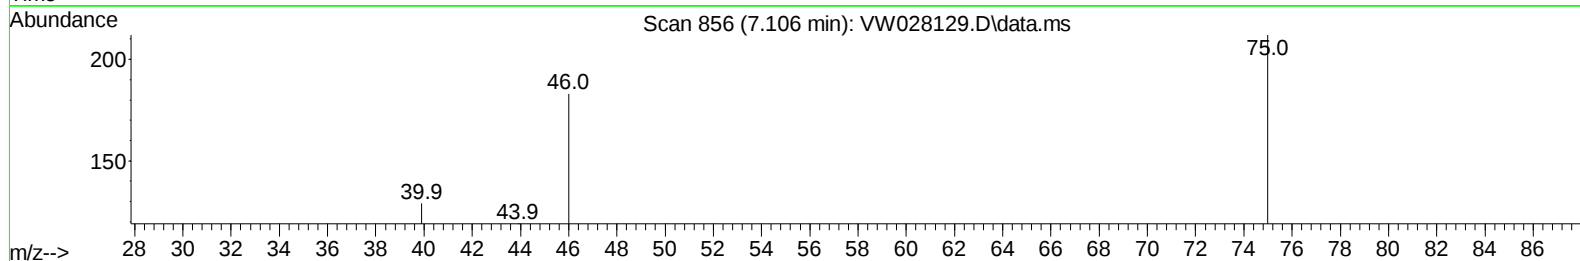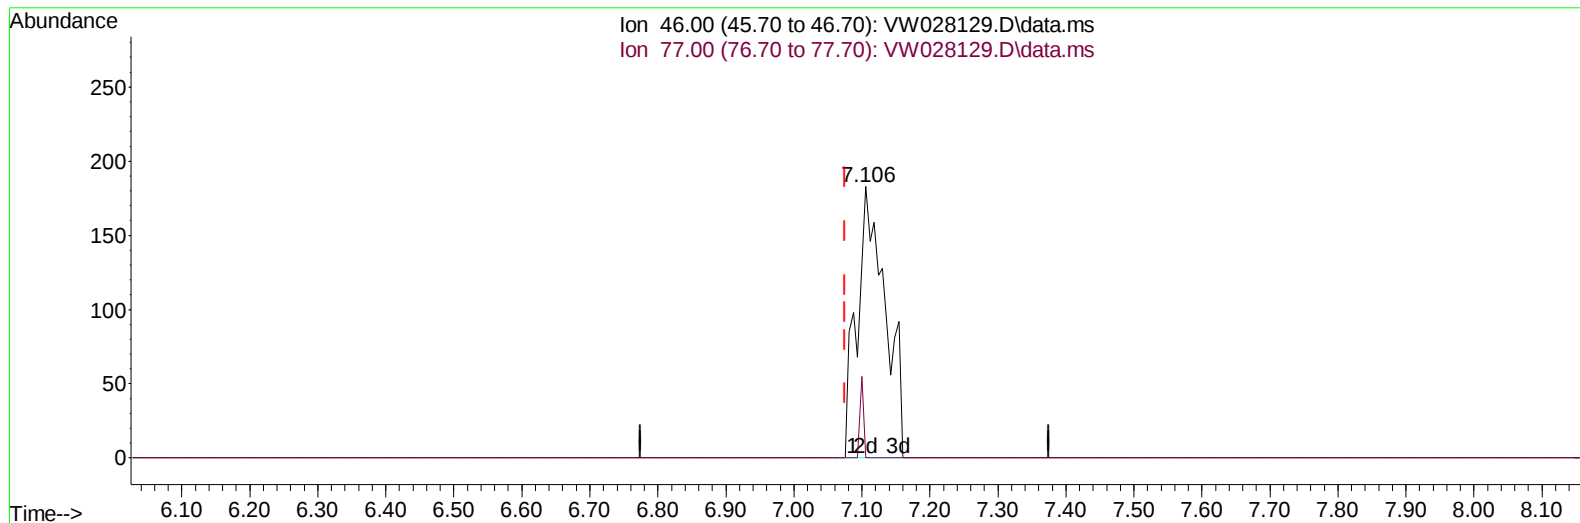

TIC: VW028129.D\data.ms

(21) 2-Butanone-d5 (S)

7.106min (+ 0.031) 12.47 ug/L m

response 527

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	32.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030724\
 Data File : VW028129.D
 Acq On : 07 Mar 2024 16:08
 Operator : SY/MD
 Sample : P1638-08
 Misc : 5.06g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 00:20:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 08 00:16:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	24815	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	21270	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	9329	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	5971	20.157	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	80.640%		
7) Chloroethane-d5	2.893	69	4757	20.730	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	82.920%		
11) 1,1-Dichloroethene-d2	4.027	65	2610	21.571	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	86.280%		
21) 2-Butanone-d5	7.106	46	527m	12.472	ug/L	0.03
Spiked Amount 50.000	Range 20	- 135	Recovery =	24.940%		
24) Chloroform-d	7.648	84	10859	20.661	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	82.640%		
26) 1,2-Dichloroethane-d4	8.307	65	5566	22.755	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	91.000%		
32) Benzene-d6	8.276	84	20410	20.555	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	82.240%		
36) 1,2-Dichloropropane-d6	9.270	67	5738	22.367	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	89.480%		
41) Toluene-d8	10.319	98	16452	17.582	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	70.320%		
43) trans-1,3-Dichloroprop...	10.575	79	1229	10.932	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	43.720%		
47) 2-Hexanone-d5	10.928	63	445	12.315	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	24.620%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	4680	23.114	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	92.440%		
66) 1,2-Dichlorobenzene-d4	13.848	152	5139	18.523	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	74.080%#		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030724\
Data File : VW028129.D
Acq On : 07 Mar 2024 16:08
Operator : SY/MD
Sample : P1638-08
Misc : 5.06g/10mL/MSVOA_W/SoIL/A
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 00:20:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 08 00:16:11 2024
Response via : Initial Calibration

