
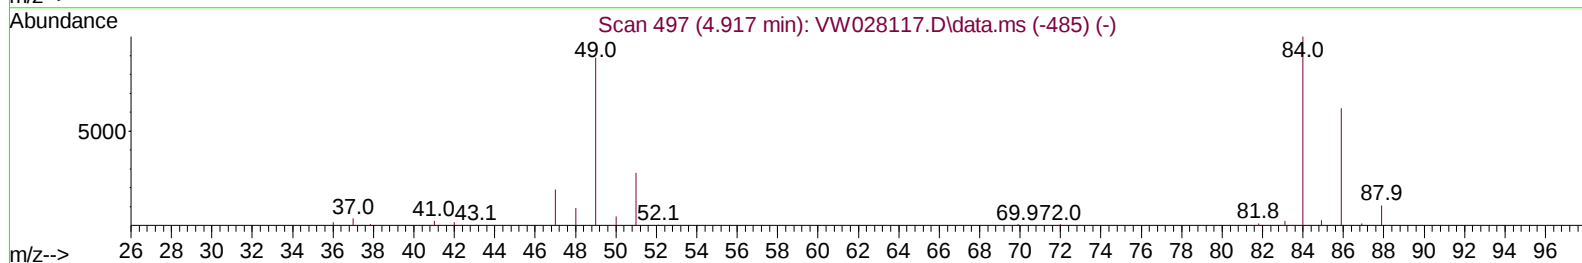
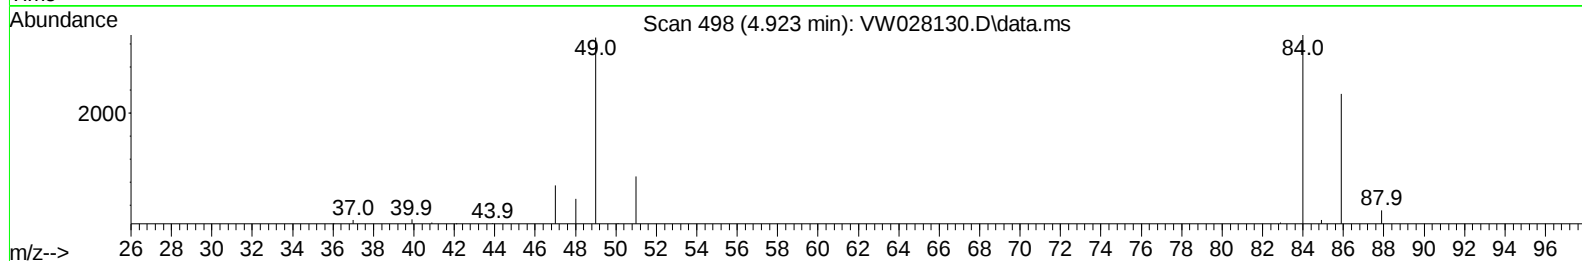


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030724\
Data File : VW028130.D
Acq On : 07 Mar 2024 16:32
Operator : SY/MD
Sample : P1638-02
Misc : 3.50g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 00:20:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 08 00:16:11 2024
Response via : Initial Calibration

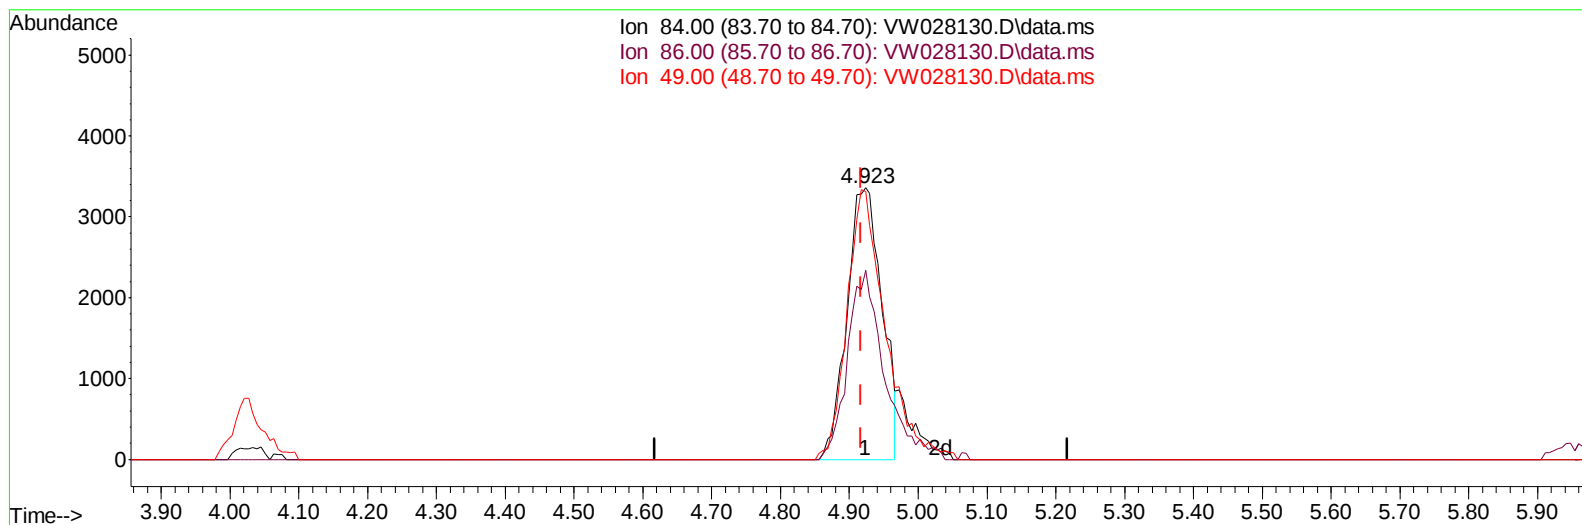

TIC: VW028130.D\data.ms

(16) Methylene chloride (T)




4.923min (+ 0.006) 2.16 ug/L

response 11888

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	58.90	69.62
49.00	95.00	98.57
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030724\
Data File : VW028130.D
Acq On : 07 Mar 2024 16:32
Operator : SY/MD
Sample : P1638-02
Misc : 3.50g/10mL/MSVOA_W/SOIL/B
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 00:20:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 08 00:16:11 2024
Response via : Initial Calibration

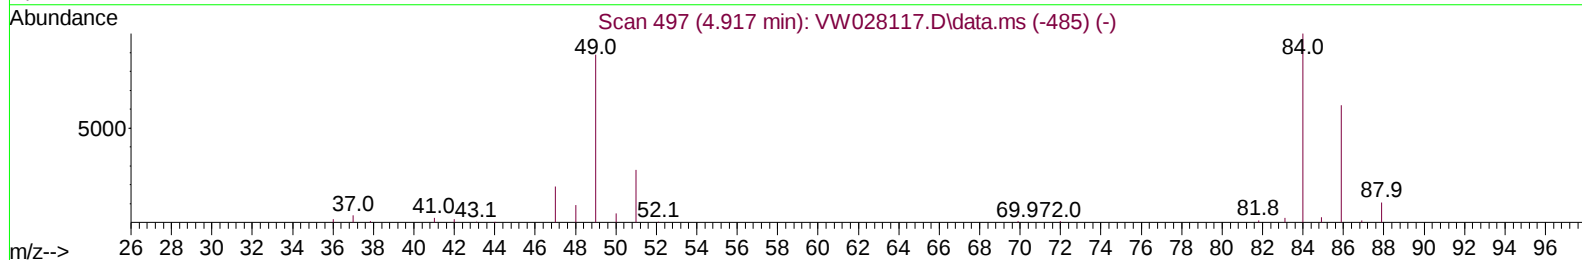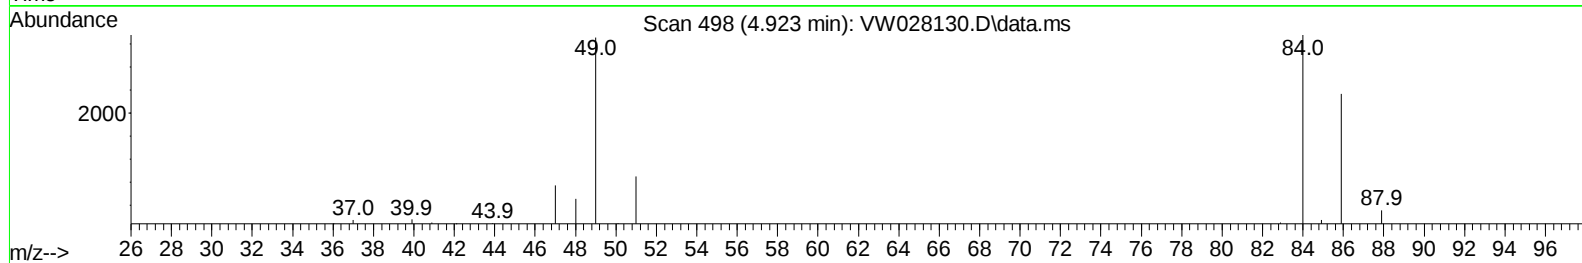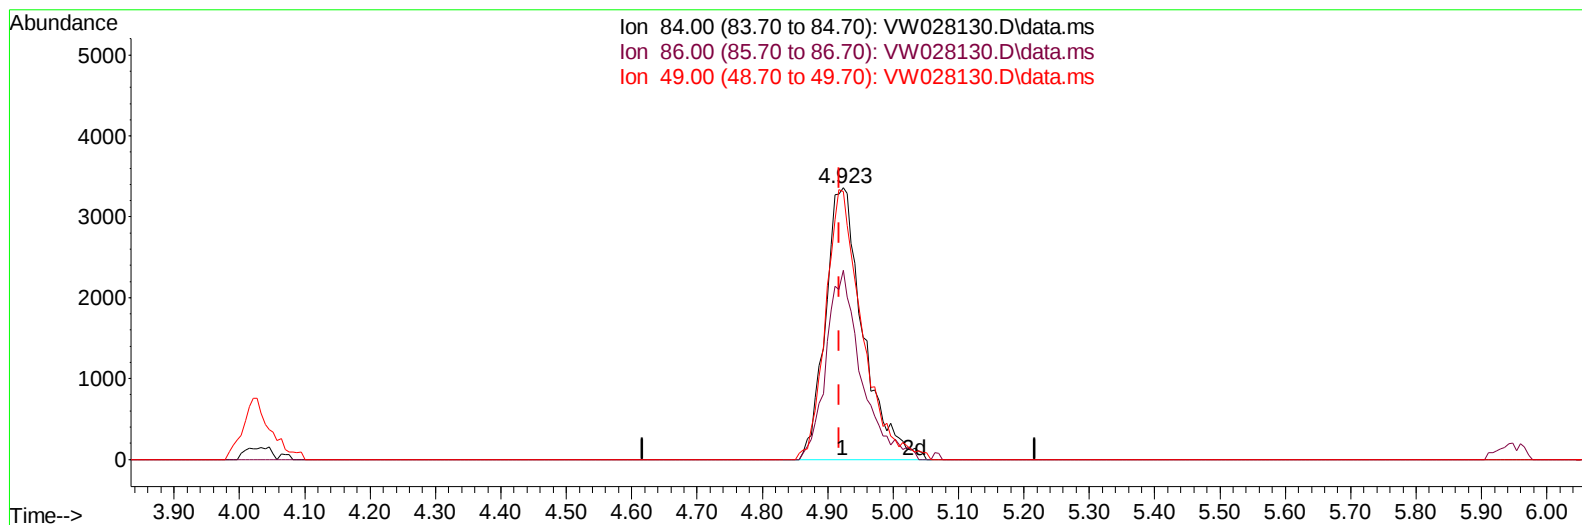

TIC: VW028130.D\data.ms

(16) Methylene chloride (T)

4.923min (+ 0.006) 2.44 ug/L m

response 13430

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	58.90	69.62
49.00	95.00	98.57
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030724\
 Data File : VW028130.D
 Acq On : 07 Mar 2024 16:32
 Operator : SY/MD
 Sample : P1638-02
 Misc : 3.50g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 00:20:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 08 00:16:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	400403	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	346114	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	158704	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	65791	13.765	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	55.040%	
7) Chloroethane-d5	2.893	69	31927	8.623	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	34.480%	
11) 1,1-Dichloroethene-d2	4.021	65	28082	14.384	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	57.520%	
21) 2-Butanone-d5	7.075	46	21427	31.426	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	62.860%	
24) Chloroform-d	7.648	84	115895	13.666	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	54.680%	
26) 1,2-Dichloroethane-d4	8.307	65	58168	14.738	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	58.960%#	
32) Benzene-d6	8.276	84	241782	14.964	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	59.840%	
36) 1,2-Dichloropropane-d6	9.270	67	62032	14.859	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	59.440%#	
41) Toluene-d8	10.319	98	225885	14.835	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	59.320%	
43) trans-1,3-Dichloroprop...	10.575	79	26581	14.530	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	58.120%	
47) 2-Hexanone-d5	10.922	63	20243	34.426	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	68.860%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	50336	15.277	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	61.120%	
66) 1,2-Dichlorobenzene-d4	13.849	152	65701	13.920	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	55.680%#	
Target Compounds						
					Qvalue	
13) Acetone	4.119	43	144257	151.366	ug/L	99
16) Methylene chloride	4.923	84	13430m	2.438	ug/L	
22) 2-Butanone	7.167	43	19989	18.780	ug/L	97
40) 4-Methyl-2-pentanone	10.209	43	3295	1.905	ug/L	94
42) Toluene	10.386	91	15472	0.732	ug/L	99
48) 2-Hexanone	10.965	43	3404	2.434	ug/L #	95
53) m,p-Xylene	11.837	106	5851	0.624	ug/L	85
65) 1,4-Dichlorobenzene	13.568	146	5462	0.538	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030724\
Data File : VW028130.D
Acq On : 07 Mar 2024 16:32
Operator : SY/MD
Sample : P1638-02
Misc : 3.50g/10mL/MSVOA_W/SoIL/B
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 00:20:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 08 00:16:11 2024
Response via : Initial Calibration

