
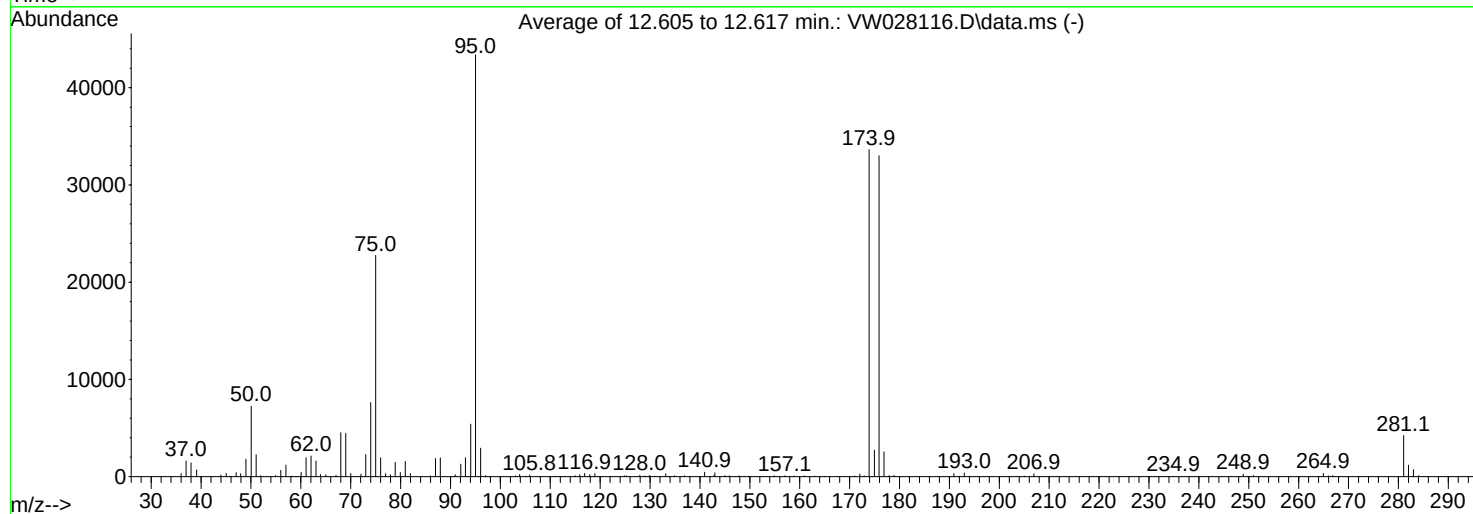


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030724\
Data File : VW028116.D
Acq On : 07 Mar 2024 08:15
Operator : SY/MD
Sample : BFB448
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB448

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Title : SFAM01.0
Last Update : Fri Mar 08 00:16:11 2024

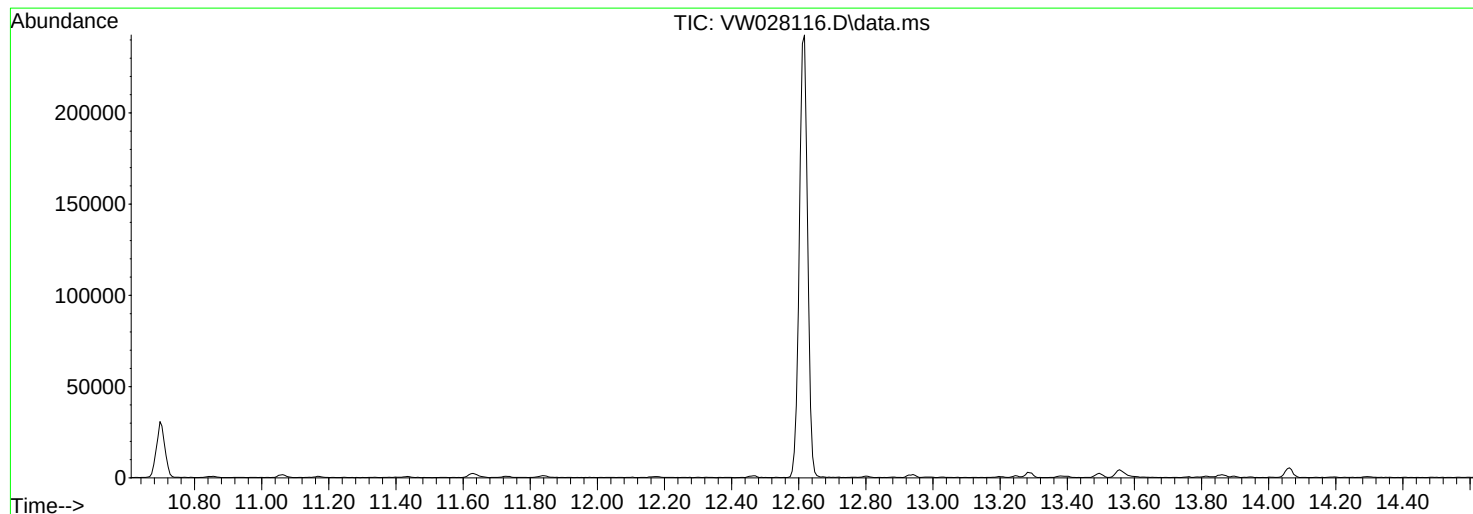

AutoFind: Scans 1758, 1759, 1760; Background Corrected with Scan 1752

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	7246	PASS
75	95	30	80	52.5	22757	PASS
95	95	100	100	100.0	43379	PASS
96	95	5	9	6.7	2927	PASS
173	174	0.00	2	0.2	80	PASS
174	95	50	120	77.5	33637	PASS
175	174	5	9	8.1	2738	PASS
176	174	95	101	98.1	33005	PASS
177	176	5	9	7.7	2550	PASS

m/z	Abundance
39.90	156.0
43.90	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

m/z	Abundance
36.00	367.0
37.00	1304.0
38.00	1100.0
39.10	502.0
40.00	193.0
44.00	265.0
45.10	256.0
47.00	351.0
48.00	222.0
49.00	1680.0
50.10	6082.0
51.10	1862.0
54.90	83.0
56.00	471.0
57.00	823.0
58.20	77.0
59.00	52.0
60.00	343.0
61.00	1614.0
62.00	1664.0
63.00	1319.0
64.00	159.0
65.00	231.0
67.00	134.0
68.00	3667.0
69.00	3511.0
70.00	222.0
72.10	209.0
73.00	1809.0
74.00	5937.0
75.00	18776.0
76.00	1638.0
77.00	261.0
78.10	96.0
78.90	1200.0
80.00	379.0
80.90	1398.0
82.00	293.0
87.00	1749.0
87.90	1403.0
90.90	137.0
92.10	972.0
93.00	1529.0
94.00	3750.0
95.00	32624.0
96.00	2393.0
97.00	61.0
103.10	89.0
103.90	186.0
105.00	92.0
105.80	125.0
110.80	52.0
112.80	74.0
115.10	61.0
115.90	134.0
116.90	206.0
117.80	132.0
119.00	243.0
124.90	200.0
125.30	113.0
128.00	99.0
128.80	74.0
129.70	88.0
130.90	64.0
133.10	515.0
134.90	101.0
136.90	84.0
140.90	461.0
142.80	366.0
145.00	71.0
145.90	67.0
147.00	123.0
147.80	105.0
148.90	66.0
149.80	55.0
154.90	67.0
157.00	86.0
161.00	103.0
163.00	65.0
165.00	87.0
171.00	53.0
172.00	280.0
172.90	240.0
173.90	24440.0
175.00	2030.0
175.90	25616.0
176.90	1677.0
177.90	78.0
178.90	89.0
190.90	471.0
192.00	70.0
193.00	576.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

194.00	101.0
194.80	55.0
205.00	112.0
207.00	496.0
235.00	52.0
249.00	313.0
249.60	101.0
250.10	84.0
251.00	215.0
265.00	602.0
266.80	156.0
281.00	5788.0
282.00	1574.0
283.00	928.0
284.10	200.0
285.10	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

m/z	Abundance
36.00	231.0
37.00	1744.0
38.00	1714.0
39.10	815.0
40.10	155.0
44.00	302.0
45.00	372.0
46.00	50.0
47.00	422.0
47.80	217.0
48.10	230.0
49.00	1742.0
50.00	7655.0
51.00	2487.0
51.90	145.0
55.00	171.0
56.00	595.0
57.00	1532.0
58.20	66.0
60.10	475.0
61.10	2091.0
62.10	2307.0
63.00	1848.0
64.00	254.0
65.00	244.0
67.00	132.0
68.00	5089.0
69.00	5008.0
70.00	384.0
72.00	336.0
73.00	2568.0
74.00	8624.0
75.00	24544.0
76.00	2004.0
77.00	395.0
77.90	327.0
78.90	1628.0
79.90	495.0
81.00	1673.0
81.90	342.0
86.00	113.0
87.00	1967.0
88.00	2037.0
91.00	268.0
92.10	1541.0
93.00	2230.0
94.00	6042.0
95.00	49872.0
96.10	3373.0
97.10	117.0
103.00	88.0
103.80	214.0
105.20	92.0
105.90	125.0
114.90	94.0
115.90	198.0
116.90	371.0
117.90	262.0
118.90	374.0
125.20	149.0
127.90	213.0
129.00	94.0
129.90	152.0
130.90	59.0
133.20	244.0
133.90	100.0
134.80	80.0
136.80	132.0
141.00	517.0
143.00	634.0
145.00	135.0
145.80	98.0
148.00	102.0
149.80	74.0
154.90	120.0
157.00	92.0
158.90	96.0
160.90	67.0
163.10	82.0
171.00	76.0
172.10	272.0
173.90	37600.0
174.90	2771.0
175.90	32024.0
176.90	2600.0
177.90	112.0
178.90	214.0
190.90	351.0
191.90	72.0
193.00	416.0
194.10	74.0
205.10	66.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

206.90	293.0
234.90	62.0
248.80	262.0
249.70	69.0
250.90	148.0
264.90	221.0
266.00	167.0
266.80	141.0
281.10	3692.0
282.00	1248.0
282.90	398.0
283.10	405.0
284.10	132.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448

m/z	Abundance
36.00	357.0
37.00	1786.0
38.00	1449.0
39.10	746.0
39.90	211.0
44.00	308.0
45.00	350.0
45.90	69.0
47.10	460.0
48.00	224.0
49.00	1973.0
50.00	8000.0
51.00	2439.0
51.90	85.0
55.00	119.0
56.00	876.0
57.00	1186.0
60.00	469.0
61.00	2131.0
62.00	2390.0
63.10	1667.0
63.90	220.0
65.10	146.0
67.10	159.0
68.00	4800.0
69.00	4789.0
70.00	379.0
72.00	240.0
73.00	2434.0
74.00	8317.0
75.00	24952.0
76.00	2171.0
77.00	266.0
77.90	160.0
78.90	1577.0
80.00	404.0
81.00	1604.0
82.00	292.0
85.90	161.0
87.00	1858.0
88.00	2359.0
91.00	166.0
92.00	1351.0
93.00	2079.0
94.10	6385.0
95.00	47640.0
96.00	3014.0
97.10	131.0
102.90	53.0
103.90	274.0
105.90	224.0
111.00	81.0
115.00	136.0
115.90	258.0
116.90	399.0
118.00	181.0
119.00	269.0
124.90	55.0
128.00	155.0
129.00	105.0
130.00	239.0
133.10	155.0
135.00	126.0
136.90	78.0
140.90	420.0
143.00	574.0
145.00	94.0
145.90	93.0
147.80	168.0
154.80	77.0
157.10	100.0
158.80	101.0
160.80	62.0
171.10	72.0
172.00	272.0
173.90	38872.0
174.90	3414.0
175.90	41376.0
176.90	3374.0
177.90	144.0
179.00	78.0
191.00	124.0
193.10	131.0
207.10	125.0
248.90	180.0
264.90	186.0
266.00	79.0
267.00	61.0
281.00	3205.0
282.00	716.0
283.00	445.0

Instrument :
MSVOA_W
ClientSampleId :
BFB448