

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022218.D
Acq On : 08 Mar 2022 11:12
Operator : SY/VA
Sample : N1816-13
Misc : 4.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSD8




Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:24:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

03/10/2022
Supervised By :Mahesh
Dadoda

03/11/2022

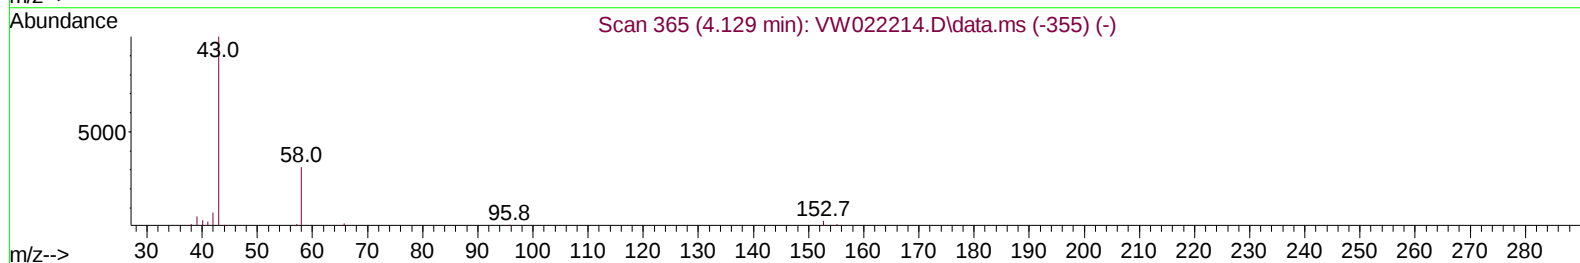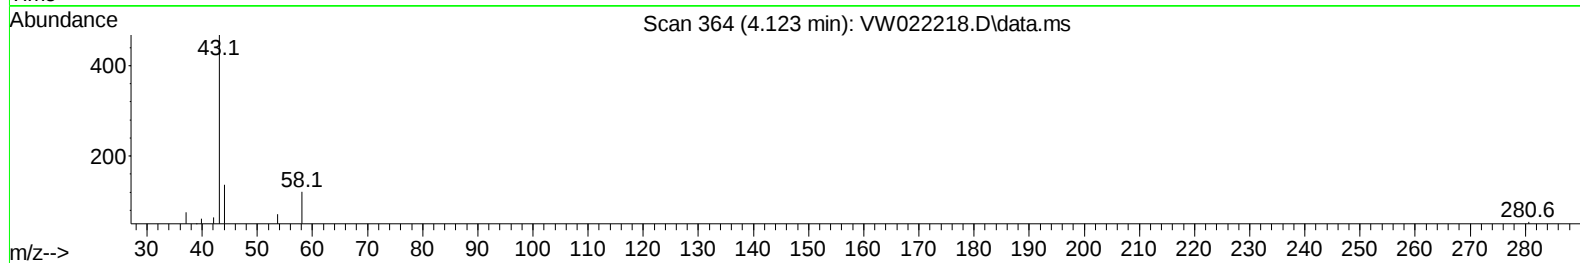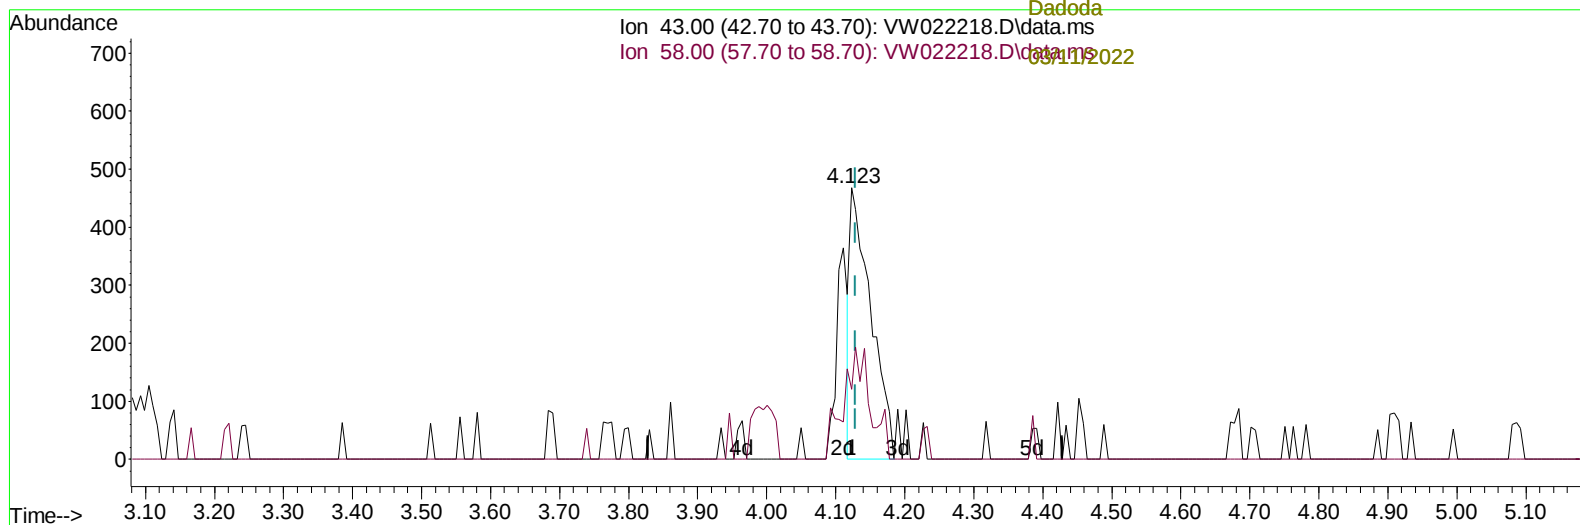

TIC: VW022218.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 3.41 ug/L

response 980

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	37.35
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022218.D
 Acq On : 08 Mar 2022 11:12
 Operator : SY/VA
 Sample : N1816-13
 Misc : 4.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD8

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:24:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

03/10/2022
 Supervised By :Mahesh
 Dadoda
 03/11/2022

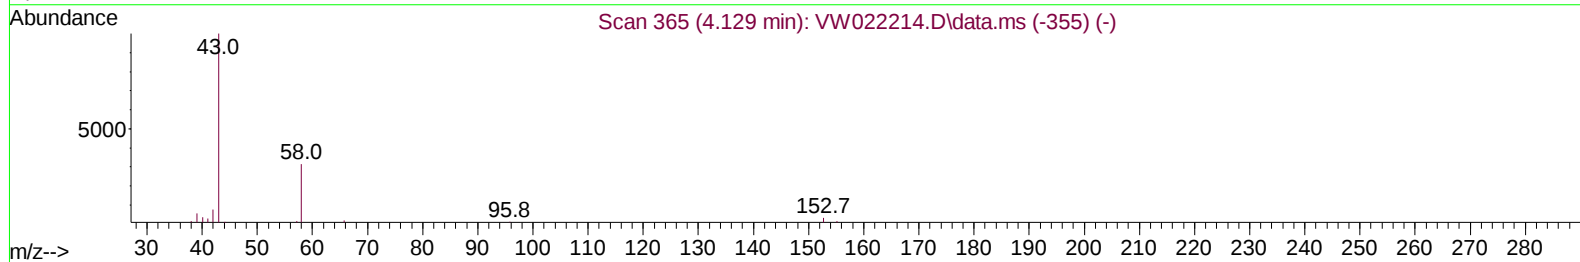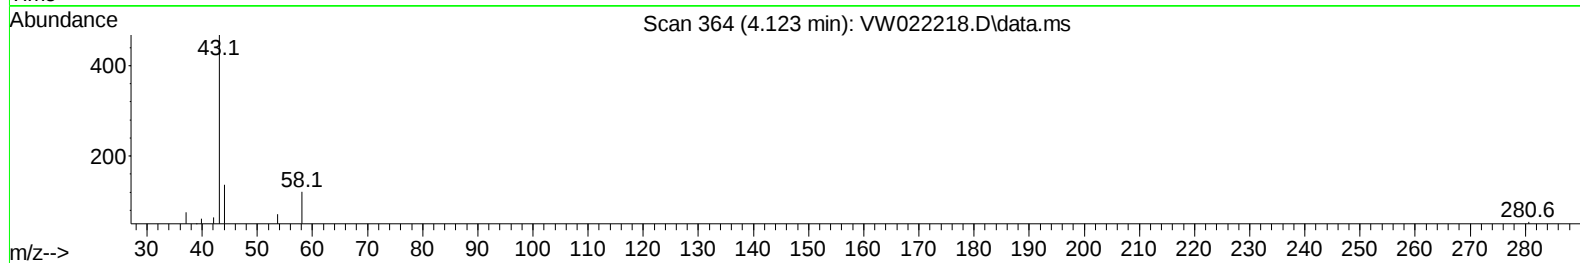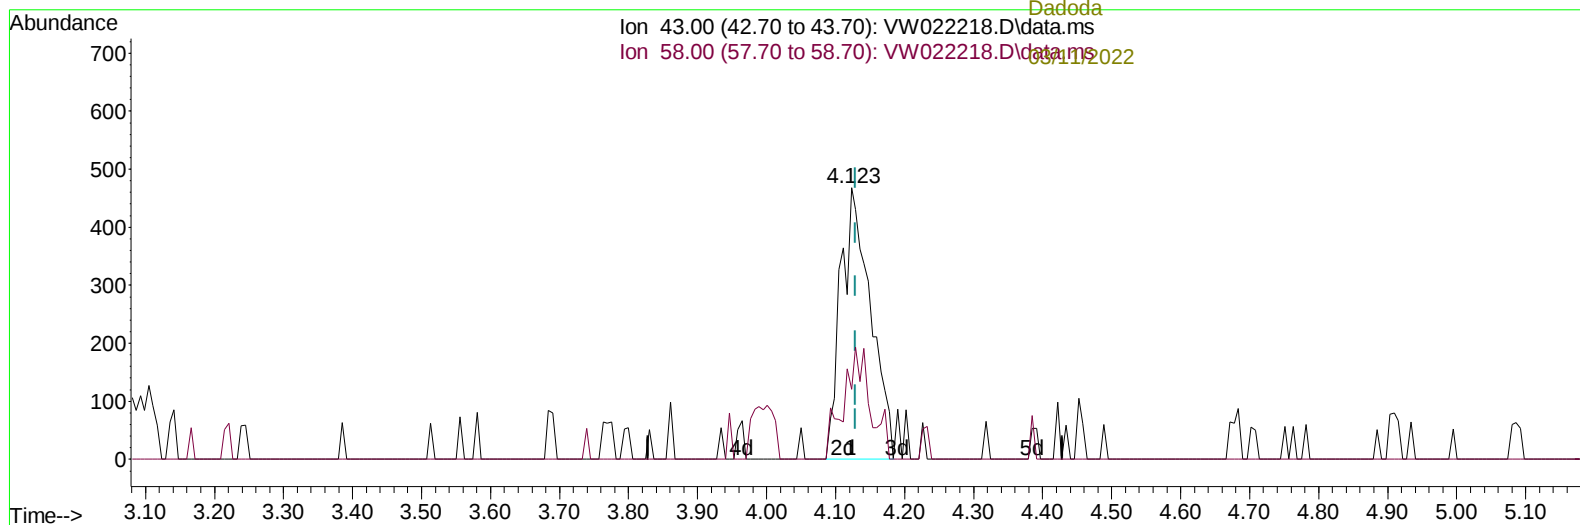

TIC: VW022218.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.88 ug/L m

response 1401

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	26.12
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022218.D
Acq On : 08 Mar 2022 11:12
Operator : SY/VA
Sample : N1816-13
Misc : 4.00g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSD8




Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:24:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

03/10/2022
Supervised By :Mahesh
Dadoda

03/11/2022

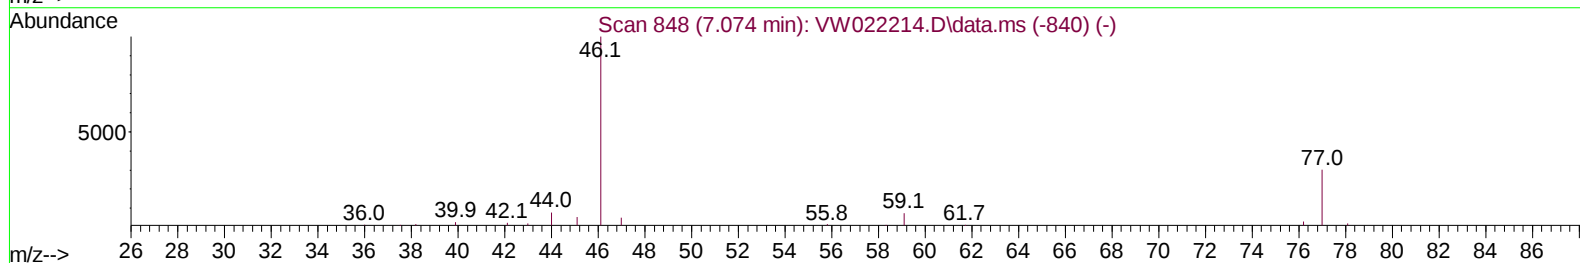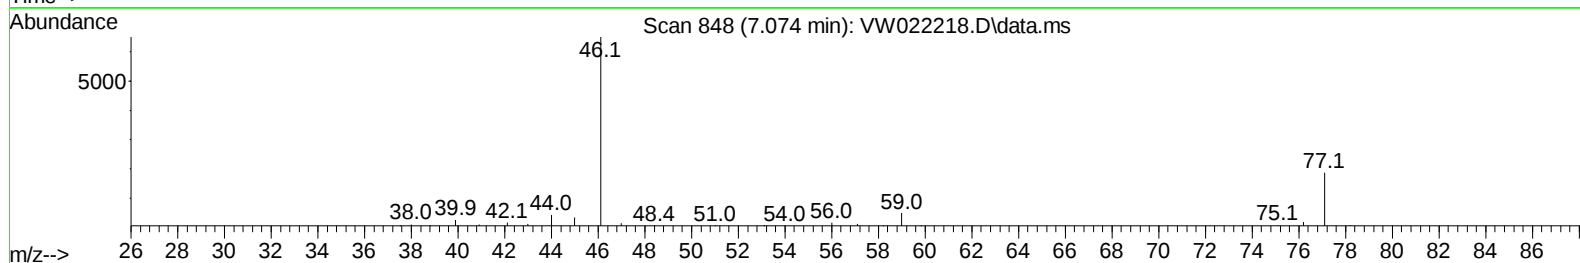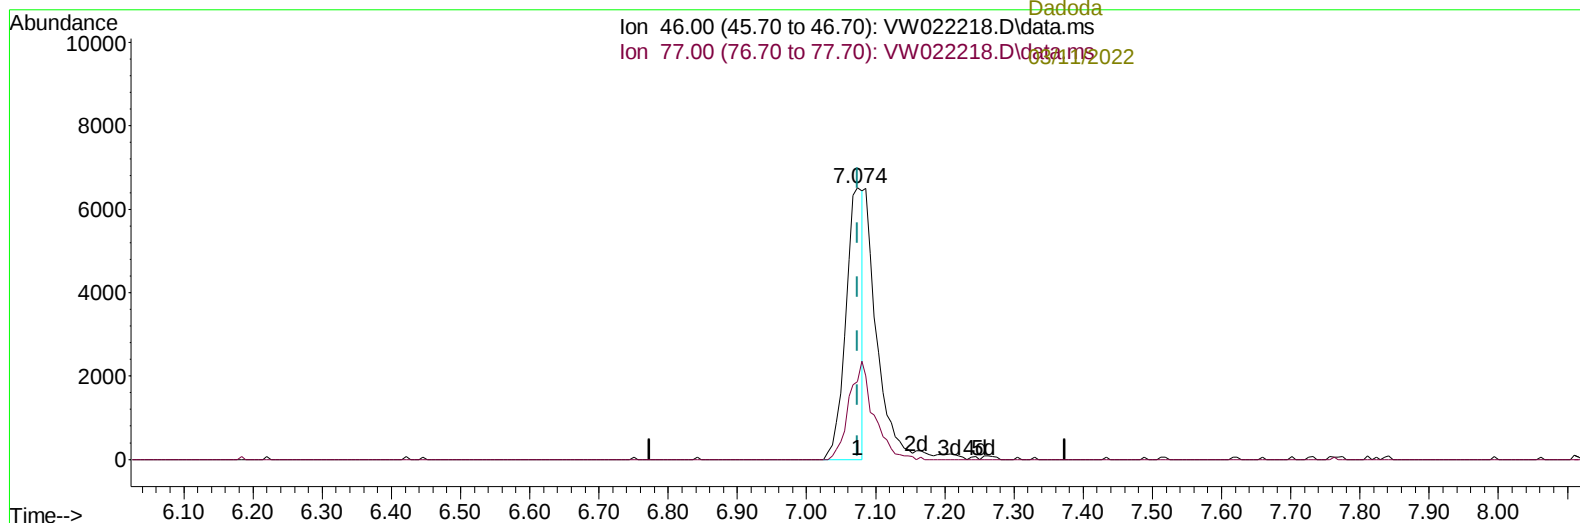

TIC: VW022218.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (+ 0.000) 31.26 ug/L

response 10991

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	28.10	52.50#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022218.D
 Acq On : 08 Mar 2022 11:12
 Operator : SY/VA
 Sample : N1816-13
 Misc : 4.00g/10mL/MSVOA_W/SoIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD8

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:24:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

03/10/2022
 Supervised By :Mahesh
 Dadoda
 03/11/2022

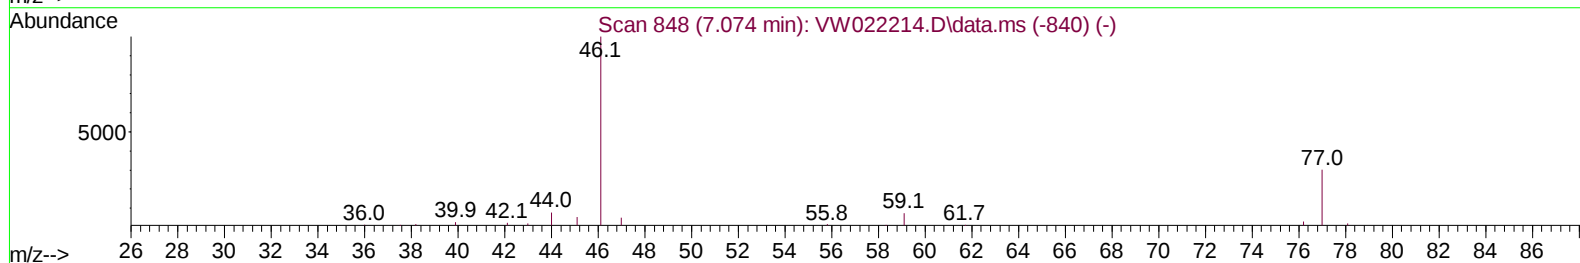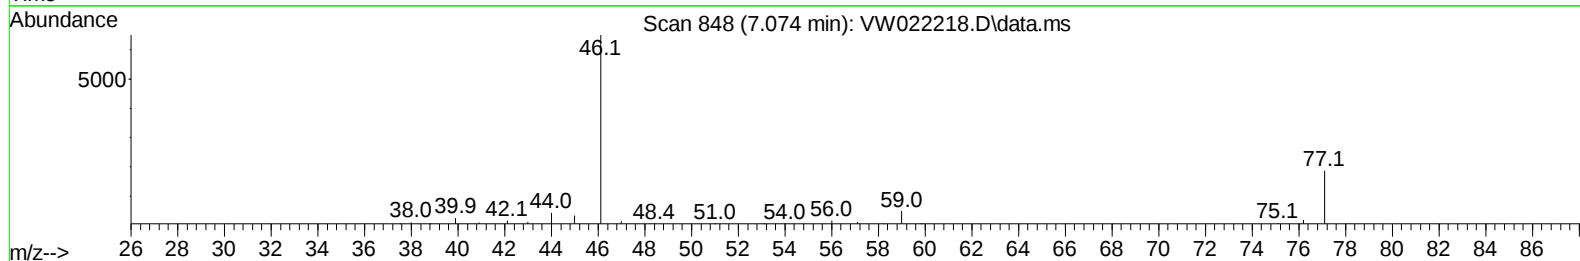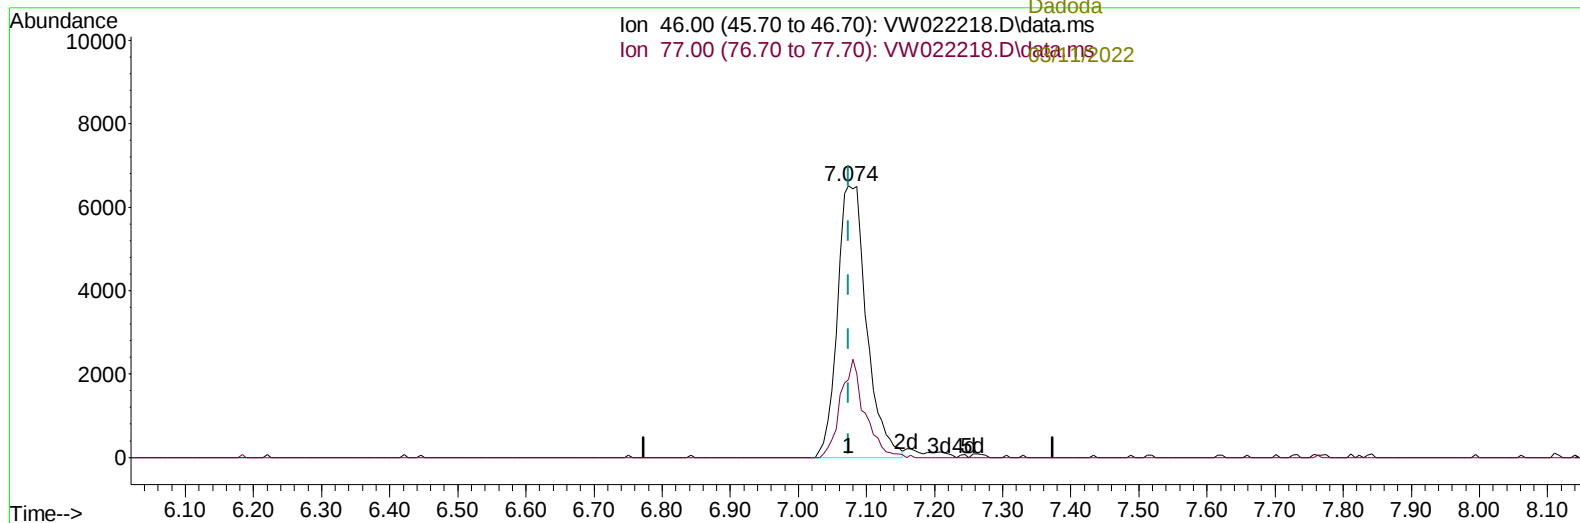

TIC: VW022218.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (+ 0.000) 54.79 ug/L m

response 19263

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	28.10	29.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022218.D
 Acq On : 08 Mar 2022 11:12
 Operator : SY/VA
 Sample : N1816-13
 Misc : 4.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

03/10/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Mar 09 00:24:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----03/11/2022						
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	160317	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	152616	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	77496	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	25020	11.965	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	47.880%	
7) Chloroethane-d5	2.879	69	25134	15.277	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	61.120%	
11) 1,1-Dichloroethene-d2	4.013	63	33513	10.466	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	41.880%#	
21) 2-Butanone-d5	7.074	46	19263m	54.790	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	109.580%	
24) Chloroform-d	7.647	84	74123	20.723	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.880%	
26) 1,2-Dichloroethane-d4	8.305	65	38559	20.738	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	82.960%	
32) Benzene-d6	8.275	84	125768	17.707	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	70.840%	
36) 1,2-Dichloropropane-d6	9.274	67	40646	20.606	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	82.440%	
41) Toluene-d8	10.323	98	117239	16.603	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	66.400%	
43) trans-1,3-Dichloroprop...	10.579	79	14474	16.550	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	66.200%	
47) 2-Hexanone-d5	10.920	63	15690	48.363	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.720%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	40341	23.304	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	93.200%	
66) 1,2-Dichlorobenzene-d4	13.847	152	52706	21.175	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	84.680%	
Target Compounds						
13) Acetone	4.123	43	1401m	4.879	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022218.D
Acq On : 08 Mar 2022 11:12
Operator : SY/VA
Sample : N1816-13
Misc : 4.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSD8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

03/10/2022
Supervised By :Mahesh
Dadoda

03/11/2022

Quant Time: Mar 09 00:24:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

