




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022229.D
 Acq On : 08 Mar 2022 15:38
 Operator : SY/VA
 Sample : N1816-19
 Misc : 6.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSE4

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:26:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

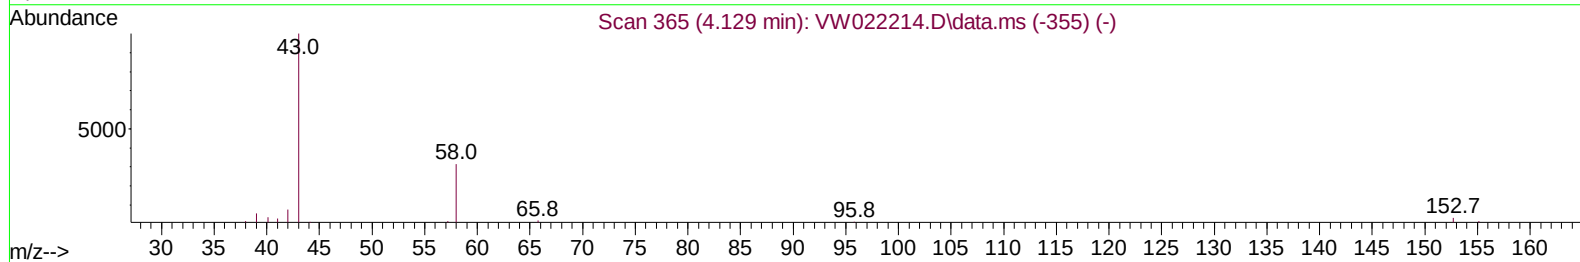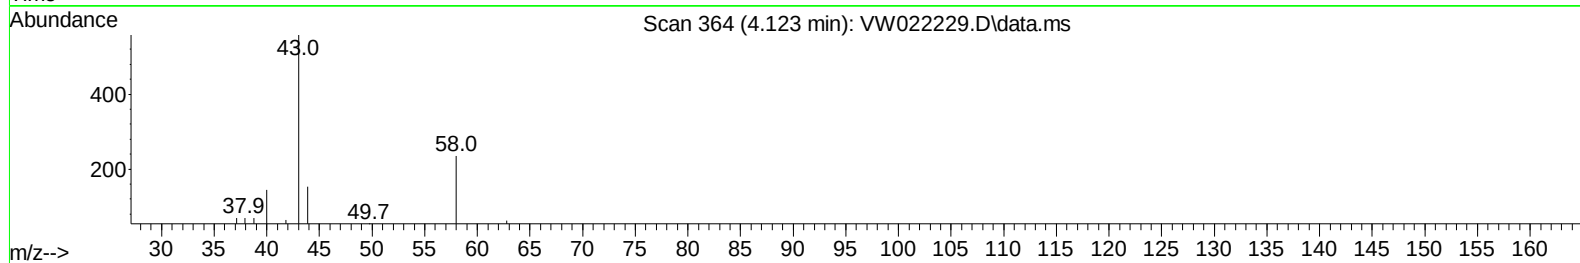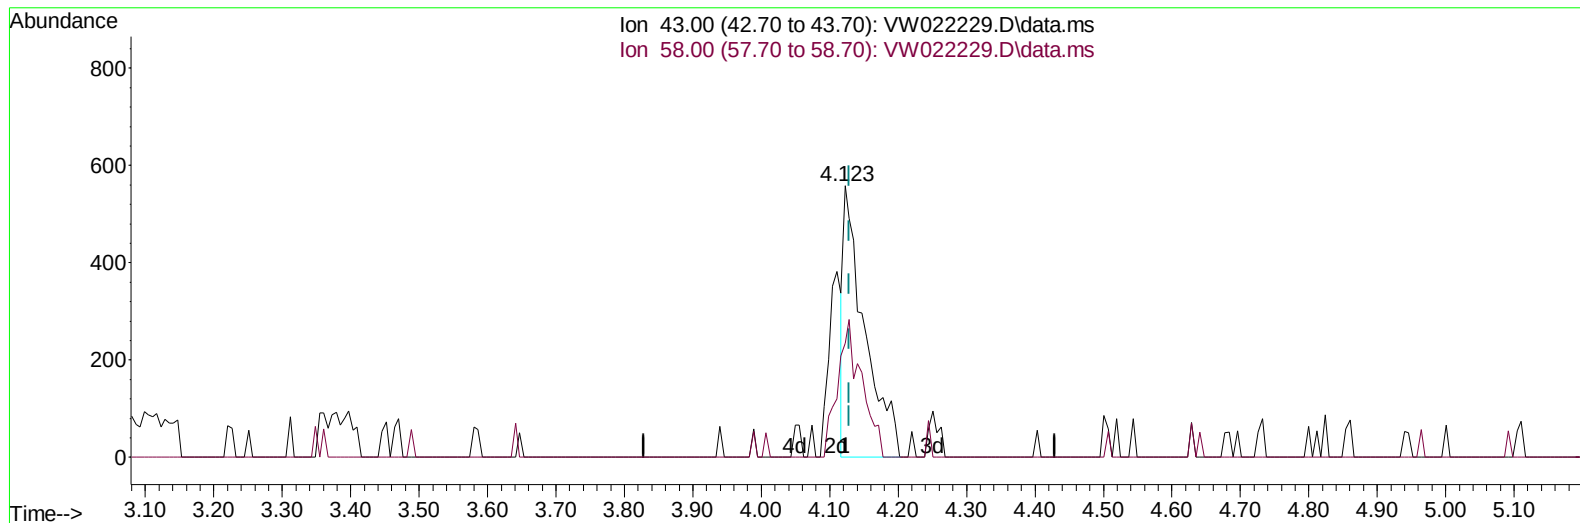

TIC: VW022229.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 4.83 ug/L

response 1175

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	37.19
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022229.D
Acq On : 08 Mar 2022 15:38
Operator : SY/VA
Sample : N1816-19
Misc : 6.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSE4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/11/2022

Quant Time: Mar 09 00:26:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

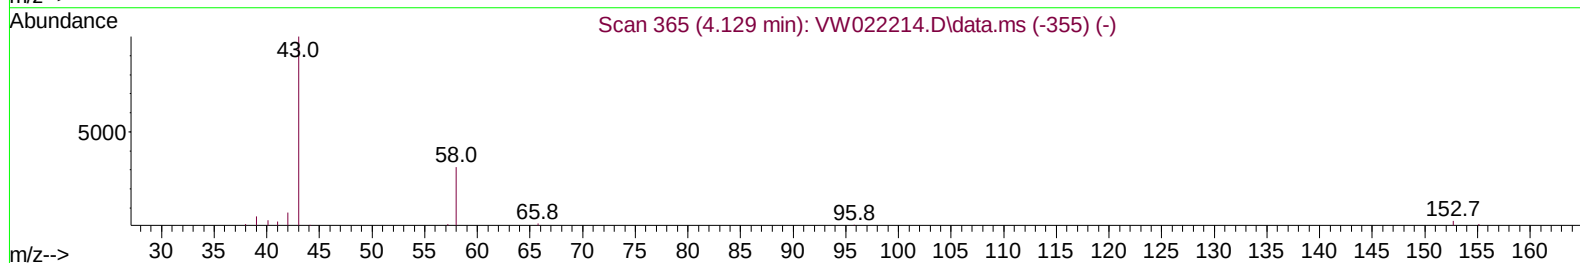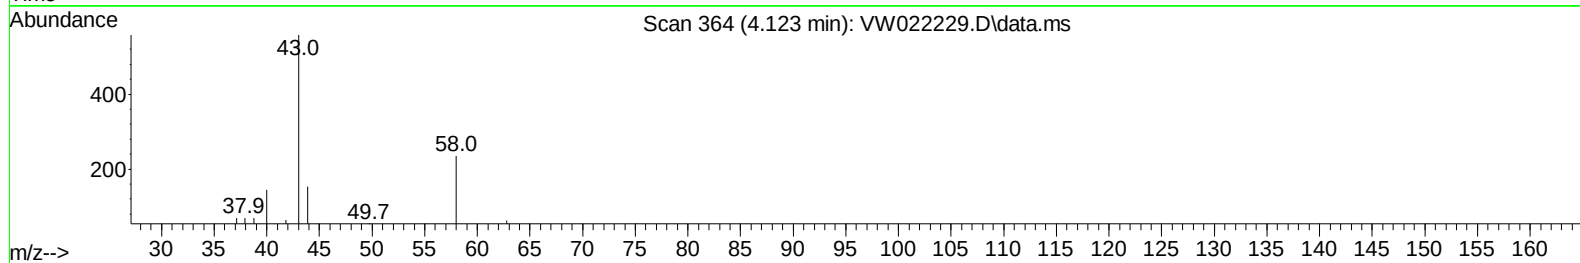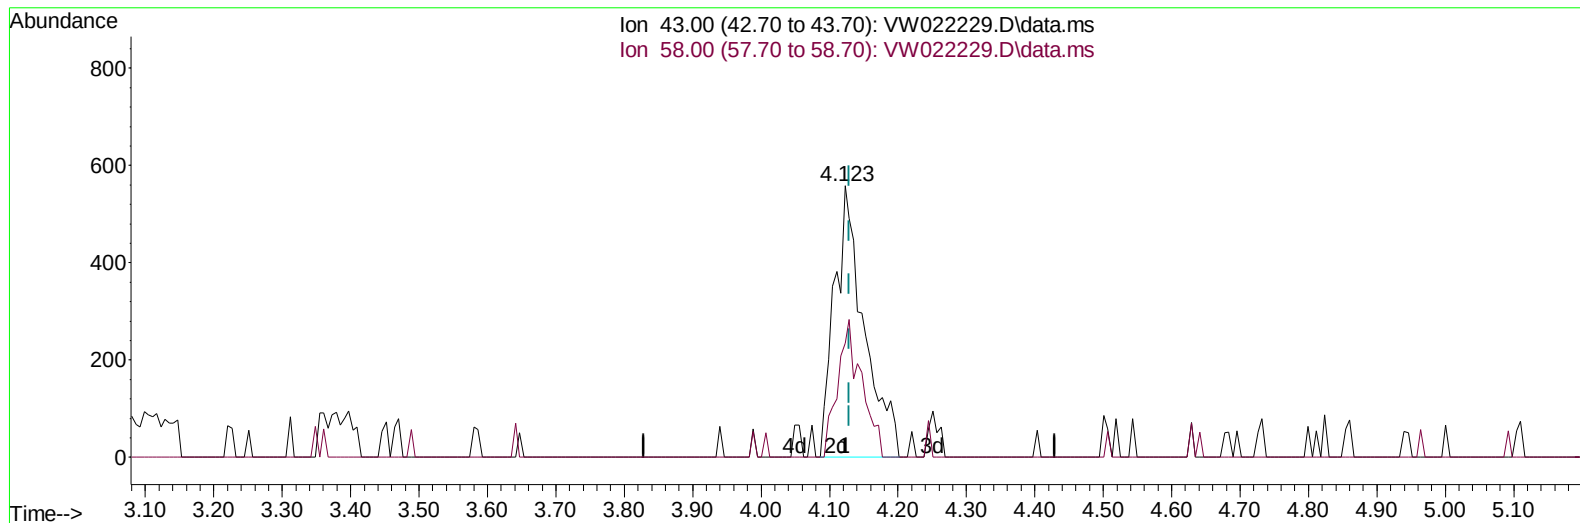

TIC: VW022229.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 6.90 ug/L m

response 1678

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	26.04
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022229.D
 Acq On : 08 Mar 2022 15:38
 Operator : SY/VA
 Sample : N1816-19
 Misc : 6.97g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSE4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

Quant Time: Mar 09 00:26:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	135781	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	131745	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	68060	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	21251	11.999	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	48.000%	
7) Chloroethane-d5	2.879	69	22208	15.937	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.760%	
11) 1,1-Dichloroethene-d2	4.013	63	27579	10.169	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	40.680%#	
21) 2-Butanone-d5	7.073	46	23719	79.656	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	159.320%#	
24) Chloroform-d	7.646	84	62711	20.700	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.800%	
26) 1,2-Dichloroethane-d4	8.305	65	35776	22.719	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.880%	
32) Benzene-d6	8.274	84	105965	17.282	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	69.120%	
36) 1,2-Dichloropropane-d6	9.274	67	34791	20.432	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	81.720%	
41) Toluene-d8	10.323	98	97614	16.014	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	64.040%	
43) trans-1,3-Dichloroprop...	10.579	79	13492	17.871	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.480%	
47) 2-Hexanone-d5	10.920	63	20093	71.747	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	143.500%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	44045	29.474	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	117.880%	
66) 1,2-Dichlorobenzene-d4	13.853	152	46534	21.287	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	85.160%	
Target Compounds						
13) Acetone	4.123	43	1678m	6.900	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022229.D
Acq On : 08 Mar 2022 15:38
Operator : SY/VA
Sample : N1816-19
Misc : 6.97g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSE4

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:26:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/11/2022

