




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022230.D
 Acq On : 08 Mar 2022 16:02
 Operator : SY/VA
 Sample : N1816-21
 Misc : 7.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSE6

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:27:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

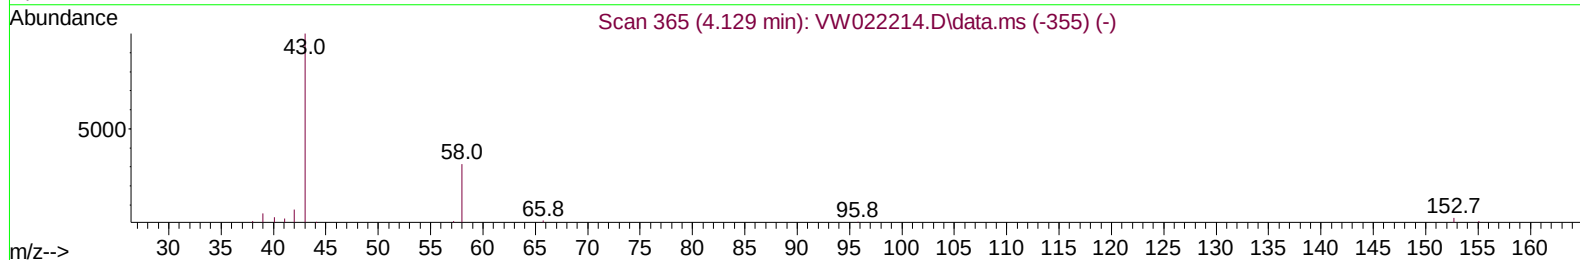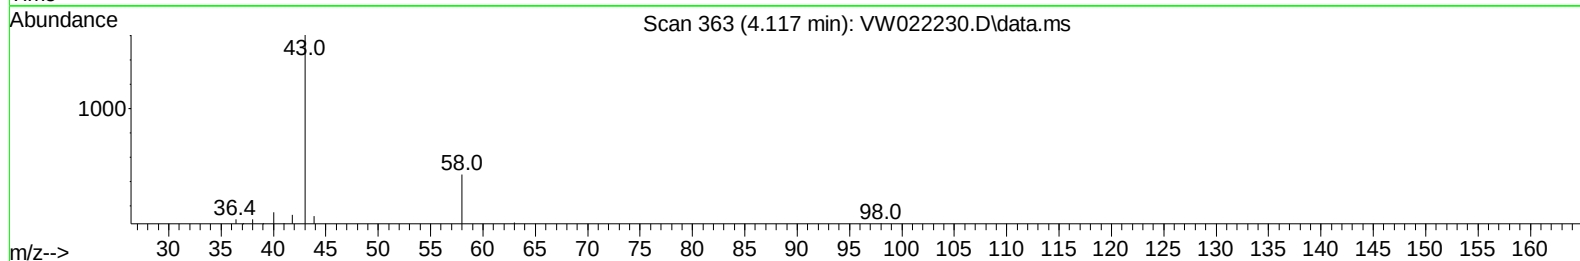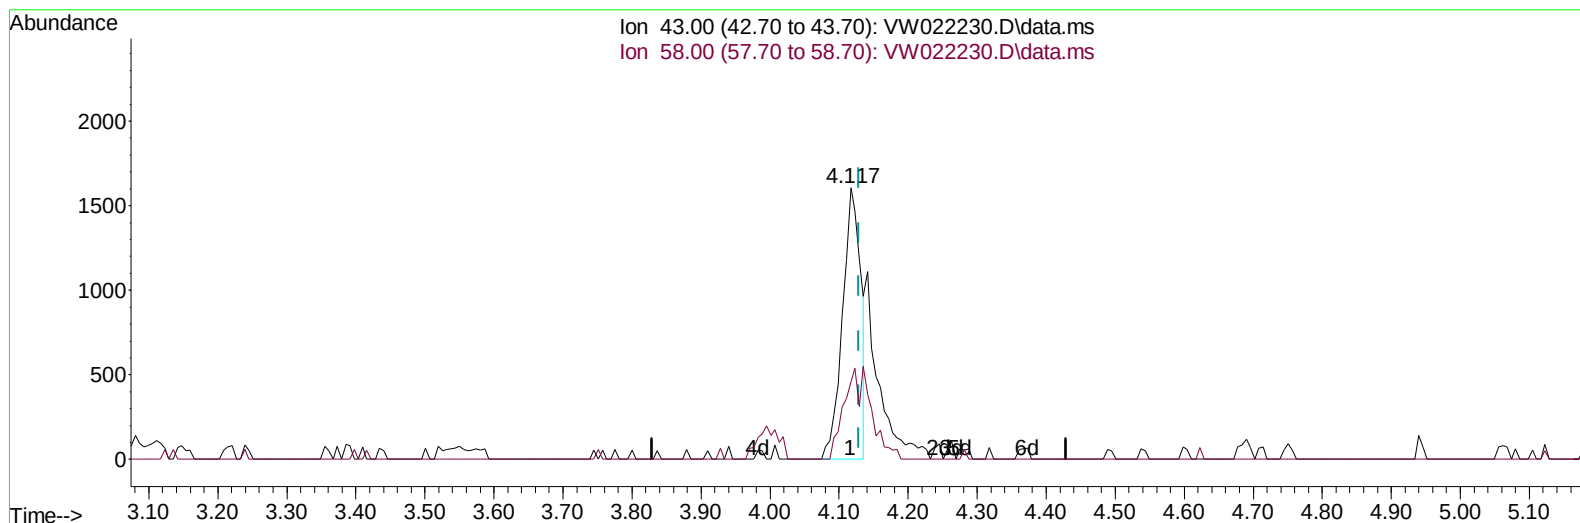

TIC: VW022230.D\data.ms

(13) Acetone (T)

4.117min (-0.012) 10.64 ug/L

response 2978

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	27.87
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022230.D
 Acq On : 08 Mar 2022 16:02
 Operator : SY/VA
 Sample : N1816-21
 Misc : 7.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSE6

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:27:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

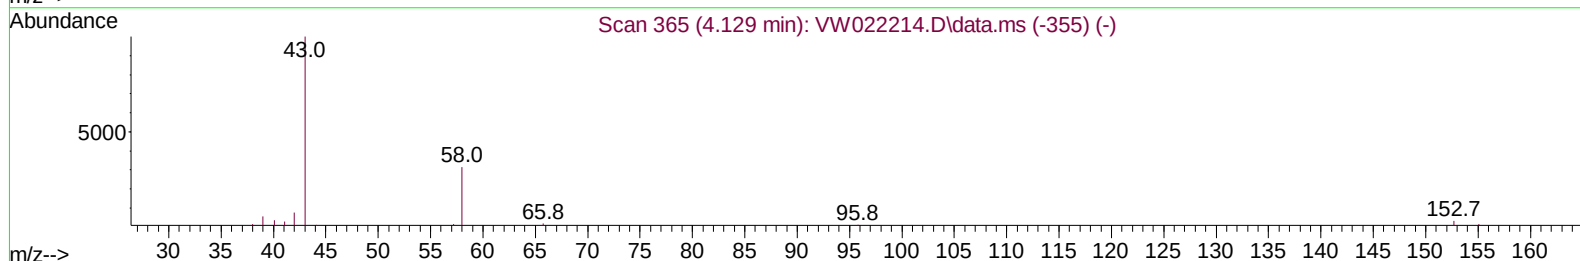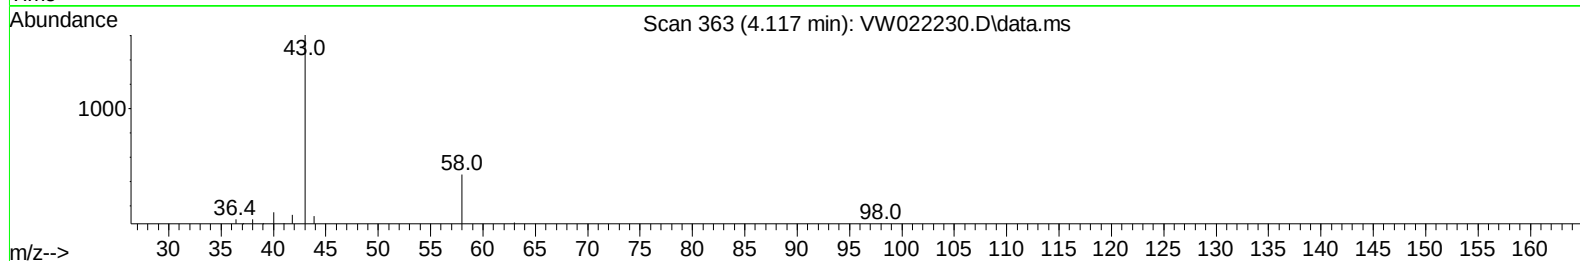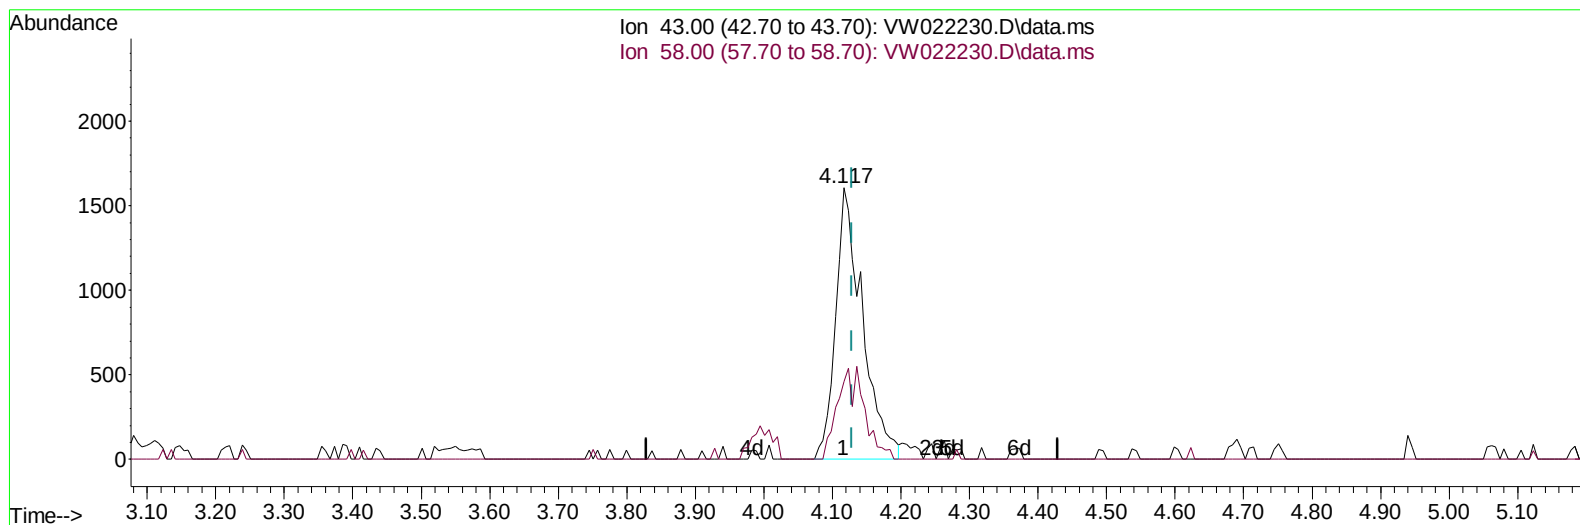

TIC: VW022230.D\data.ms

(13) Acetone (T)

4.117min (-0.012) 15.46 ug/L m

response 4326

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	34.60	19.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022230.D
 Acq On : 08 Mar 2022 16:02
 Operator : SY/VA
 Sample : N1816-21
 Misc : 7.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSE6

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:27:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	156234	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	148240	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	78445	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	26552	13.030	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	52.120%	
7) Chloroethane-d5	2.879	69	27238	16.988	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.960%	
11) 1,1-Dichloroethene-d2	4.013	63	32832	10.521	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	42.080%#	
21) 2-Butanone-d5	7.074	46	21230	61.963	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	123.920%	
24) Chloroform-d	7.647	84	74246	21.300	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	85.200%	
26) 1,2-Dichloroethane-d4	8.305	65	38074	21.013	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	84.040%	
32) Benzene-d6	8.275	84	121653	17.633	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	70.520%	
36) 1,2-Dichloropropane-d6	9.274	67	39684	20.712	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	82.840%	
41) Toluene-d8	10.323	98	111554	16.264	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	65.040%	
43) trans-1,3-Dichloroprop...	10.573	79	14711	17.317	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	69.280%	
47) 2-Hexanone-d5	10.920	63	17389	55.182	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	110.360%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	43001	25.574	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	102.280%	
66) 1,2-Dichlorobenzene-d4	13.853	152	51588	20.475	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	81.880%	
Target Compounds					Qvalue	
13) Acetone	4.117	43	4326m	15.459	ug/L	
14) Carbon disulfide	4.379	76	6706	1.603	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022230.D
Acq On : 08 Mar 2022 16:02
Operator : SY/VA
Sample : N1816-21
Misc : 7.59g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSE6

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:27:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/11/2022

