




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022236.D
Acq On : 08 Mar 2022 18:27
Operator : SY/VA
Sample : N1818-01
Misc : 6.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSE7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/11/2022

Quant Time: Mar 09 00:28:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

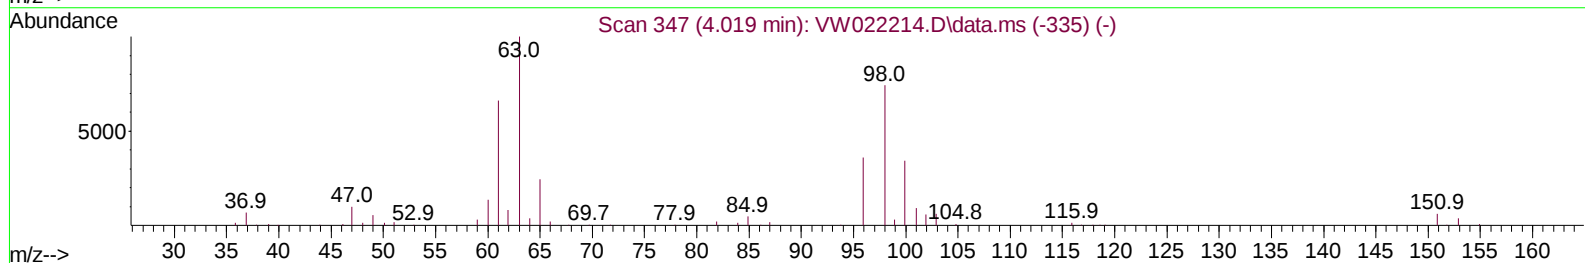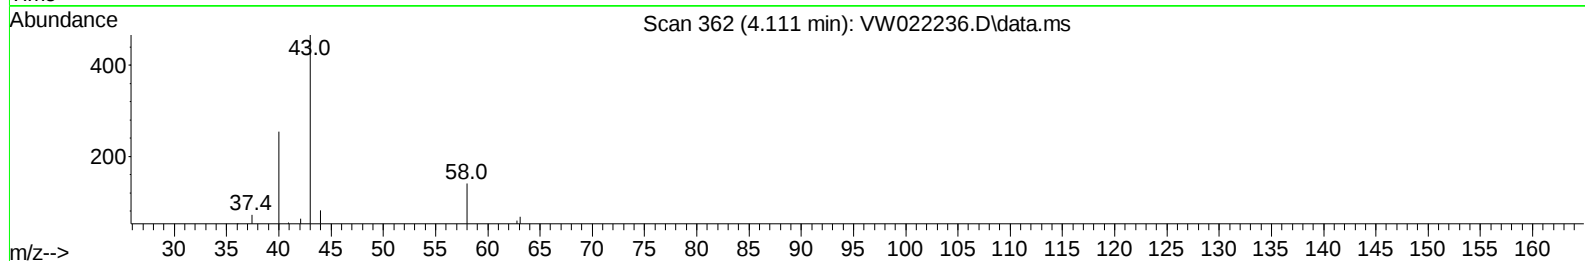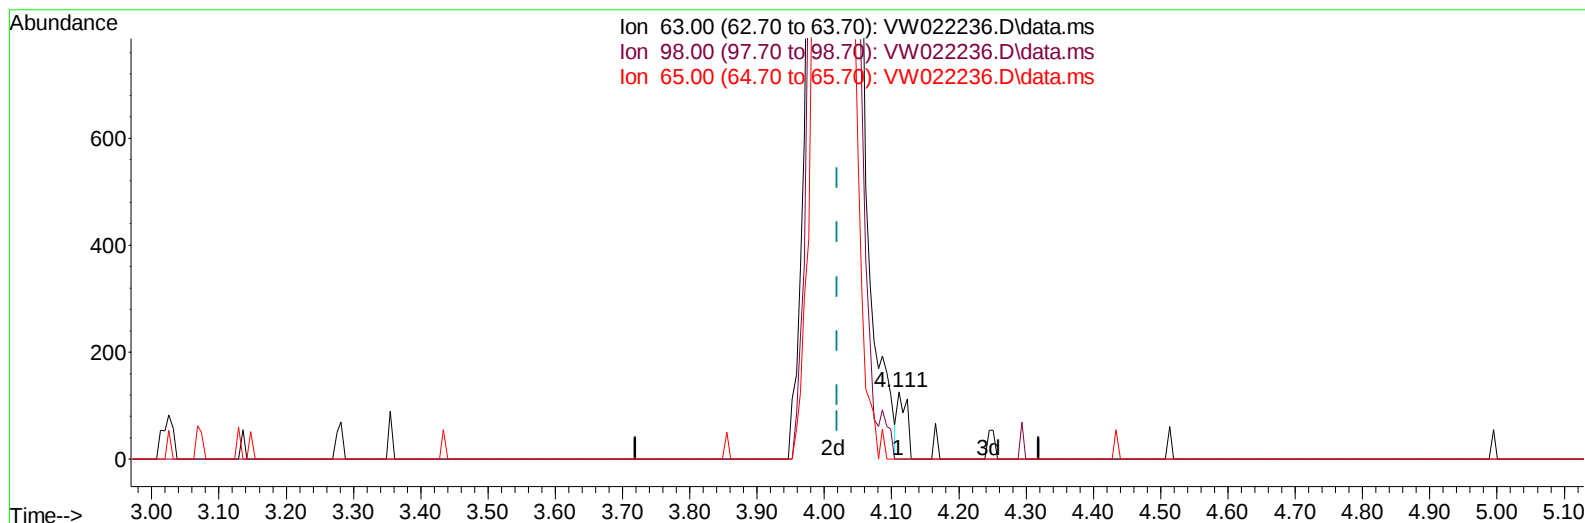

TIC: VW022236.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.111min (+ 0.091) 0.04 ug/L

response 119

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	78.60	64.71
65.00	24.30	17.65
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022236.D
Acq On : 08 Mar 2022 18:27
Operator : SY/VA
Sample : N1818-01
Misc : 6.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSE7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/11/2022

Quant Time: Mar 09 00:28:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

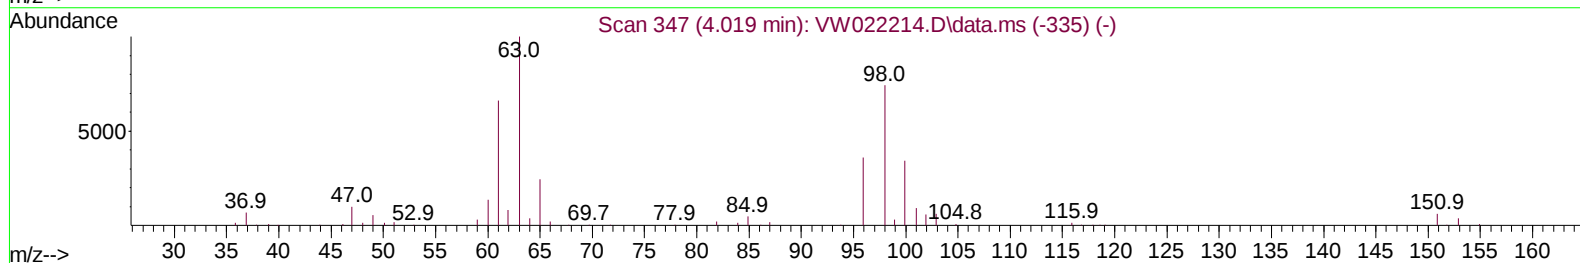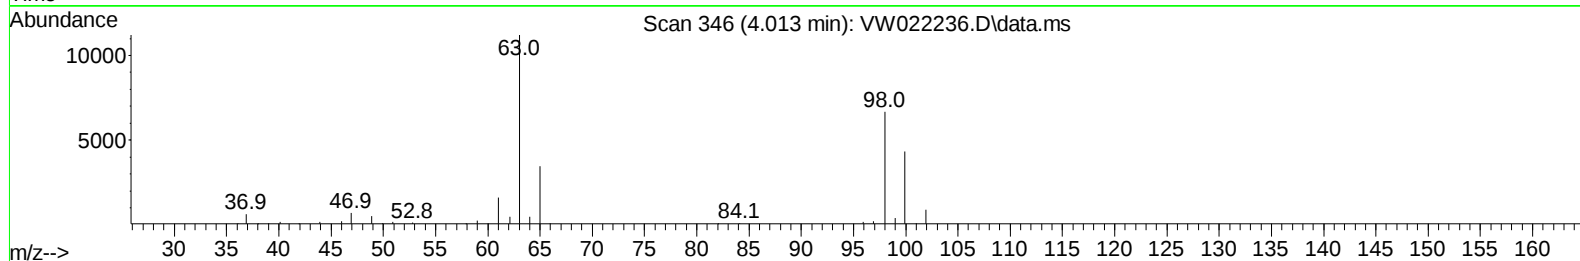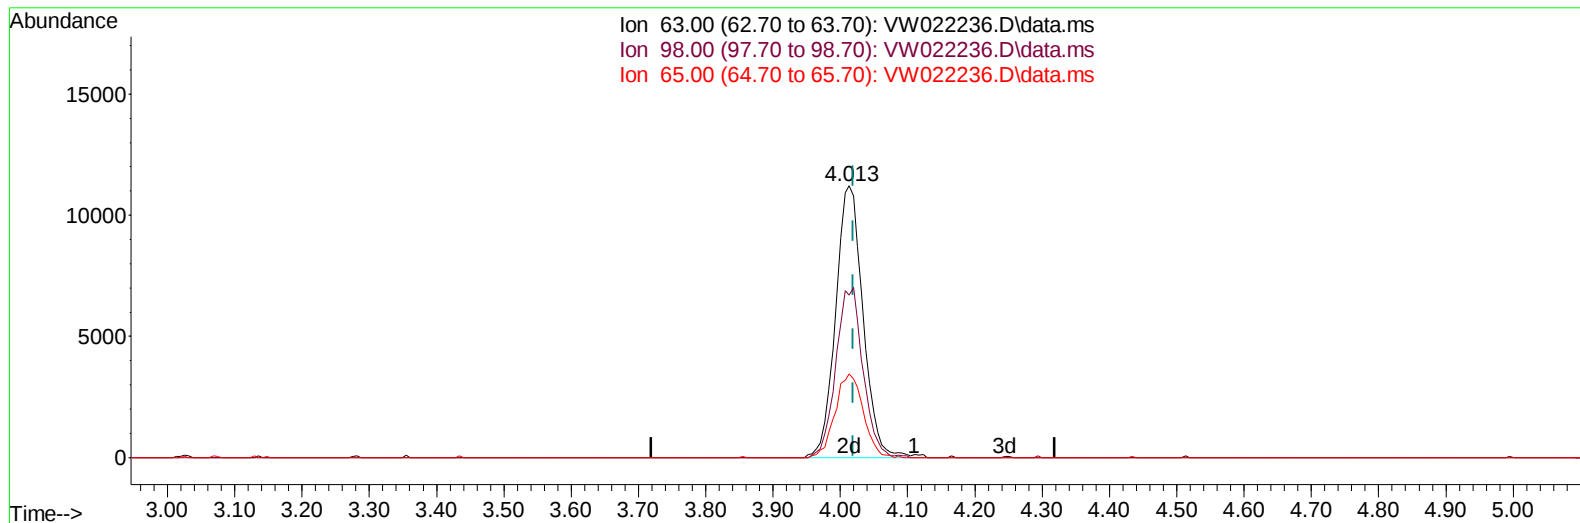

TIC: VW022236.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 10.91 ug/L m

response 31630

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	78.60	0.24#
65.00	24.30	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022236.D
 Acq On : 08 Mar 2022 18:27
 Operator : SY/VA
 Sample : N1818-01
 Misc : 6.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSE7

Manual IntegrationsAPPROVED

Quant Time: Mar 09 00:28:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	145197	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	132337	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	59477	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	23959	12.651	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	50.600%	
7) Chloroethane-d5	2.879	69	24424	16.391	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	65.560%	
11) 1,1-Dichloroethene-d2	4.013	63	31630m	10.906	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	43.640%#	
21) 2-Butanone-d5	7.074	46	23646	74.261	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	148.520%#	
24) Chloroform-d	7.647	84	75981	23.454	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	93.800%	
26) 1,2-Dichloroethane-d4	8.305	65	40659	24.145	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	96.600%	
32) Benzene-d6	8.275	84	125479	20.373	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	81.480%	
36) 1,2-Dichloropropane-d6	9.268	67	41261	24.124	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	96.480%	
41) Toluene-d8	10.323	98	109980	17.961	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	71.840%	
43) trans-1,3-Dichloroprop...	10.579	79	14727	19.419	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	77.680%	
47) 2-Hexanone-d5	10.920	63	19286	68.557	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	137.120%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	44552	29.680	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	118.720%	
66) 1,2-Dichlorobenzene-d4	13.847	152	44110	23.090	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	92.360%	
Target Compounds						
13) Acetone	4.129	43	1820	6.998	ug/L	Qvalue 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022236.D
Acq On : 08 Mar 2022 18:27
Operator : SY/VA
Sample : N1818-01
Misc : 6.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSE7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/11/2022

Quant Time: Mar 09 00:28:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

