

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022218.D
 Acq On : 08 Mar 2022 11:12
 Operator : SY/VA
 Sample : N1816-13
 Misc : 4.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

Quant Time: Mar 09 00:24:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Mar 09 00:23:14 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	160317	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	152616	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	77496	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	25020	11.965	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	47.880%		
7) Chloroethane-d5	2.879	69	25134	15.277	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	61.120%		
11) 1,1-Dichloroethene-d2	4.013	63	33513	10.466	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	41.880%#		
21) 2-Butanone-d5	7.074	46	19263m	54.790	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	109.580%		
24) Chloroform-d	7.647	84	74123	20.723	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.880%		
26) 1,2-Dichloroethane-d4	8.305	65	38559	20.738	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	82.960%		
32) Benzene-d6	8.275	84	125768	17.707	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	70.840%		
36) 1,2-Dichloropropane-d6	9.274	67	40646	20.606	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	82.440%		
41) Toluene-d8	10.323	98	117239	16.603	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	66.400%		
43) trans-1,3-Dichloroprop...	10.579	79	14474	16.550	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	66.200%		
47) 2-Hexanone-d5	10.920	63	15690	48.363	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.720%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	40341	23.304	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.200%		
66) 1,2-Dichlorobenzene-d4	13.847	152	52706	21.175	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.680%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	1401m	4.879	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
Data File : VW022218.D
Acq On : 08 Mar 2022 11:12
Operator : SY/VA
Sample : N1816-13
Misc : 4.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DBSD8

Quant Time: Mar 09 00:24:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Mar 09 00:23:14 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/10/2022
Supervised By :Mahesh Dadoda 03/11/2022

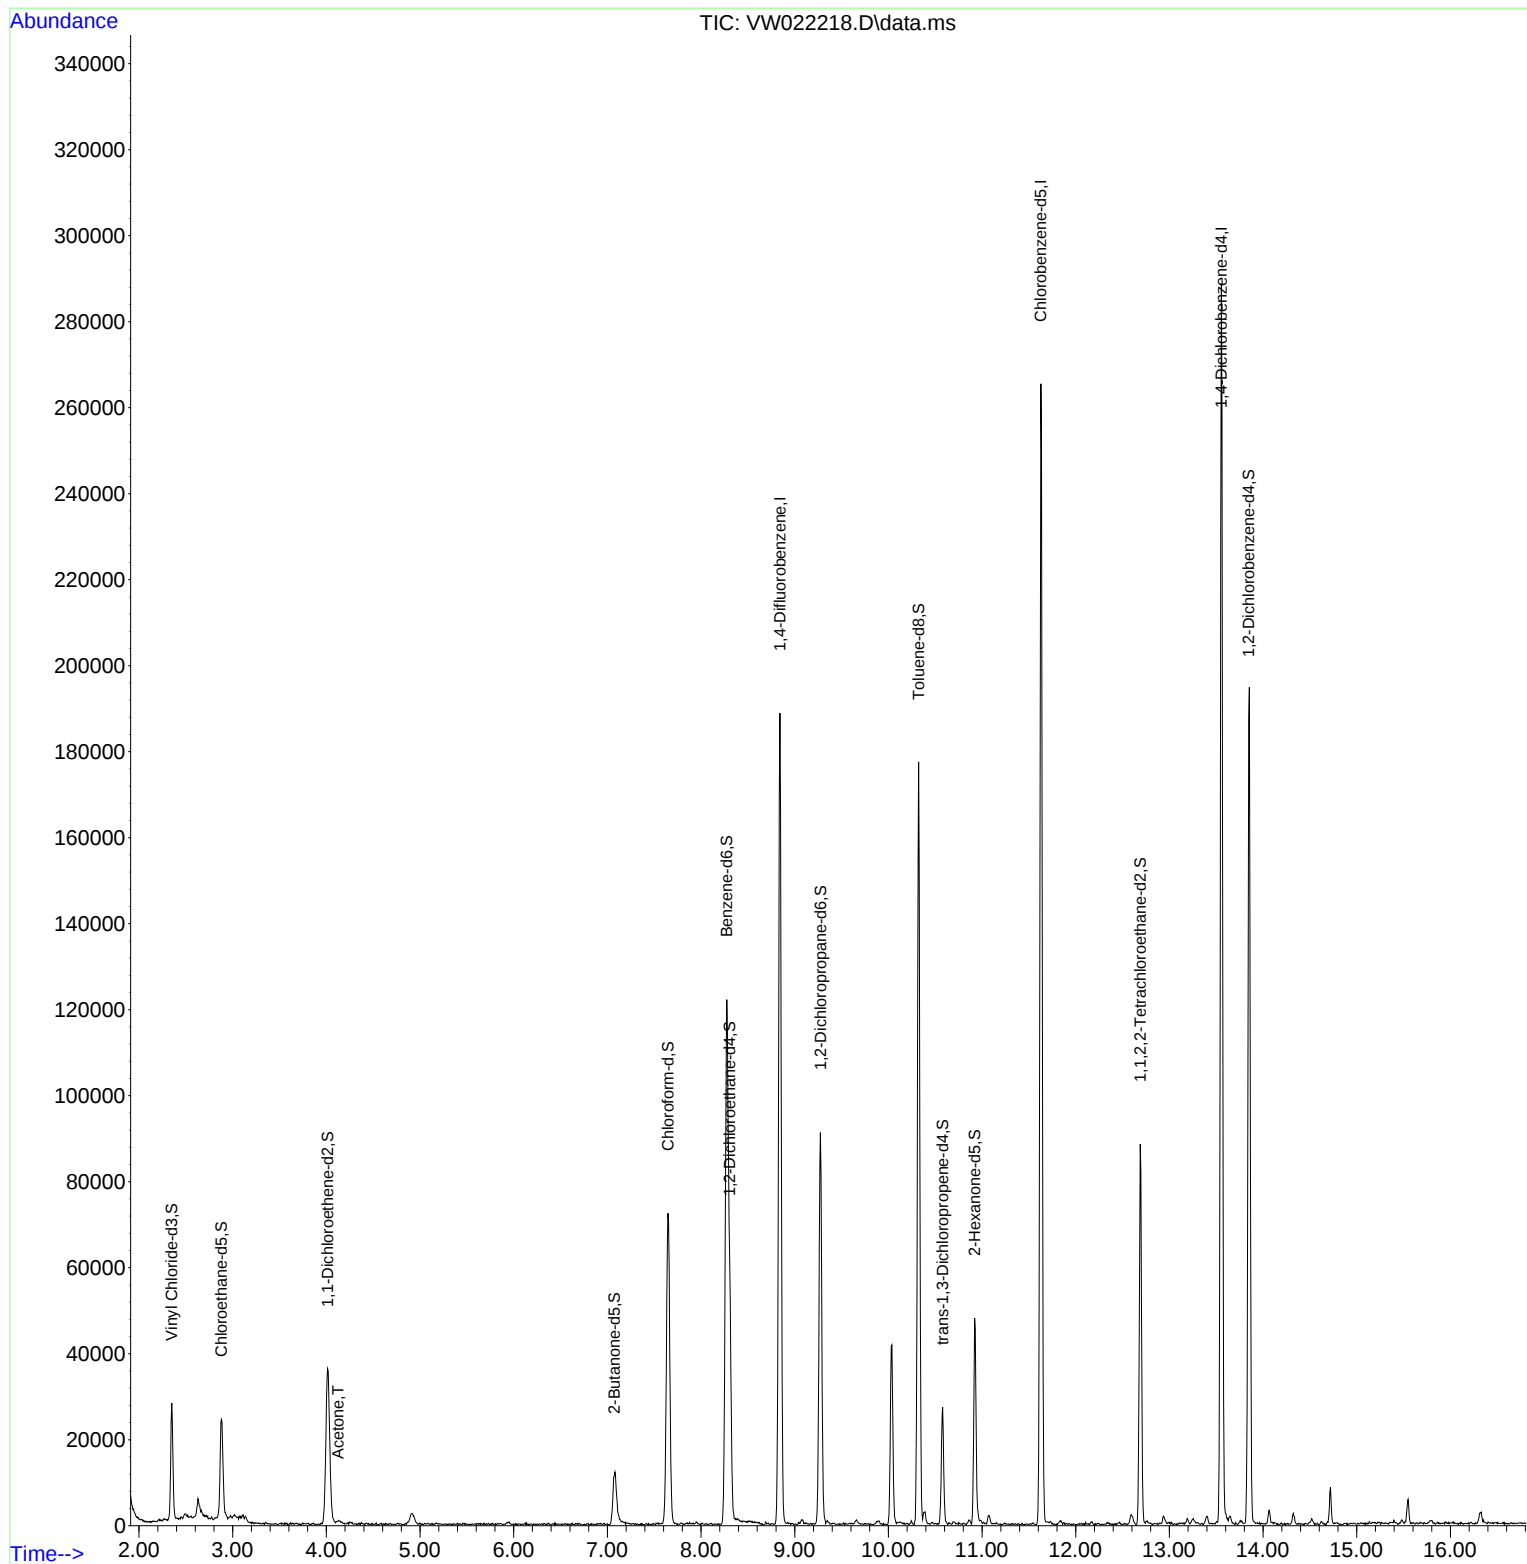

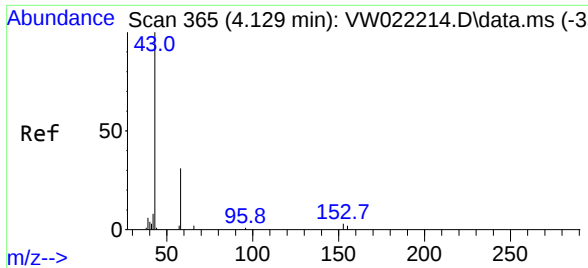

#13
 Acetone
 Concen: 4.879 ug/L m
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW022218.D
 Acq: 08 Mar 2022 11:12

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSD8

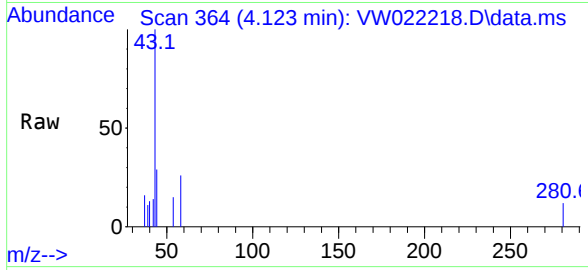

Tgt Ion: 43 Resp: 140

Ion	Ratio	Lower	Upper
43	100		
58	26.1	0.0	69.2

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/10/2022
 Supervised By :Mahesh Dadoda 03/11/2022

