
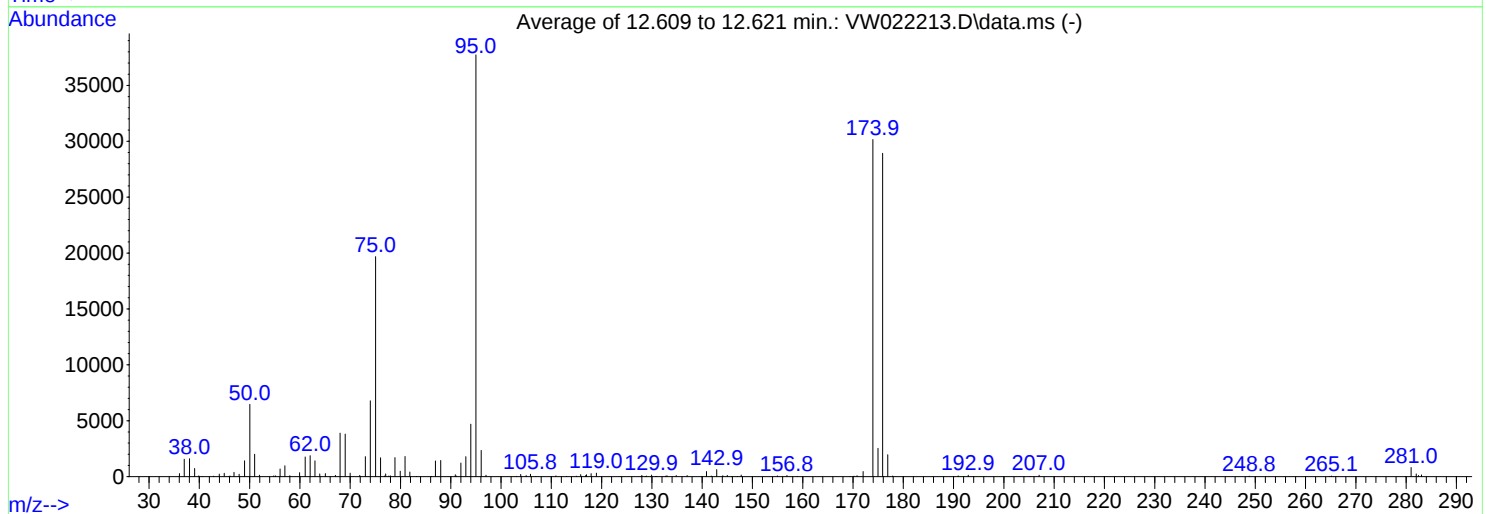


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030822\
 Data File : VW022213.D
 Acq On : 08 Mar 2022 08:28
 Operator : SY/VA
 Sample : BFB518
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB518

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Title : SFAM01.0
 Last Update : Fri Mar 11 03:07:48 2022

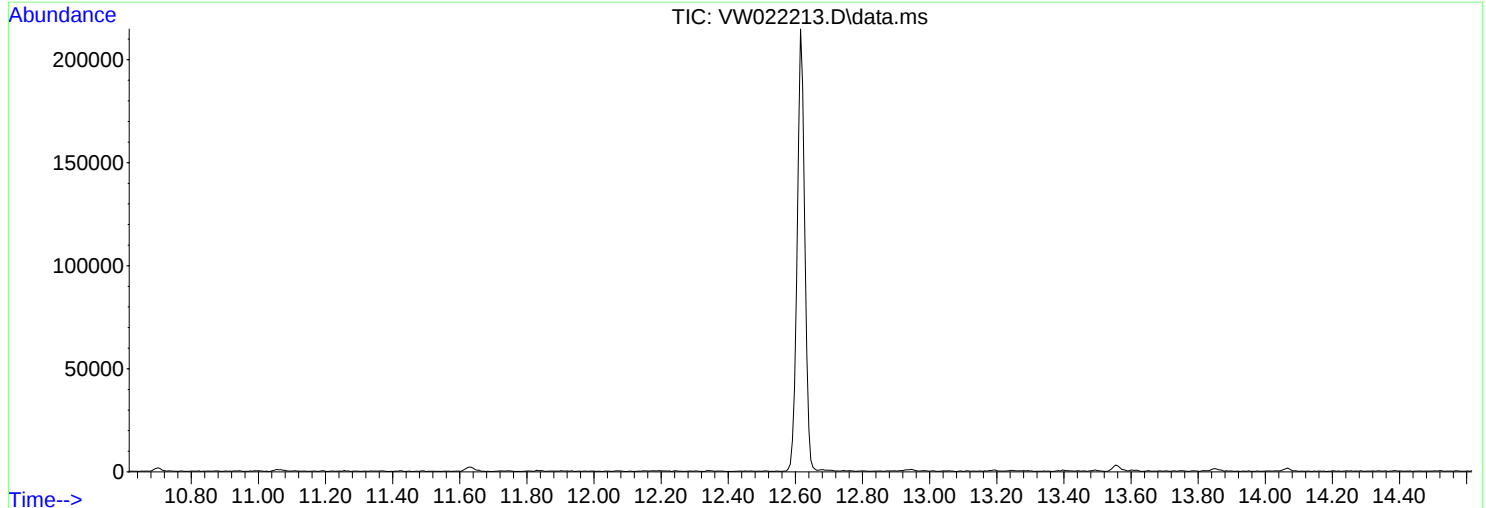

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	6464	PASS
75	95	30	80	52.1	19675	PASS
95	95	100	100	100.0	37731	PASS
96	95	5	9	6.2	2346	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.9	30163	PASS
175	174	5	9	8.4	2540	PASS
176	174	95	105	95.9	28923	PASS
177	176	5	10	6.8	1964	PASS

m/z	Abundance
36.10	76.0
39.90	146.0
44.00	93.0
57.00	75.0

Instrument :
MSVOA_W
ClientSampleId :
BFB518

m/z	Abundance
36.10	295.0
37.00	1377.0
38.00	1213.0
39.00	709.0
40.00	189.0
42.80	84.0
44.00	301.0
45.00	329.0
45.90	79.0
46.90	335.0
47.90	275.0
49.00	1189.0
50.10	6058.0
51.00	1708.0
51.90	97.0
54.90	112.0
56.10	774.0
57.00	1020.0
57.90	85.0
59.90	344.0
61.00	1507.0
62.10	1754.0
63.00	1578.0
64.10	260.0
65.00	244.0
67.00	121.0
68.00	3268.0
69.00	3582.0
70.00	273.0
71.90	186.0
73.00	1704.0
74.00	6159.0
75.00	17680.0
76.00	1613.0
76.80	167.0
77.20	166.0
78.00	91.0
78.90	1605.0
80.00	431.0
80.90	1521.0
81.90	449.0
86.20	91.0
86.90	1117.0
88.00	1000.0
90.90	240.0
92.00	1081.0
93.00	1802.0
94.00	4194.0
95.00	32984.0
96.00	2052.0
97.10	77.0
103.10	95.0
104.00	134.0
105.10	69.0
105.90	200.0
110.90	60.0
115.00	64.0
115.90	183.0
116.80	275.0
117.80	254.0
118.90	390.0
127.80	63.0
128.70	62.0
129.80	110.0
132.70	113.0
137.00	111.0
140.90	376.0
142.90	503.0
144.10	89.0
144.90	112.0
145.90	84.0
147.00	58.0
147.90	110.0
156.90	51.0
170.20	86.0
170.80	93.0
172.10	379.0
174.00	24088.0
174.90	2160.0
175.90	22536.0
176.90	1488.0
177.90	56.0
190.90	126.0
192.90	206.0
194.00	60.0
205.20	51.0
207.00	128.0
248.80	129.0
264.80	109.0
265.20	87.0
281.00	1101.0
282.10	323.0

Instrument :
MSVOA_W
ClientSampleId :
BFB518

283.10

147.0

Instrument :
MSVOA_W
ClientSampleId :
BFB518

m/z	Abundance
36.00	364.0
37.00	1905.0
38.00	2223.0
39.10	764.0
40.00	251.0
40.60	53.0
42.90	63.0
44.00	330.0
44.90	332.0
46.10	96.0
46.90	393.0
47.90	237.0
49.00	1783.0
50.00	7412.0
51.00	2320.0
52.00	141.0
54.70	93.0
55.20	101.0
56.10	667.0
57.00	1149.0
58.00	89.0
60.00	411.0
61.10	1988.0
62.00	2005.0
63.00	1466.0
63.90	235.0
65.10	243.0
67.10	122.0
68.00	4659.0
69.00	4129.0
70.00	436.0
73.00	2015.0
74.00	7837.0
75.00	22264.0
76.00	1888.0
77.00	381.0
77.70	184.0
78.90	1799.0
79.90	558.0
80.90	2233.0
81.80	359.0
87.00	1745.0
88.00	1357.0
90.90	257.0
92.00	1317.0
93.00	1815.0
94.00	5563.0
95.00	42792.0
96.10	2779.0
97.00	180.0
103.90	266.0
105.00	91.0
105.80	242.0
110.90	67.0
113.00	101.0
115.00	68.0
115.90	191.0
117.00	272.0
117.90	299.0
119.00	308.0
123.70	56.0
128.00	100.0
128.90	89.0
130.00	259.0
131.10	52.0
133.00	114.0
134.90	153.0
137.00	96.0
139.90	55.0
140.80	517.0
141.80	119.0
142.90	772.0
144.10	105.0
145.00	103.0
147.70	129.0
155.00	106.0
156.80	120.0
158.90	101.0
170.20	68.0
170.80	105.0
172.00	434.0
174.00	33720.0
174.90	2581.0
175.90	34976.0
176.90	2111.0
177.90	54.0
190.90	102.0
192.70	95.0
206.90	145.0
265.10	93.0
265.60	59.0
279.80	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB518

281.00	807.0
282.00	272.0
282.40	230.0
283.00	220.0

Instrument :
MSVOA_W
ClientSampleId :
BFB518

m/z	Abundance
36.10	396.0
37.00	1402.0
38.10	1380.0
39.00	722.0
39.90	236.0
43.90	326.0
44.90	236.0
46.10	84.0
46.90	412.0
47.90	142.0
49.00	1301.0
50.10	5921.0
51.00	1991.0
52.00	141.0
55.10	129.0
56.00	617.0
57.00	999.0
58.10	88.0
59.90	303.0
61.00	1811.0
62.00	1853.0
63.00	1203.0
63.90	218.0
65.00	317.0
67.00	119.0
68.00	3750.0
69.00	3731.0
70.00	223.0
71.90	184.0
73.00	1641.0
74.00	6367.0
75.10	19080.0
76.10	1570.0
77.00	207.0
78.00	123.0
78.90	1729.0
80.00	483.0
80.90	1654.0
81.90	440.0
83.20	55.0
86.90	1332.0
87.80	1021.0
88.10	960.0
91.10	167.0
92.00	1239.0
93.00	1770.0
94.00	4352.0
95.00	37416.0
96.00	2206.0
96.90	146.0
103.80	209.0
104.90	132.0
105.90	196.0
106.90	51.0
110.90	107.0
115.80	189.0
117.00	247.0
118.00	245.0
118.90	258.0
128.00	257.0
129.00	96.0
129.90	172.0
130.70	53.0
130.90	54.0
133.00	137.0
134.80	130.0
137.00	97.0
140.90	490.0
141.80	55.0
142.90	604.0
144.00	60.0
145.10	112.0
147.70	176.0
154.90	131.0
156.80	118.0
169.40	62.0
170.70	63.0
171.90	549.0
173.90	32680.0
175.00	2879.0
175.90	29256.0
176.90	2292.0
177.90	59.0
193.00	70.0
207.10	109.0
281.10	549.0
281.90	123.0
282.50	83.0
283.00	105.0

Instrument :
MSVOA_W
ClientSampleId :
BFB518