

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030823\
 Data File : VW025381.D
 Acq On : 08 Mar 2023 12:38
 Operator : SY/MD
 Sample : 01838-01
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1168




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/09/2023
 Supervised By :Mahesh Dadoda 03/09/2023

Supervised By :Mahesh
 Dadoda

03/09/2023

Quant Time: Mar 09 01:01:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 07 05:10:09 2023
 Response via : Initial Calibration

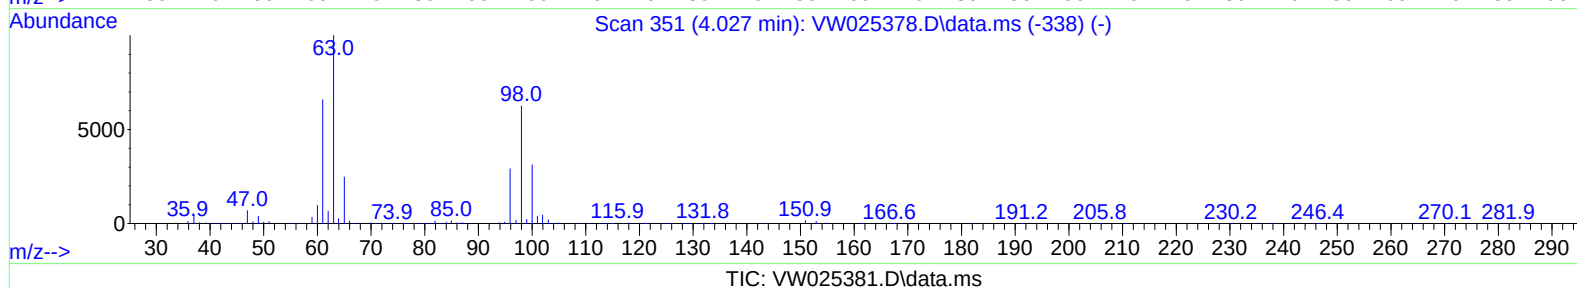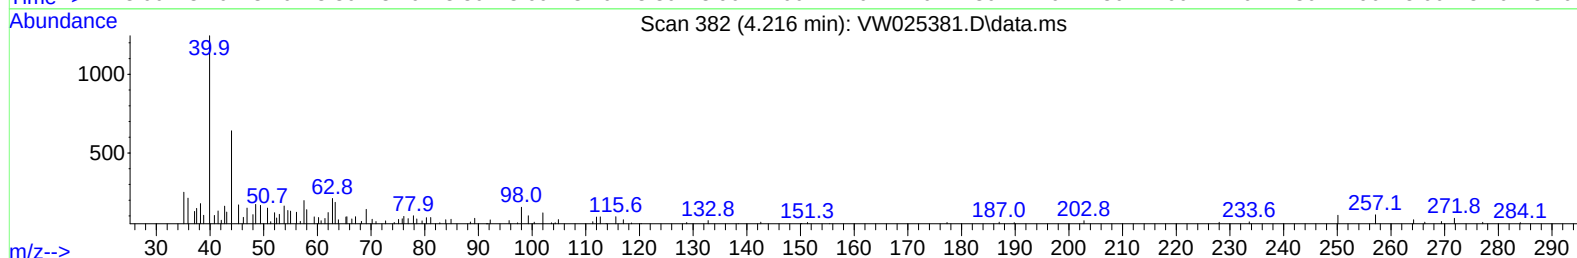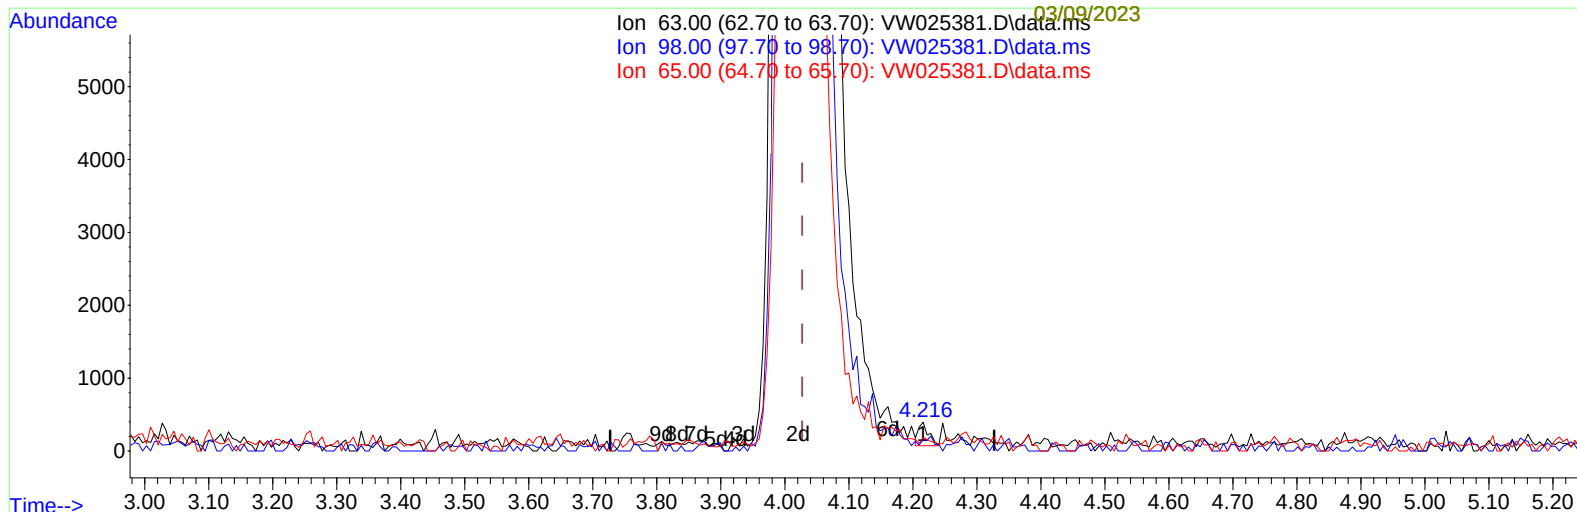

TIC: VW025381.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.216min (+ 0.189) 0.01 ug/L

response 346

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	73.41
65.00	23.70	21.39
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030823\
 Data File : VW025381.D
 Acq On : 08 Mar 2023 12:38
 Operator : SY/MD
 Sample : 01838-01
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1168




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/09/2023
 Supervised By :Mahesh Dadoda 03/09/2023

Supervised By :Mahesh
 Dadoda

03/09/2023

Quant Time: Mar 09 01:01:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 07 05:10:09 2023
 Response via : Initial Calibration

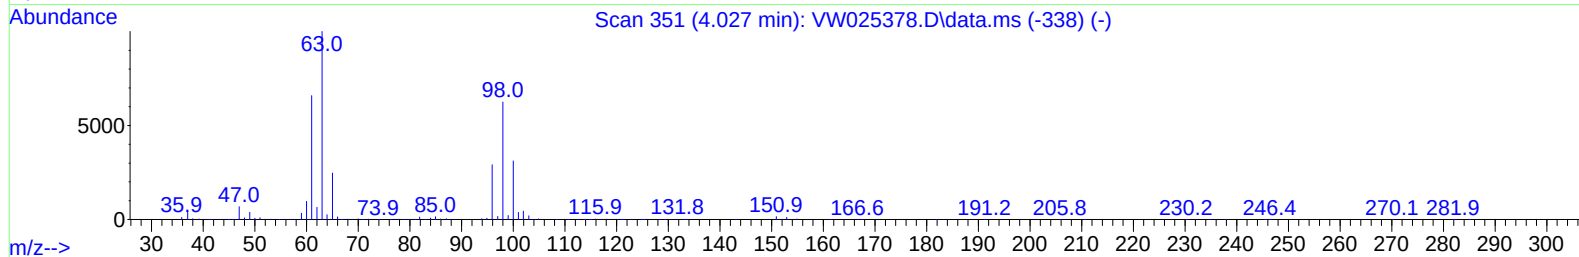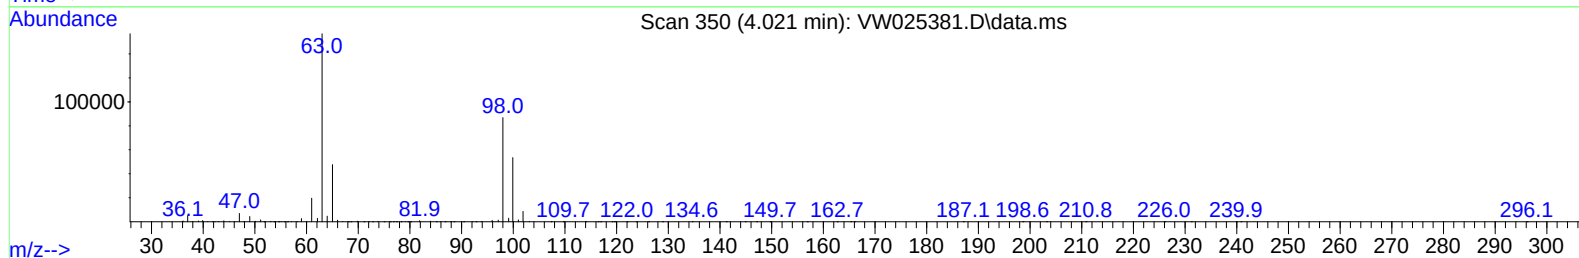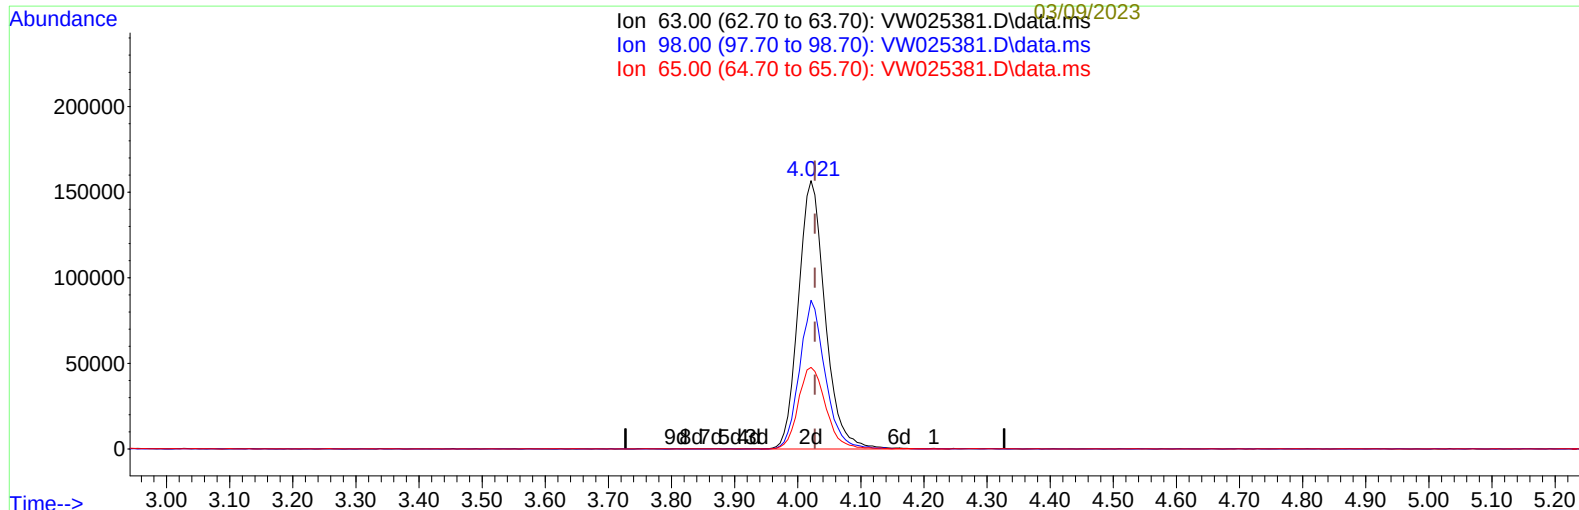

TIC: VW025381.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.006) 14.02 ug/L m

response 462116

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	0.05#
65.00	23.70	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030823\
 Data File : VW025381.D
 Acq On : 08 Mar 2023 12:38
 Operator : SY/MD
 Sample : 01838-01
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1168

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/09/2023
 Supervised By :Mahesh Dadoda 03/09/2023

Supervised By :Mahesh
 Dadoda
 03/09/2023

Quant Time: Mar 09 01:01:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Mar 07 05:10:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	1026572	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	860871	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	334370	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	300858	17.626	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.520%		
7) Chloroethane-d5	2.899	69	219817	17.898	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	71.600%		
11) 1,1-Dichloroethene-d2	4.021	63	462116m	14.017	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.080%		
21) 2-Butanone-d5	7.075	46	137448	32.806	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	65.620%		
24) Chloroform-d	7.648	84	554155	18.725	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	74.880%		
26) 1,2-Dichloroethane-d4	8.301	65	302895	19.069	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	76.280%		
32) Benzene-d6	8.276	84	1169900	19.889	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	79.560%		
36) 1,2-Dichloropropane-d6	9.276	67	367371	20.188	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	80.760%		
41) Toluene-d8	10.325	98	988418	19.058	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	76.240%		
43) trans-1,3-Dichloroprop...	10.581	79	130249	17.975	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.880%		
47) 2-Hexanone-d5	10.922	63	86427	33.029	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	66.060%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	228177	17.115	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	68.480%		
66) 1,2-Dichlorobenzene-d4	13.855	152	241194	19.397	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	77.600%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030823\
Data File : VW025381.D
Acq On : 08 Mar 2023 12:38
Operator : SY/MD
Sample : 01838-01
Misc : 5.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C1168

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/09/2023
Supervised By :Mahesh Dadoda 03/09/2023

Supervised By :Mahesh
Dadoda
03/09/2023

Quant Time: Mar 09 01:01:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Mar 07 05:10:09 2023
Response via : Initial Calibration

