
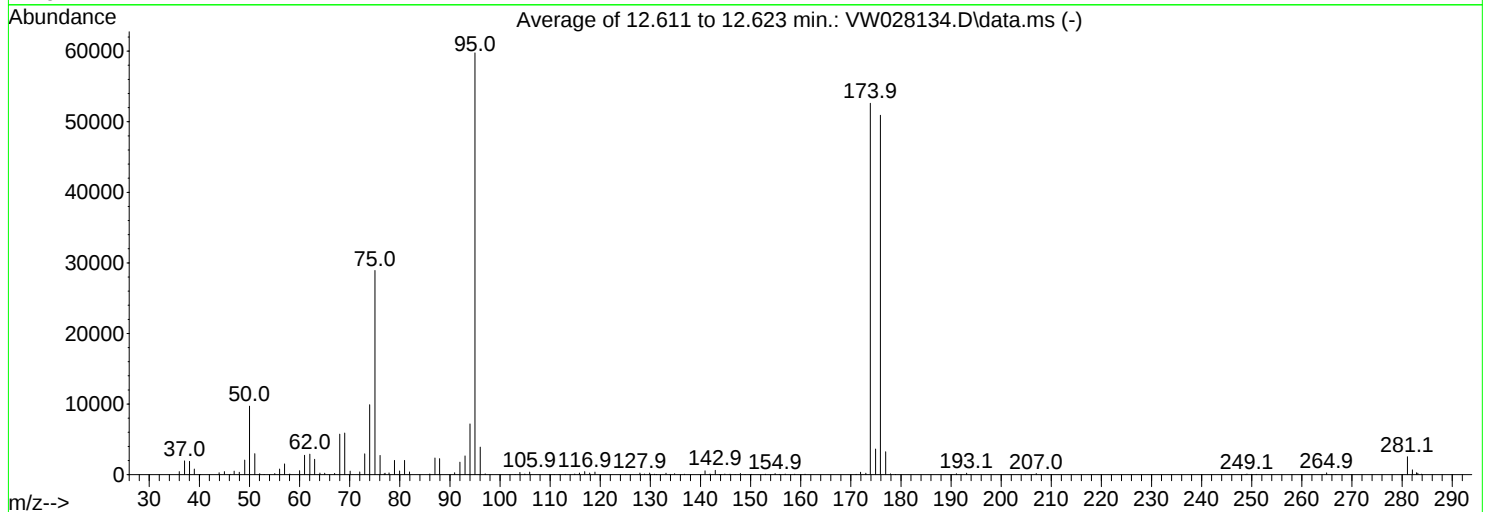


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW030824\
Data File : VW028134.D
Acq On : 08 Mar 2024 08:04
Operator : SY/MD
Sample : BFB449
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB449

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022924SMA.M
Title : SFAM01.0
Last Update : Fri Mar 08 22:41:29 2024

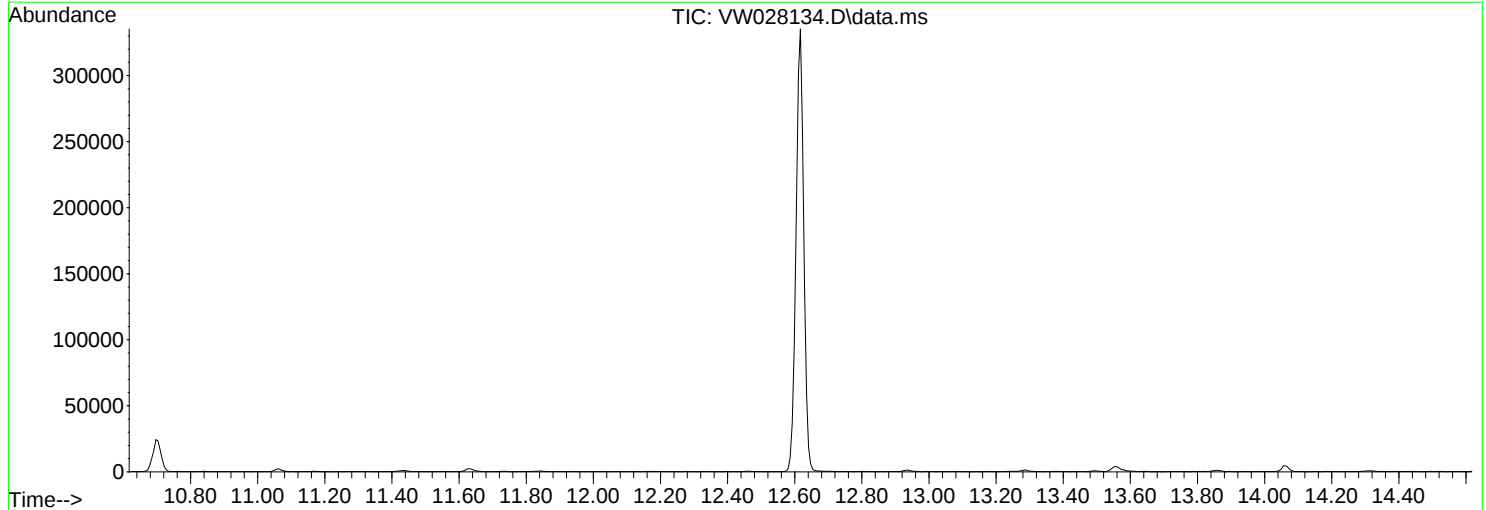

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	9698	PASS
75	95	30	80	48.4	28920	PASS
95	95	100	100	100.0	59760	PASS
96	95	5	9	6.5	3901	PASS
173	174	0.00	2	0.4	200	PASS
174	95	50	120	88.1	52621	PASS
175	174	5	9	6.9	3636	PASS
176	174	95	101	96.8	50920	PASS
177	176	5	9	6.3	3232	PASS

m/z	Abundance
40.10	143.0
43.80	114.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

m/z	Abundance
36.00	510.0
37.10	2144.0
38.10	2136.0
39.00	903.0
39.90	154.0
44.00	415.0
45.00	446.0
46.10	56.0
46.90	455.0
48.00	429.0
49.00	2189.0
50.00	10680.0
51.00	3125.0
52.00	154.0
52.90	60.0
55.00	170.0
56.00	879.0
57.00	1561.0
58.00	106.0
60.00	685.0
61.00	2725.0
62.10	2864.0
63.00	2512.0
64.00	277.0
65.00	239.0
67.00	191.0
68.00	6235.0
69.00	6129.0
70.10	567.0
72.00	382.0
73.00	2956.0
74.00	10715.0
75.10	32200.0
76.10	2810.0
76.90	344.0
77.80	194.0
78.90	2148.0
79.90	515.0
80.90	2212.0
82.00	360.0
85.90	104.0
87.00	2414.0
87.90	2057.0
90.90	329.0
92.00	1802.0
93.00	2638.0
94.00	7914.0
95.00	61816.0
96.00	4072.0
97.10	169.0
103.00	82.0
104.00	343.0
105.00	141.0
105.90	360.0
110.80	54.0
113.00	71.0
114.90	111.0
115.90	211.0
117.00	412.0
117.90	211.0
118.90	449.0
125.10	69.0
127.90	265.0
128.80	100.0
129.90	191.0
131.20	88.0
133.10	331.0
133.90	128.0
134.80	113.0
136.80	54.0
140.90	480.0
142.00	102.0
143.00	596.0
144.10	57.0
144.90	111.0
145.90	78.0
147.90	160.0
148.90	64.0
149.90	73.0
153.00	68.0
154.90	216.0
156.90	55.0
158.90	117.0
160.80	90.0
171.10	66.0
172.00	412.0
173.90	49936.0
175.00	3643.0
175.90	41832.0
177.00	3495.0
177.90	134.0
178.90	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

191.00	316.0
192.00	105.0
193.10	345.0
193.90	88.0
204.80	56.0
207.00	219.0
207.90	69.0
249.00	185.0
250.00	130.0
250.90	122.0
265.00	474.0
265.90	81.0
266.80	79.0
281.00	4565.0
282.10	1008.0
282.90	832.0
283.90	203.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

m/z	Abundance
36.00	435.0
37.10	2087.0
38.10	1946.0
39.00	887.0
39.90	149.0
44.00	417.0
45.00	405.0
46.20	52.0
47.00	658.0
47.90	306.0
49.00	2305.0
50.00	10588.0
51.00	3309.0
52.10	143.0
55.10	171.0
56.00	906.0
57.00	1641.0
58.00	85.0
60.00	629.0
61.00	3182.0
62.00	3377.0
63.00	2316.0
64.10	209.0
65.00	221.0
67.00	219.0
68.00	6180.0
69.00	6596.0
70.10	652.0
72.00	488.0
73.00	3177.0
74.00	10723.0
75.00	31136.0
76.00	3181.0
77.10	349.0
77.80	329.0
79.00	2344.0
80.00	559.0
81.00	2248.0
82.00	454.0
86.00	126.0
87.00	2792.0
88.00	2741.0
90.90	238.0
92.00	2065.0
93.00	2906.0
94.00	7626.0
95.00	65080.0
96.10	4438.0
97.00	114.0
103.90	303.0
104.90	136.0
105.90	324.0
109.90	89.0
111.80	105.0
113.00	62.0
114.90	107.0
115.80	265.0
116.90	502.0
118.00	307.0
119.00	412.0
127.90	299.0
128.90	105.0
129.80	266.0
130.90	138.0
133.10	229.0
134.90	171.0
136.80	106.0
140.90	740.0
141.80	90.0
142.90	744.0
143.80	99.0
144.80	84.0
145.90	76.0
146.90	94.0
148.00	176.0
150.10	69.0
152.90	108.0
154.90	195.0
155.80	59.0
157.00	78.0
160.90	70.0
171.00	68.0
171.90	376.0
173.90	60088.0
174.90	4084.0
175.90	63032.0
177.00	3395.0
177.90	112.0
191.10	124.0
193.10	209.0
207.00	208.0
248.70	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

249.10	80.0
264.90	196.0
281.10	2295.0
282.00	671.0
283.10	449.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449

m/z	Abundance
36.00	343.0
37.00	1627.0
38.00	1577.0
39.00	573.0
40.00	137.0
44.00	317.0
45.00	414.0
46.90	385.0
48.00	285.0
49.10	1715.0
50.00	7825.0
51.10	2464.0
52.00	148.0
55.00	158.0
56.00	628.0
57.00	1369.0
58.10	79.0
60.00	387.0
61.00	2329.0
62.10	2463.0
63.00	1669.0
64.00	197.0
64.90	148.0
67.00	132.0
68.00	4821.0
69.00	4992.0
70.00	259.0
72.00	306.0
73.00	2722.0
74.00	8264.0
75.00	23424.0
76.00	2159.0
77.00	297.0
77.90	255.0
78.90	1545.0
79.90	523.0
81.00	1569.0
81.90	357.0
86.10	63.0
87.00	1893.0
87.90	2000.0
91.00	253.0
92.00	1413.0
93.00	2421.0
94.00	6036.0
95.00	52384.0
96.00	3192.0
97.00	77.0
103.90	299.0
105.80	218.0
106.00	217.0
114.90	76.0
115.90	205.0
116.80	357.0
117.80	170.0
119.00	226.0
128.00	146.0
128.80	72.0
129.80	236.0
130.80	84.0
133.20	56.0
134.90	99.0
136.80	69.0
140.90	412.0
141.90	61.0
142.90	511.0
144.80	75.0
145.90	75.0
147.90	151.0
150.10	50.0
152.90	50.0
154.90	98.0
155.80	79.0
156.90	158.0
158.70	81.0
160.80	69.0
171.90	231.0
173.00	601.0
173.90	47840.0
174.90	3181.0
175.90	47896.0
176.90	2807.0
177.90	102.0
192.90	50.0
207.10	74.0
264.90	81.0
281.00	742.0
282.00	335.0
283.20	172.0

Instrument :
MSVOA_W
ClientSampleId :
BFB449