




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
 Data File : VW022274.D
 Acq On : 10 Mar 2022 15:28
 Operator : SY/VA
 Sample : N1775-07
 Misc : 6.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRV3

Manual IntegrationsAPPROVED

Quant Time: Mar 11 03:10:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 03:07:48 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

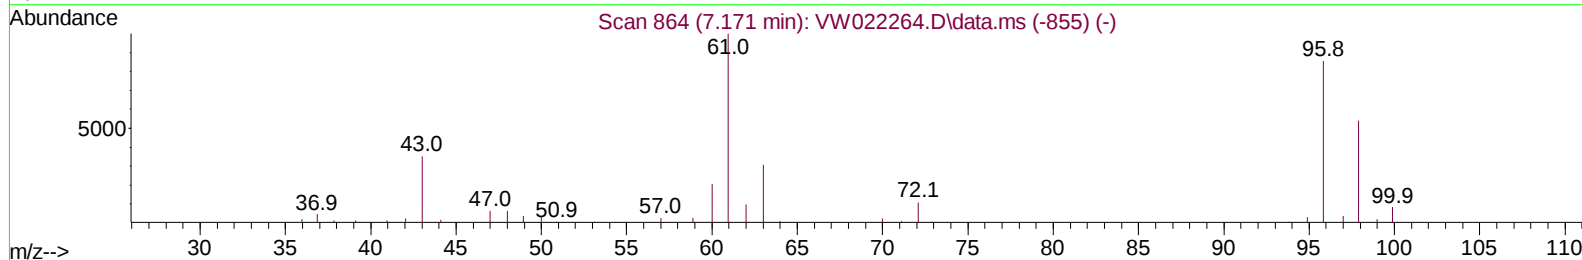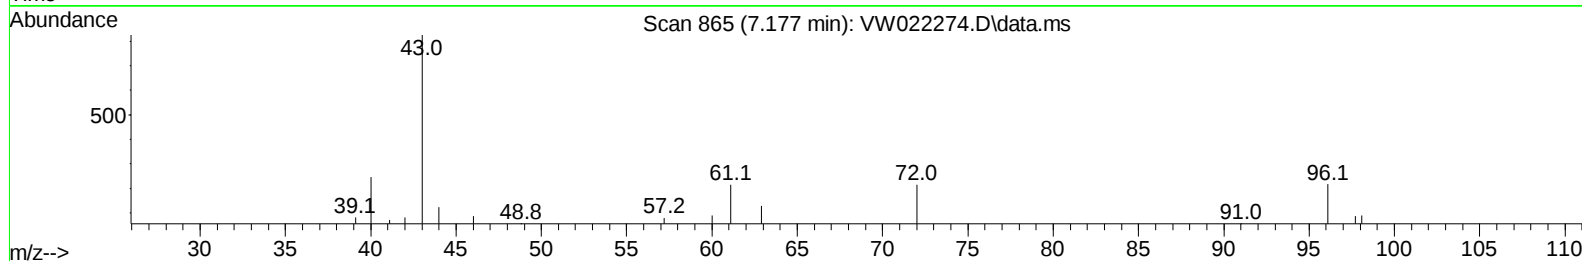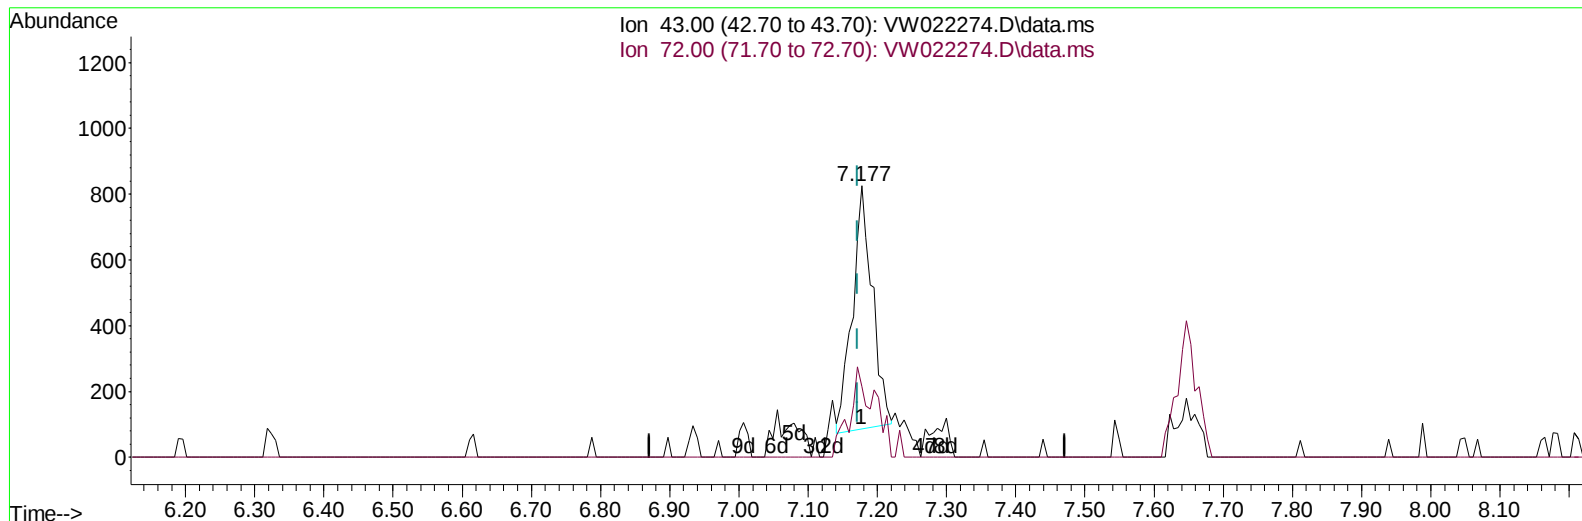

TIC: VW022274.D\data.ms

(22) 2-Butanone (T)

7.177min (+ 0.006) 3.31 ug/L

response 1486

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	34.00	23.35
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
 Data File : VW022274.D
 Acq On : 10 Mar 2022 15:28
 Operator : SY/VA
 Sample : N1775-07
 Misc : 6.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRV3

Manual IntegrationsAPPROVED

Quant Time: Mar 11 03:10:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 03:07:48 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

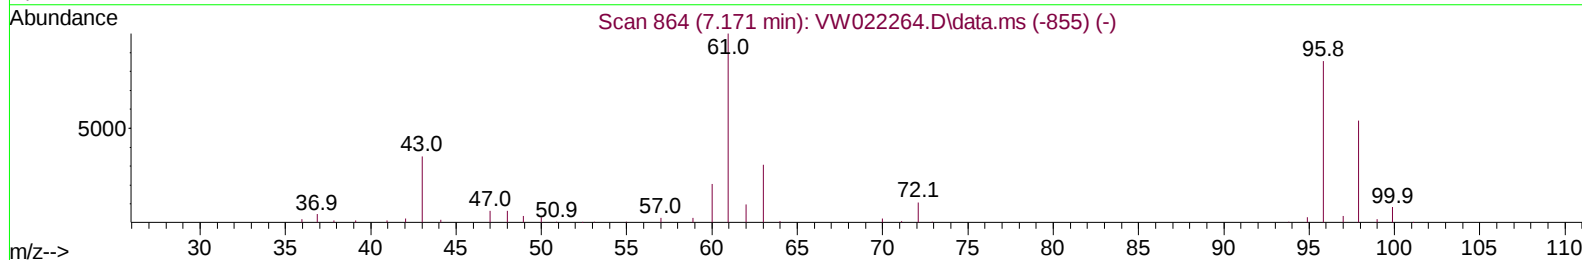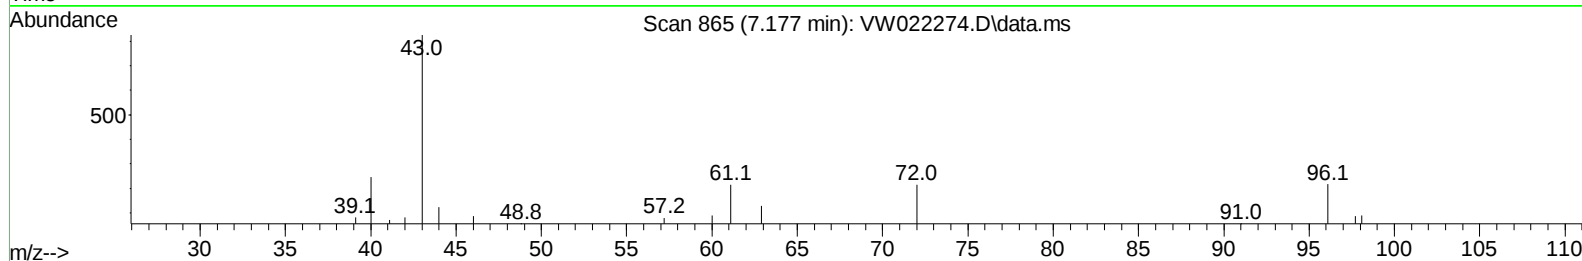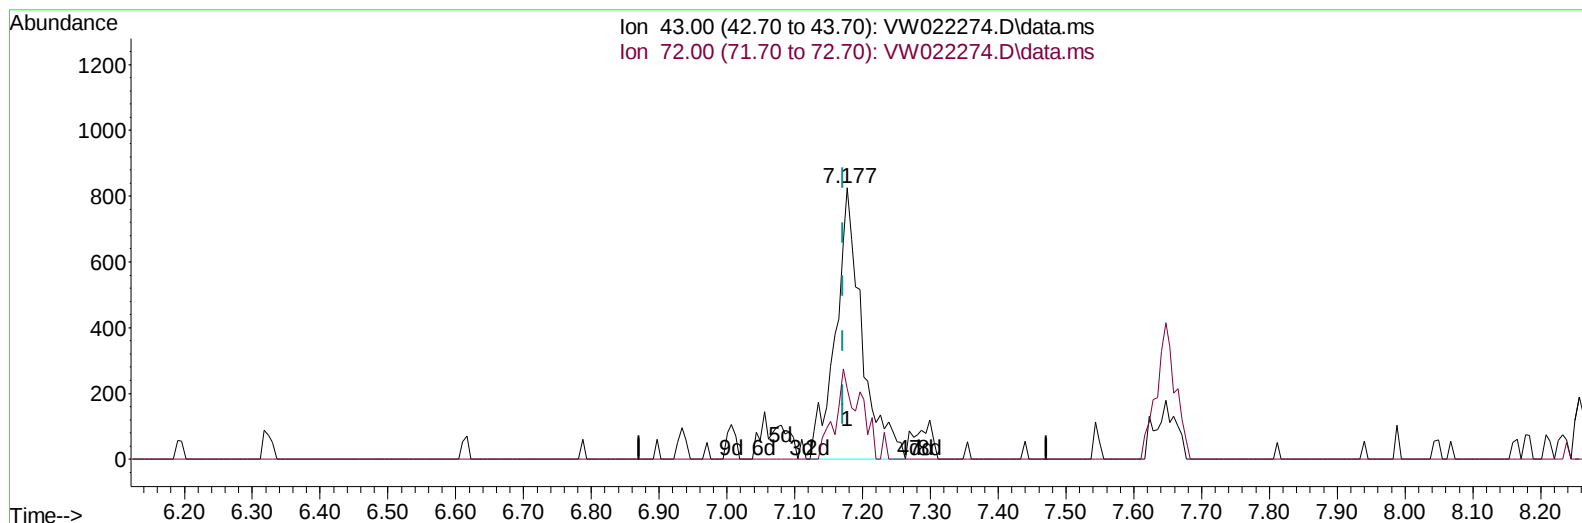

TIC: VW022274.D\data.ms

(22) 2-Butanone (T)

7.177min (+ 0.006) 4.96 ug/L m

response 2228

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	34.00	15.57#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
 Data File : VW022274.D
 Acq On : 10 Mar 2022 15:28
 Operator : SY/VA
 Sample : N1775-07
 Misc : 6.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRV3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
 Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 03:10:28 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 03:07:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	174539	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	162316	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	78646	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	66158	29.061	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	116.240%	
7) Chloroethane-d5	2.879	69	48464	27.057	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	108.240%	
11) 1,1-Dichloroethene-d2	4.013	63	64161	18.404	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	73.600%	
21) 2-Butanone-d5	7.074	46	23064	60.256	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	120.520%	
24) Chloroform-d	7.647	84	95979	24.647	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	98.600%	
26) 1,2-Dichloroethane-d4	8.305	65	54339	26.844	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	107.360%	
32) Benzene-d6	8.275	84	195125	25.830	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	103.320%	
36) 1,2-Dichloropropane-d6	9.275	67	53741	25.617	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	102.480%	
41) Toluene-d8	10.323	98	186775	24.869	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	99.480%	
43) trans-1,3-Dichloroprop...	10.573	79	22590	24.286	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	97.160%	
47) 2-Hexanone-d5	10.927	63	18456	53.489	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	106.980%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	49466	26.867	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	107.480%	
66) 1,2-Dichlorobenzene-d4	13.853	152	66193	26.204	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	104.800%	
Target Compounds						
13) Acetone	4.117	43	5323	17.027	ug/L	84
14) Carbon disulfide	4.379	76	6491	1.389	ug/L	98
22) 2-Butanone	7.177	43	2228m	4.961	ug/L	
46) Tetrachloroethene	10.860	164	1676	0.851	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
Data File : VW022274.D
Acq On : 10 Mar 2022 15:28
Operator : SY/VA
Sample : N1775-07
Misc : 6.28g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRV3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/13/2022
Supervised By :Mahesh Dadoda 03/14/2022

Quant Time: Mar 11 03:10:28 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 03:07:48 2022
Response via : Initial Calibration

