

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
 Data File : VW022273.D
 Acq On : 10 Mar 2022 15:04
 Operator : SY/VA
 Sample : N1775-05
 Misc : 7.30g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRV1

Quant Time: Mar 11 03:10:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 03:07:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	187603	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	172157	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	80754	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	73364	29.982	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	119.920%
7) Chloroethane-d5	2.879	69	47646	24.748	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.000%
11) 1,1-Dichloroethene-d2	4.013	63	69076	18.434	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.720%
21) 2-Butanone-d5	7.074	46	25599	62.222	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.440%
24) Chloroform-d	7.653	84	103704	24.776	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.120%
26) 1,2-Dichloroethane-d4	8.305	65	56686	26.053	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.200%
32) Benzene-d6	8.275	84	209216	26.112	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.440%
36) 1,2-Dichloropropane-d6	9.274	67	56872	25.560	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.240%
41) Toluene-d8	10.323	98	198687	24.943	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.760%
43) trans-1,3-Dichloroprop...	10.579	79	24901	25.240	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.960%
47) 2-Hexanone-d5	10.920	63	20872	57.034	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.060%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	52118	26.690	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.760%
66) 1,2-Dichlorobenzene-d4	13.847	152	73543	28.354	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	113.400%
Target Compounds					Qvalue	
13) Acetone	4.123	43	1994	5.934	ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
Data File : VW022273.D
Acq On : 10 Mar 2022 15:04
Operator : SY/VA
Sample : N1775-05
Misc : 7.30g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBRV1


Quant Time: Mar 11 03:10:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 03:07:48 2022
Response via : Initial Calibration

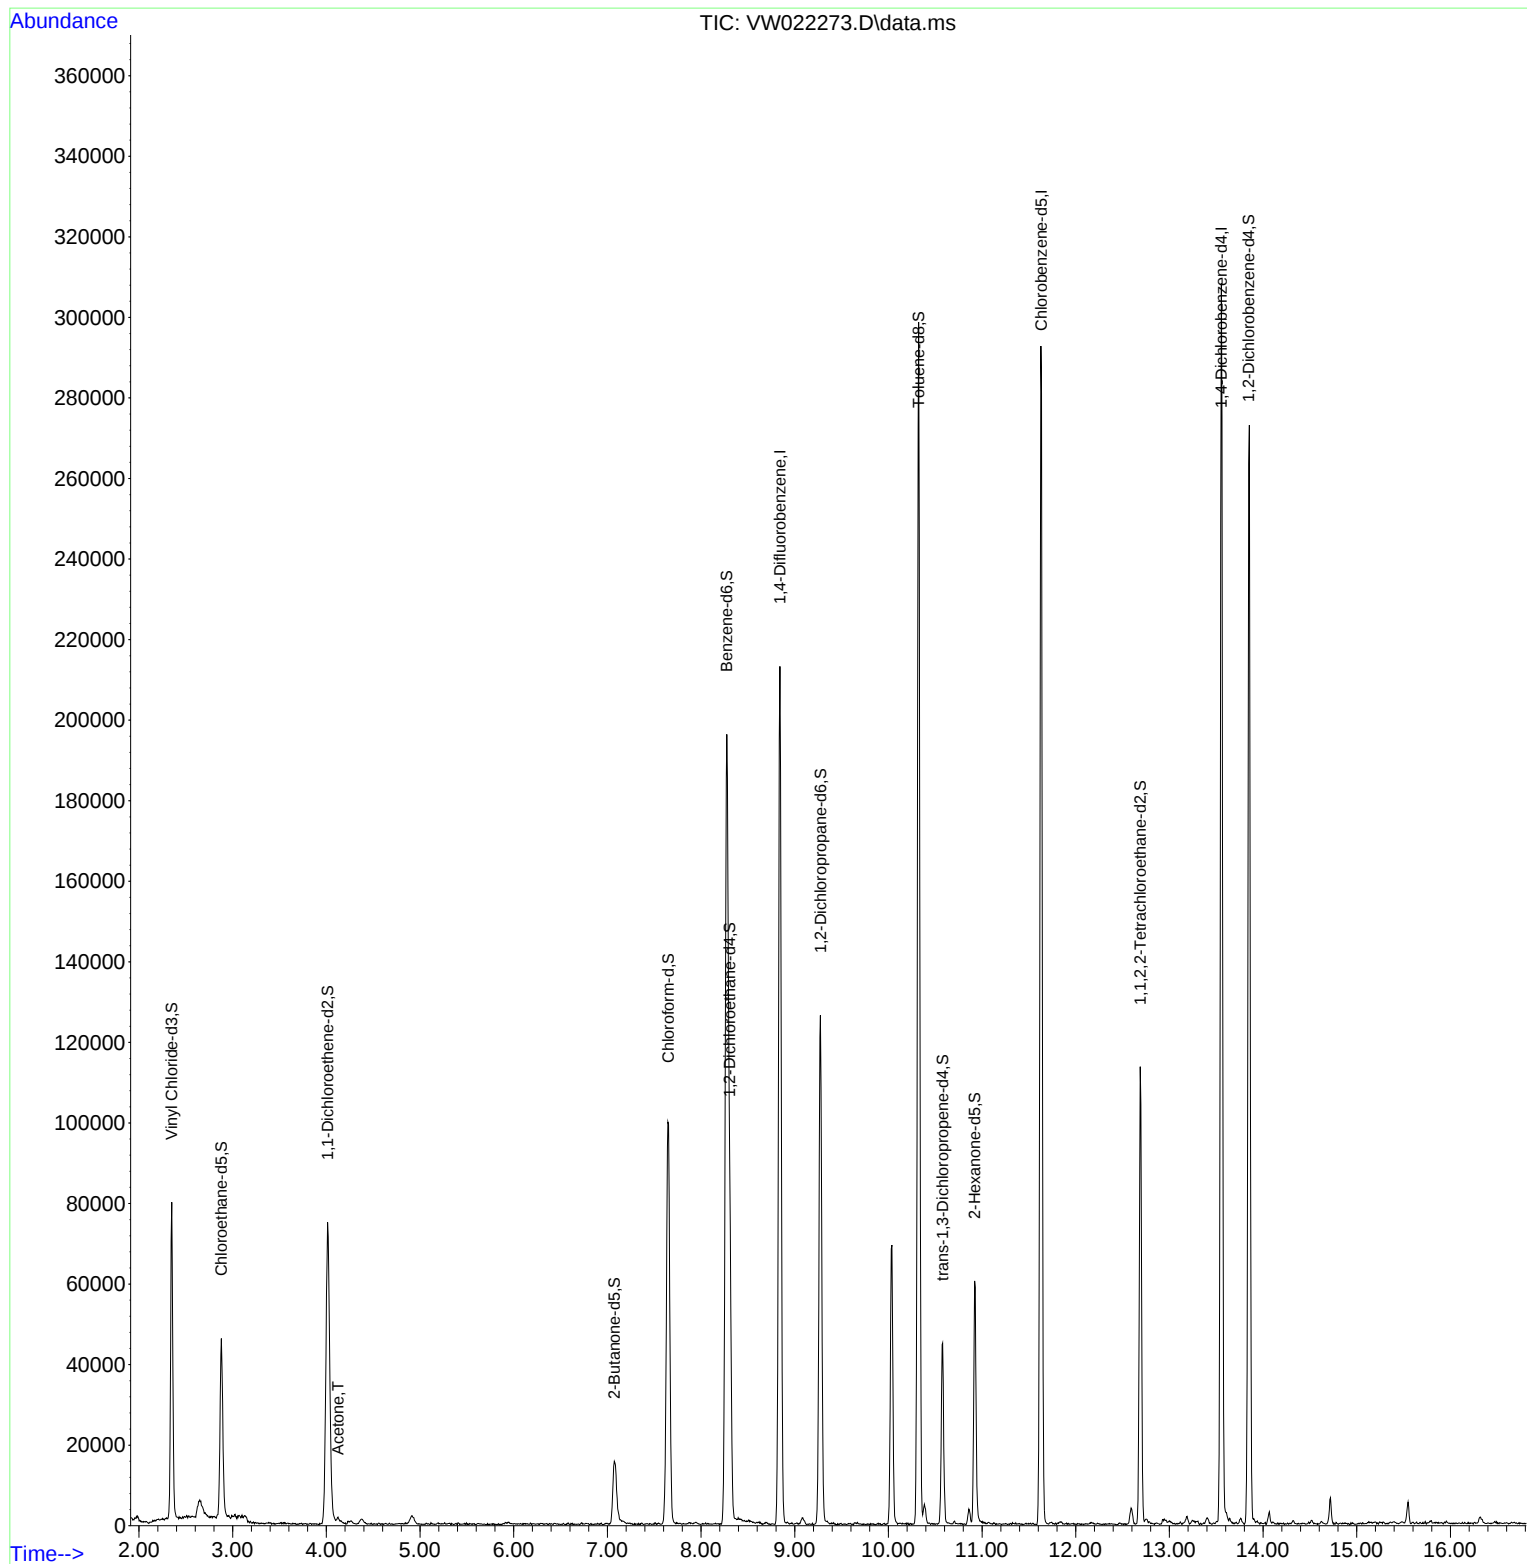

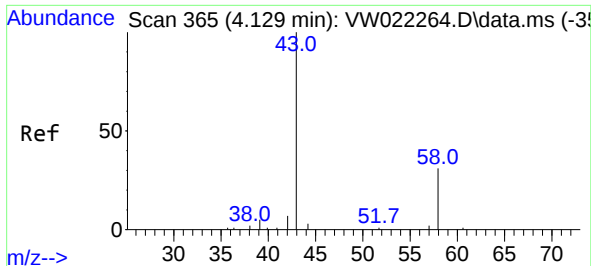

#13
 Acetone
 Concen: 5.934 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW022273.D
 Acq: 10 Mar 2022 15:04

Instrument :
 MSVOA_W
 ClientSampleId :
 DBRV1

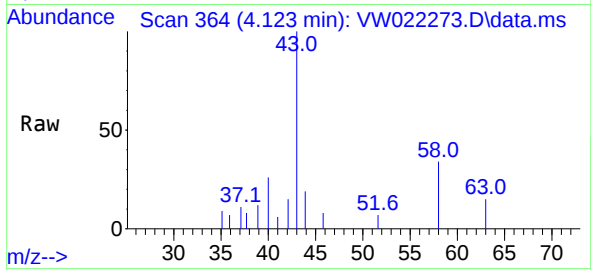

Tgt Ion: 43 Resp: 1994
 Ion Ratio Lower Upper
 43 100
 58 19.2 0.0 69.2

