

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
 Data File : VW022276.D
 Acq On : 10 Mar 2022 16:20
 Operator : SY/VA
 Sample : N1846-01
 Misc : 5.13g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG1

Quant Time: Mar 11 03:10:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 03:07:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	184232	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	172533	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	83190	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	68983	28.708	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	114.840%
7) Chloroethane-d5	2.873	69	48834	25.829	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.320%
11) 1,1-Dichloroethene-d2	4.007	63	67457	18.332	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.320%
21) 2-Butanone-d5	7.074	46	27146	67.189	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.380%
24) Chloroform-d	7.647	84	102707	24.987	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.960%
26) 1,2-Dichloroethane-d4	8.305	65	59439	27.819	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.280%
32) Benzene-d6	8.275	84	202840	25.261	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.040%
36) 1,2-Dichloropropane-d6	9.268	67	57035	25.577	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.320%
41) Toluene-d8	10.323	98	199950	25.047	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.200%
43) trans-1,3-Dichloroprop...	10.573	79	25136	25.423	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.680%
47) 2-Hexanone-d5	10.921	63	22020	60.039	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.080%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	55497	28.358	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	113.440%
66) 1,2-Dichlorobenzene-d4	13.853	152	71571	26.786	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.160%
Target Compounds						
13) Acetone	4.123	43	1063	3.221	ug/L	Qvalue 51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
Data File : VW022276.D
Acq On : 10 Mar 2022 16:20
Operator : SY/VA
Sample : N1846-01
Misc : 5.13g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG1


Quant Time: Mar 11 03:10:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 03:07:48 2022
Response via : Initial Calibration

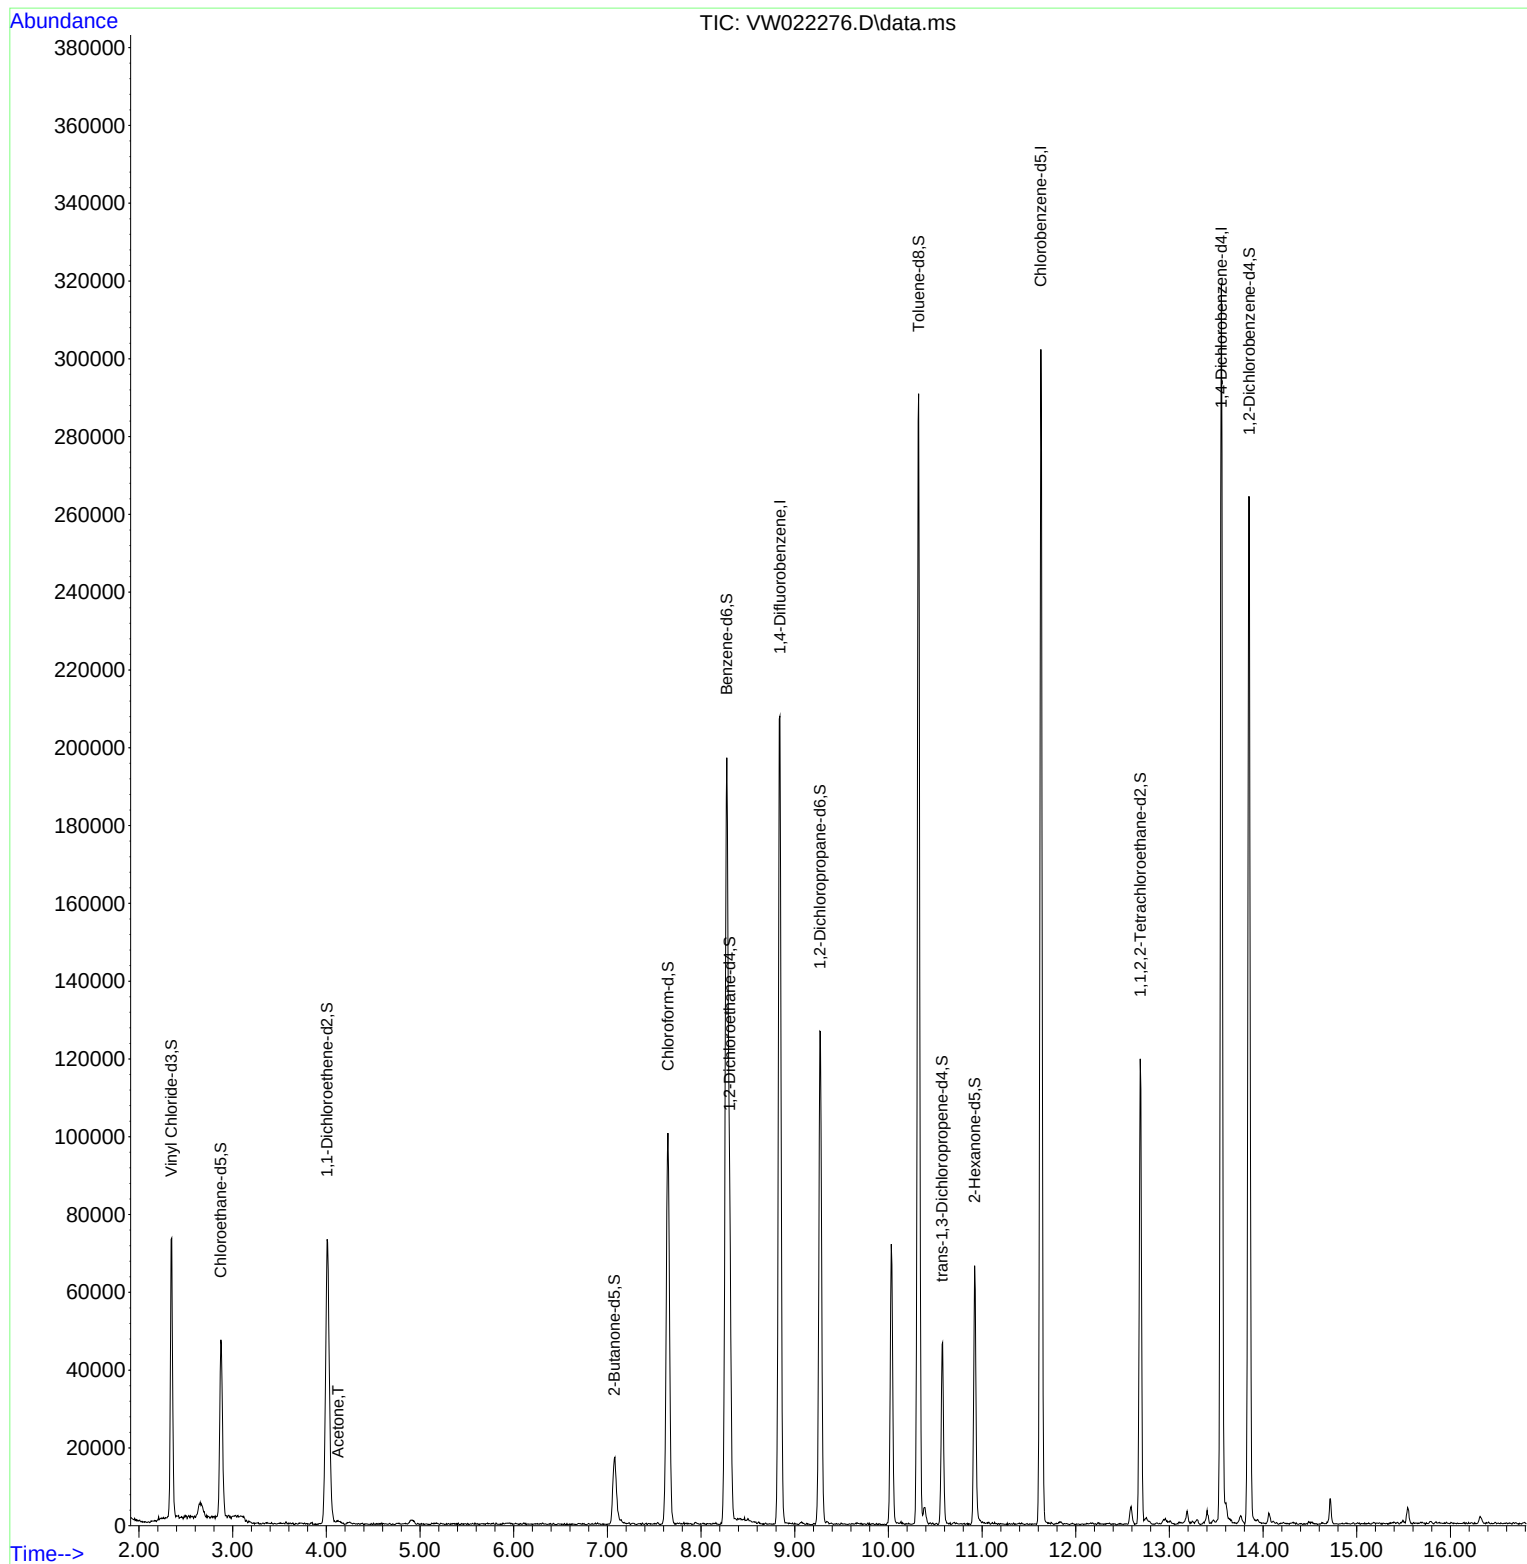

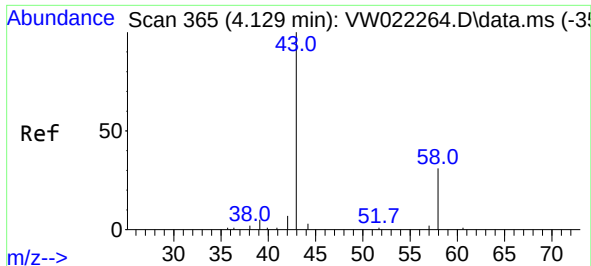

#13
 Acetone
 Concen: 3.221 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW022276.D
 Acq: 10 Mar 2022 16:20

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG1

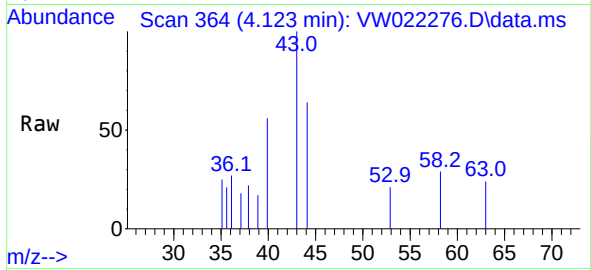

Tgt Ion: 43 Resp: 1063
 Ion Ratio Lower Upper
 43 100
 58 6.3 0.0 69.2

