

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
 Data File : VW022277.D
 Acq On : 10 Mar 2022 16:44
 Operator : SY/VA
 Sample : N1846-02
 Misc : 4.93g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSG2

Quant Time: Mar 11 03:11:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 11 03:07:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	169220	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	162210	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	81606	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	64159	29.069	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.280%
7) Chloroethane-d5	2.885	69	47758	27.501	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	110.000%
11) 1,1-Dichloroethene-d2	4.013	63	62421	18.468	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.880%
21) 2-Butanone-d5	7.074	46	28938	77.979	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	155.960%#
24) Chloroform-d	7.653	84	94925	25.142	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.560%
26) 1,2-Dichloroethane-d4	8.305	65	56072	28.571	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	114.280%
32) Benzene-d6	8.275	84	188231	24.934	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.720%
36) 1,2-Dichloropropane-d6	9.274	67	52686	25.130	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.520%
41) Toluene-d8	10.323	98	184548	24.589	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.360%
43) trans-1,3-Dichloroprop...	10.579	79	25396	27.320	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	109.280%
47) 2-Hexanone-d5	10.921	63	23170	67.195	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.400%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	56057	30.467	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.880%#
66) 1,2-Dichlorobenzene-d4	13.847	152	72364	27.608	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.440%
Target Compounds					Qvalue	
13) Acetone	4.123	43	1293	4.266	ug/L	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031022\
Data File : VW022277.D
Acq On : 10 Mar 2022 16:44
Operator : SY/VA
Sample : N1846-02
Misc : 4.93g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DBSG2

Quant Time: Mar 11 03:11:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM022322SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 11 03:07:48 2022
Response via : Initial Calibration

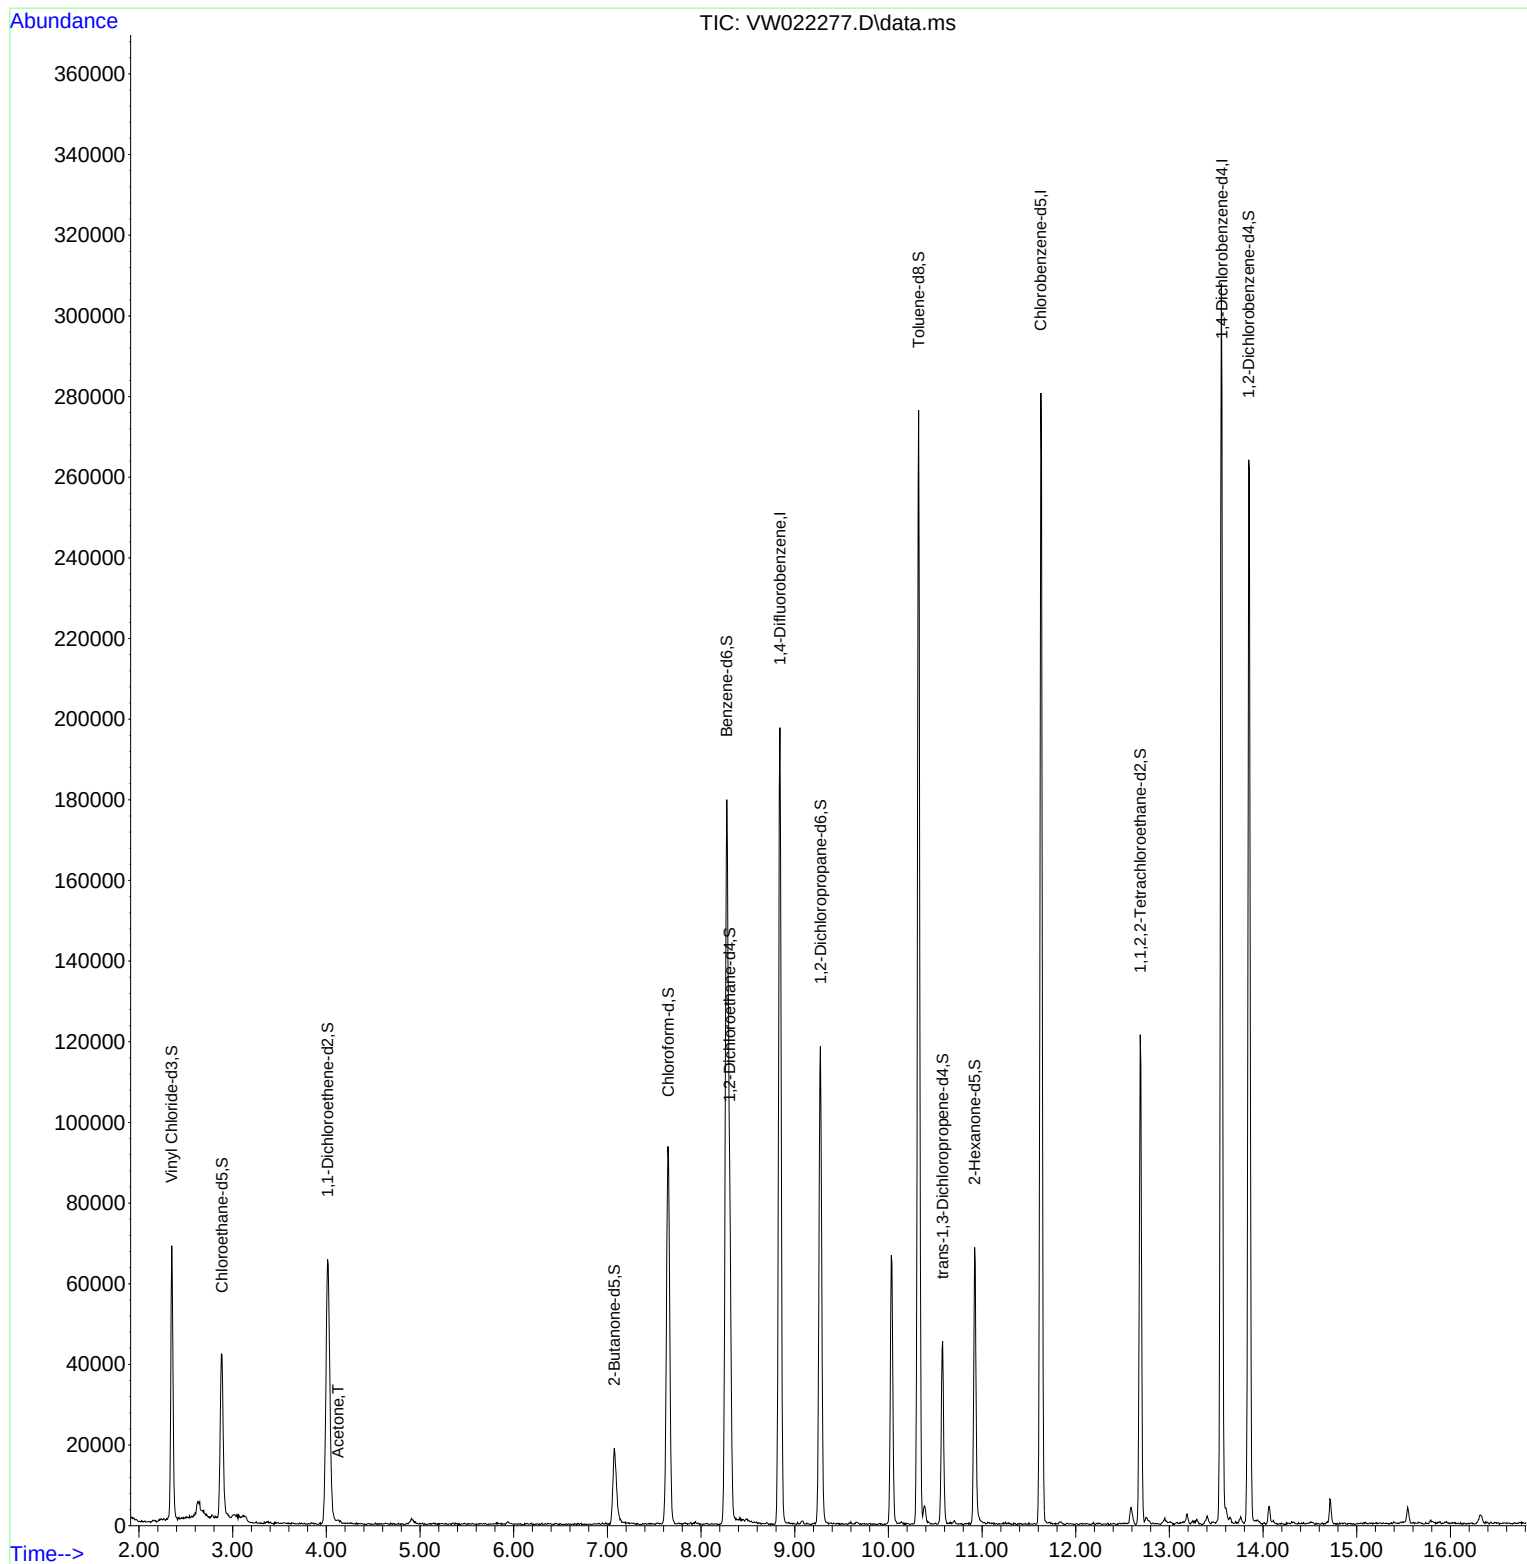

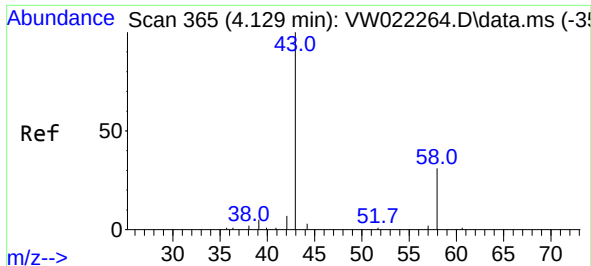

#13

Acetone

Concen: 4.266 ug/L

RT: 4.123 min Scan# 3

Delta R.T. -0.006 min

Lab File: VW022277.D


Acq: 10 Mar 2022 16:44

Instrument :

MSVOA_W

ClientSampleId :

DBSG2

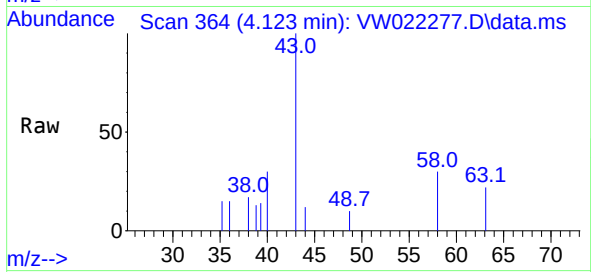

Tgt Ion: 43 Resp: 1293

Ion Ratio Lower Upper

43 100

58 16.6 0.0 69.2

