

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031424\
 Data File : VW028188.D
 Acq On : 14 Mar 2024 19:02
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 15 02:00:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 15 01:46:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	186186	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	166661	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	85469	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	48157	22.106	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.440%
7) Chloroethane-d5	2.899	69	34341	22.563	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.240%
11) 1,1-Dichloroethene-d2	4.027	65	31412	22.738	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.960%
21) 2-Butanone-d5	7.075	46	31843	49.560	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.120%
24) Chloroform-d	7.648	84	129327	23.556	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.240%
26) 1,2-Dichloroethane-d4	8.307	65	75231	24.865	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.480%
32) Benzene-d6	8.276	84	256812	25.239	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.960%
36) 1,2-Dichloropropane-d6	9.276	67	73982	25.265	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.080%
41) Toluene-d8	10.318	98	239869	25.558	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	102.240%
43) trans-1,3-Dichloroprop...	10.575	79	32414	24.372	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.480%
47) 2-Hexanone-d5	10.922	63	25278	52.225	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.460%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	54657	25.269	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.080%
66) 1,2-Dichlorobenzene-d4	13.848	152	78340	25.161	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.640%
Target Compounds						
37) 1,2-Dichloropropane	9.270	63	9336	3.559	ug/L	Qvalue # 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031424\
Data File : VW028188.D
Acq On : 14 Mar 2024 19:02
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 15 02:00:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 15 01:46:51 2024
Response via : Initial Calibration

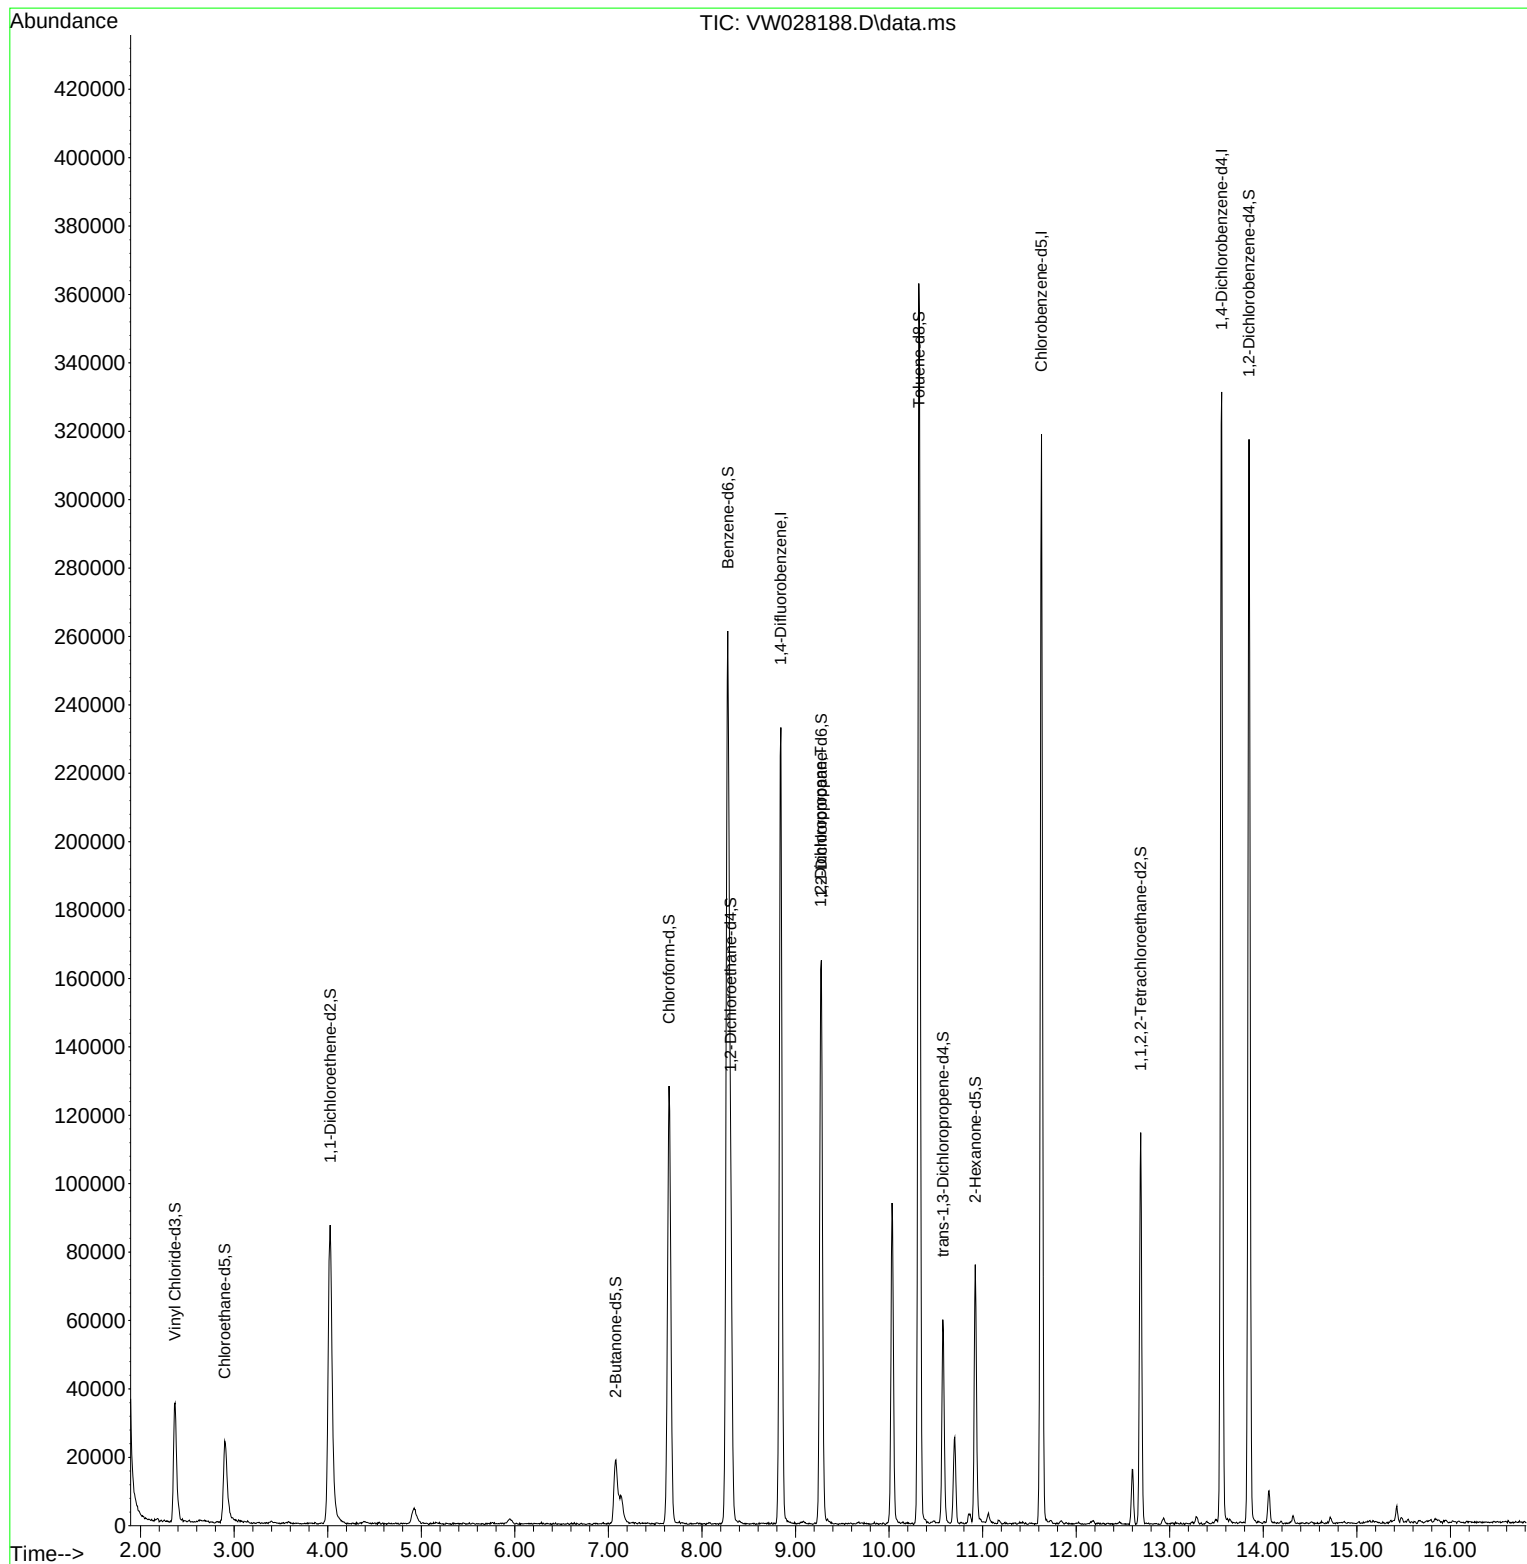

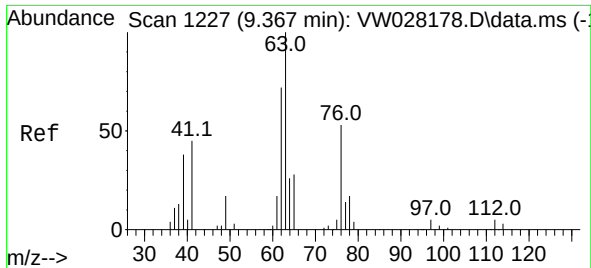

#37
 1,2-Dichloropropane
 Concen: 3.559 ug/L
 RT: 9.270 min Scan# 11
 Delta R.T. -0.097 min
 Lab File: VW028188.D
 Acq: 14 Mar 2024 19:02

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 63 Resp: 9336
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.8 5.8#

