

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031424\
 Data File : VW028190.D
 Acq On : 14 Mar 2024 19:50
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 15 02:01:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 15 01:46:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	185749	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	165910	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	82861	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	54589	25.117	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 100.480%			
7) Chloroethane-d5	2.899	69	40093	26.405	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 105.600%			
11) 1,1-Dichloroethene-d2	4.021	65	36192	26.260	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 105.040%			
21) 2-Butanone-d5	7.075	46	36845	57.480	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 114.960%			
24) Chloroform-d	7.648	84	153564	28.037	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 112.160%			
26) 1,2-Dichloroethane-d4	8.307	65	89445	29.633	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 118.520%			
32) Benzene-d6	8.276	84	308017	30.408	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 121.640%			
36) 1,2-Dichloropropane-d6	9.270	67	87770	30.110	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 120.440%#			
41) Toluene-d8	10.319	98	285566	30.564	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 122.240%			
43) trans-1,3-Dichloroprop...	10.575	79	38134	28.803	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 115.200%			
47) 2-Hexanone-d5	10.922	63	28199	58.524	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 117.040%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	62498	29.024	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 116.080%			
66) 1,2-Dichlorobenzene-d4	13.848	152	92752	30.728	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 122.920%#			
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	2835	0.678	ug/L #	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031424\
Data File : VW028190.D
Acq On : 14 Mar 2024 19:50
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 15 02:01:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 15 01:46:51 2024
Response via : Initial Calibration

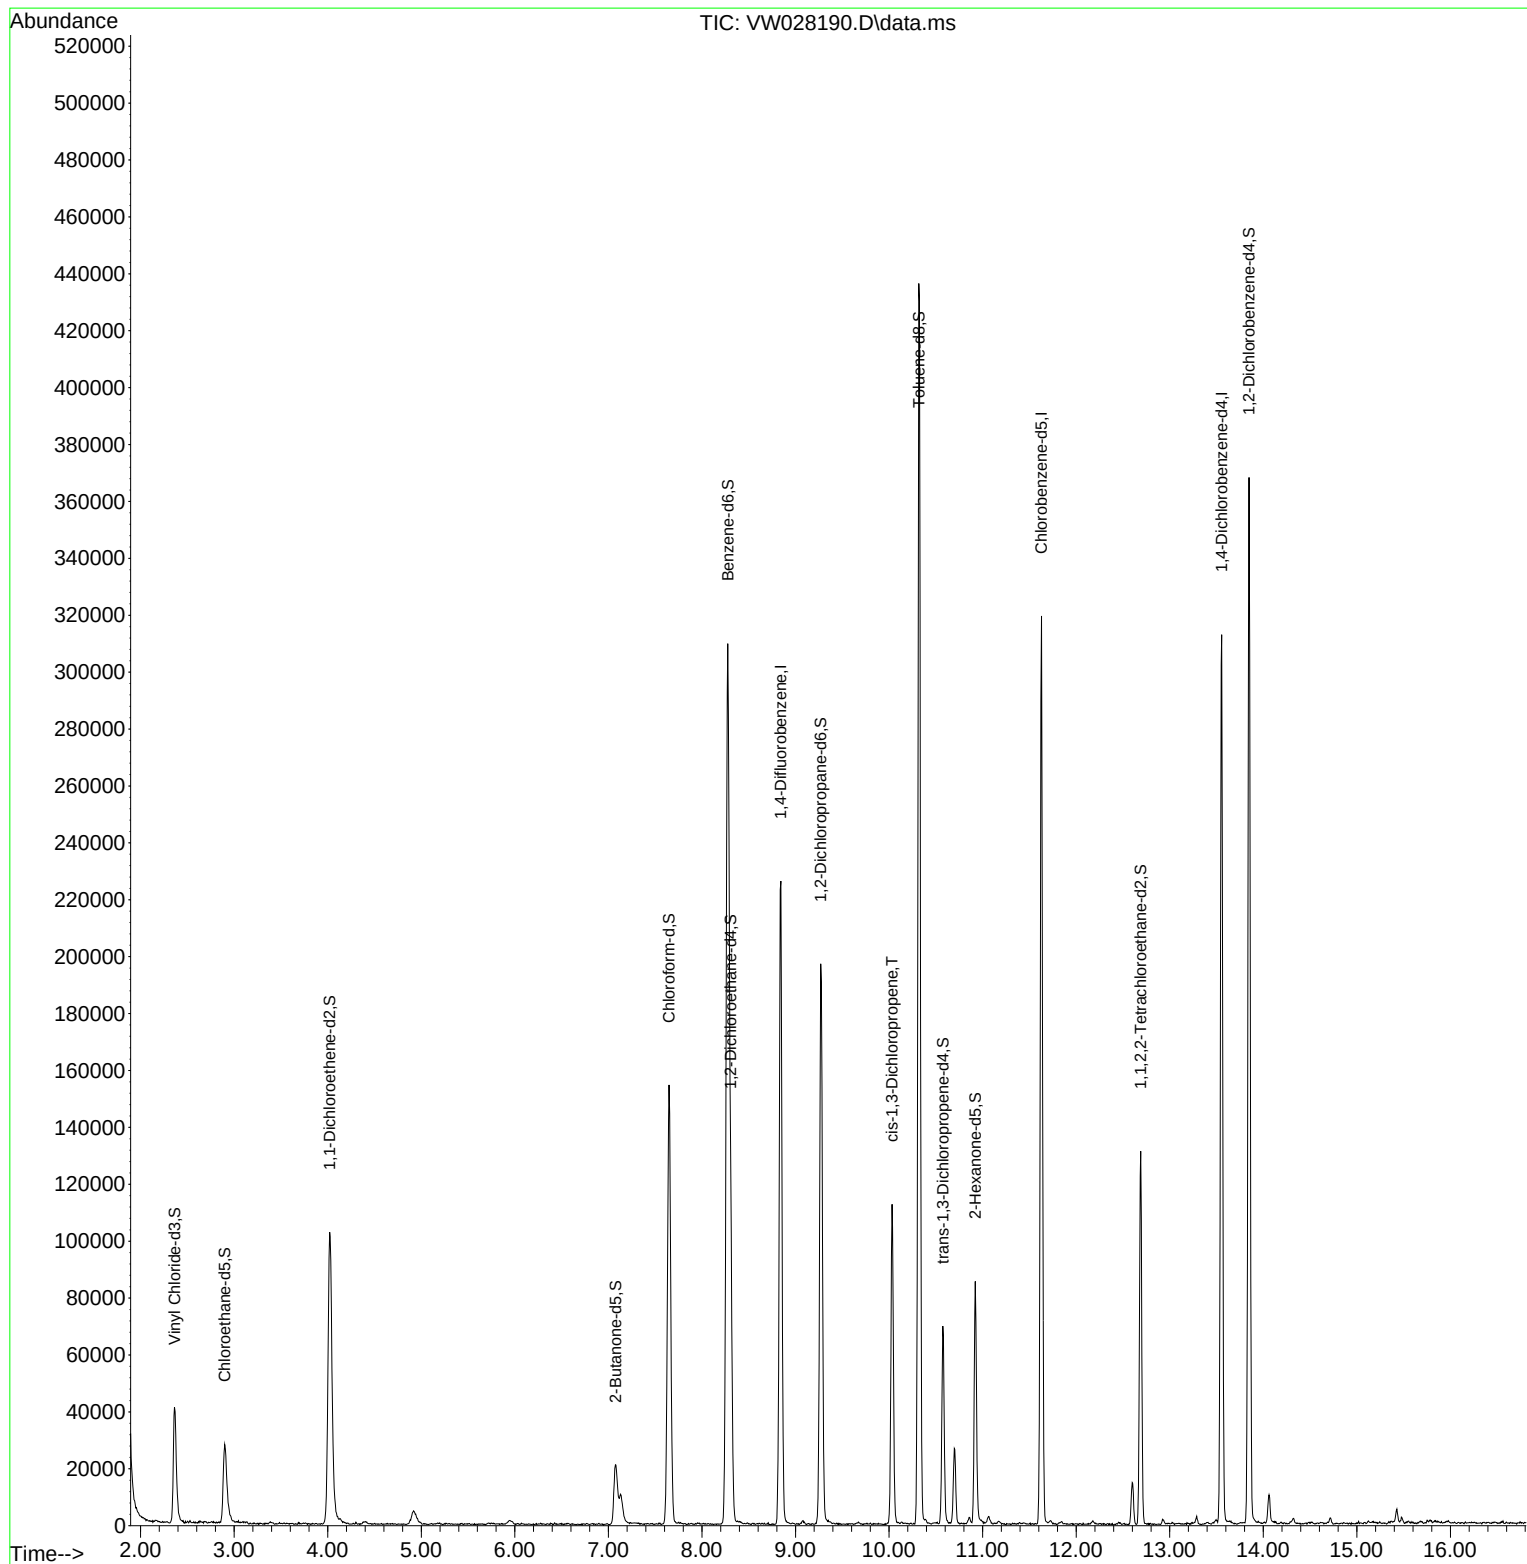

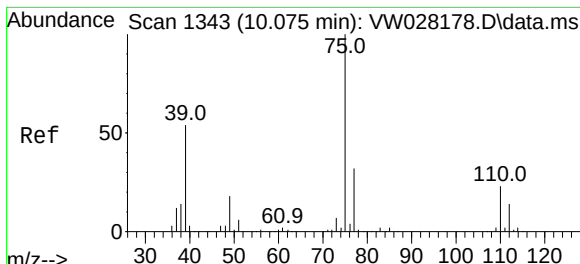

#39
 cis-1,3-Dichloropropene
 Concen: 0.678 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW028190.D
 Acq: 14 Mar 2024 19:50

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion:	75	Resp:	2835
Ion Ratio	Lower	Upper	
75	100		
77	47.2	22.5	41.7#

