

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031424\
 Data File : VW028185.D
 Acq On : 14 Mar 2024 17:51
 Operator : SY/MD
 Sample : P1742-21MSD
 Misc : 4.65g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 15 01:59:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 15 01:46:51 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	197982	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	176441	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	75747	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	65919	28.457	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 113.840%	
7) Chloroethane-d5	2.899	69	47039	29.065	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 116.280%	
11) 1,1-Dichloroethene-d2	4.027	65	41366	28.160	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 112.640%#	
21) 2-Butanone-d5	7.075	46	47911	70.125	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 140.240%#	
24) Chloroform-d	7.648	84	176311	30.201	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 120.800%	
26) 1,2-Dichloroethane-d4	8.307	65	102818	31.959	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 127.840%	
32) Benzene-d6	8.276	84	338397	31.413	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 125.640%	
36) 1,2-Dichloropropane-d6	9.276	67	98412	31.745	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 127.000%#	
41) Toluene-d8	10.318	98	307362	30.934	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 123.720%	
43) trans-1,3-Dichloroprop...	10.575	79	45364	32.219	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 128.880%	
47) 2-Hexanone-d5	10.922	63	39366	76.823	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 153.640%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	74890	32.703	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 130.800%#	
66) 1,2-Dichlorobenzene-d4	13.848	152	82940	30.058	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 120.240%#	
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.015	85	71150m	24.774	ug/L	
3) Chloromethane	2.222	50	49222	24.164	ug/L	99
5) Vinyl chloride	2.369	62	54686	23.750	ug/L	93
6) Bromomethane	2.795	94	33376	24.339	ug/L	97
8) Chloroethane	2.936	64	29448	23.794	ug/L	99
9) Trichlorofluoromethane	3.271	101	78954	28.361	ug/L	100
10) 1,1,2-Trichloro-1,2,2-...	4.076	101	64951m	23.485	ug/L	
12) 1,1-Dichloroethene	4.045	96	61539	24.071	ug/L	99
13) Acetone	4.118	43	47845	63.070	ug/L	99
14) Carbon disulfide	4.387	76	188083	23.587	ug/L	98
15) Methyl Acetate	4.673	43	30983	26.515	ug/L	99
16) Methylene chloride	4.923	84	64105	21.274	ug/L	93
17) trans-1,2-Dichloroethene	5.435	96	63637	23.422	ug/L	92
18) Methyl tert-butyl Ether	5.423	73	115551	28.189	ug/L #	91
19) 1,1-Dichloroethane	6.222	63	126897	24.125	ug/L	97
20) cis-1,2-Dichloroethene	7.173	96	71265	24.287	ug/L	96
22) 2-Butanone	7.167	43	50596	58.744	ug/L	99
23) Bromochloromethane	7.520	128	31371	24.183	ug/L	93
25) Chloroform	7.679	83	132723	24.510	ug/L	99

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031424\
 Data File : VW028185.D
 Acq On : 14 Mar 2024 17:51
 Operator : SY/MD
 Sample : P1742-21MSD
 Misc : 4.65g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 15 01:59:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 15 01:46:51 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
27) 1,2-Dichloroethane	8.398	62	96236	25.166	ug/L	96
29) Cyclohexane	7.959	56	106056	23.045	ug/L	100
30) 1,1,1-Trichloroethane	7.874	97	117181	25.336	ug/L	99
31) Carbon tetrachloride	8.069	117	103058	23.755	ug/L	100
33) Benzene	8.325	78	269796	24.849	ug/L	100
34) Trichloroethene	9.093	95	74023	24.437	ug/L	96
35) Methylcyclohexane	9.331	83	95769	18.704	ug/L	99
37) 1,2-Dichloropropane	9.367	63	69582	25.056	ug/L	99
38) Bromodichloromethane	9.642	83	95753	25.574	ug/L	96
39) cis-1,3-Dichloropropene	10.069	75	116243	26.137	ug/L	99
40) 4-Methyl-2-pentanone	10.209	43	91797	59.884	ug/L	100
42) Toluene	10.386	91	288531	24.349	ug/L	99
44) trans-1,3-Dichloropropene	10.605	75	100201	26.685	ug/L	94
45) 1,1,2-Trichloroethane	10.788	97	51408	25.621	ug/L	99
46) Tetrachloroethene	10.861	164	222746	91.225	ug/L	99
48) 2-Hexanone	10.965	43	73990	61.618	ug/L	97
49) Dibromochloromethane	11.123	129	61078	25.703	ug/L	96
50) 1,2-Dibromoethane	11.233	107	49304	25.698	ug/L	95
51) Chlorobenzene	11.654	112	176351	23.447	ug/L	98
52) Ethylbenzene	11.727	91	319397	23.090	ug/L	99
53) m,p-Xylene	11.836	106	118917	22.845	ug/L	94
54) o-Xylene	12.160	106	112859	23.380	ug/L	89
55) Styrene	12.178	104	193487	23.335	ug/L	97
57) 1,1,2,2-Tetrachloroethane	12.708	83	58698	25.576	ug/L	94
59) Bromoform	12.349	173	36185	31.880	ug/L	95
60) Isopropylbenzene	12.458	105	307668	27.338	ug/L	97
61) 1,2,3-Trichloropropane	12.763	75	45882	31.738	ug/L	99
62) 1,3,5-Trimethylbenzene	12.940	105	186395	24.684	ug/L	100
63) 1,2,4-Trimethylbenzene	13.245	105	229197	25.137	ug/L	99
64) 1,3-Dichlorobenzene	13.495	146	114881	22.881	ug/L	99
65) 1,4-Dichlorobenzene	13.574	146	118521	23.607	ug/L	93
67) 1,2-Dichlorobenzene	13.867	146	101345	23.439	ug/L	93
68) 1,2-Dibromo-3-chloropr...	14.476	75	9872	29.070	ug/L	96
69) 1,3,5-Trichlorobenzene	14.623	180	54223	15.504	ug/L	98
70) 1,2,4-trichlorobenzene	15.129	180	40666	13.687	ug/L	96
71) Naphthalene	15.360	128	103306	20.258	ug/L	99
72) 1,2,3-Trichlorobenzene	15.549	180	31897	13.023	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031424\
Data File : VW028185.D
Acq On : 14 Mar 2024 17:51
Operator : SY/MD
Sample : P1742-21MSD
Misc : 4.65g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 15 01:59:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 15 01:46:51 2024
Response via : Initial Calibration




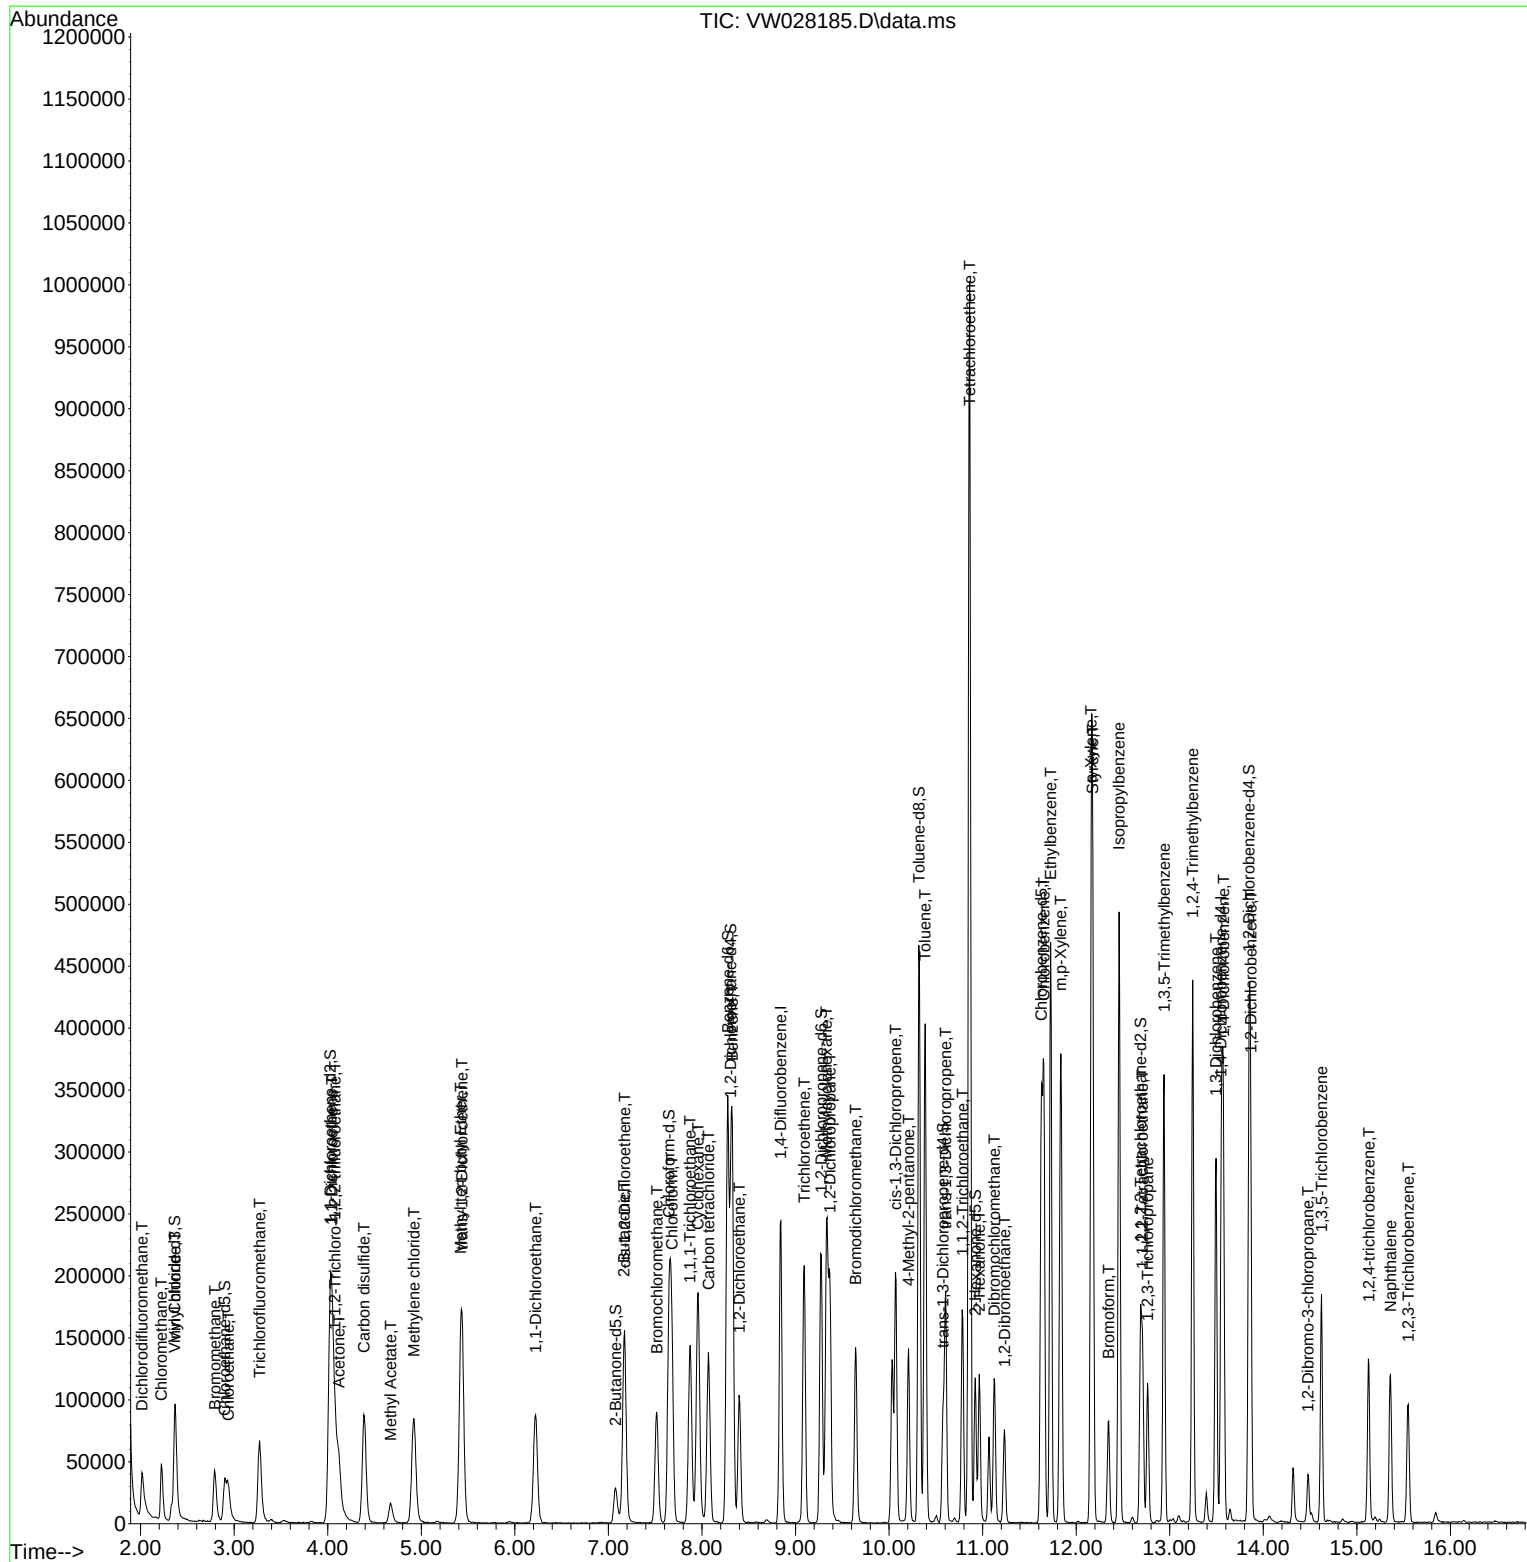




#2
Dichlorodifluoromethane
Concen: 24.774 ug/L m
RT: 2.015 min Scan# 21
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 85 Resp: 71150
Ion Ratio Lower Upper
85 100
87 0.1 20.9 31.3#

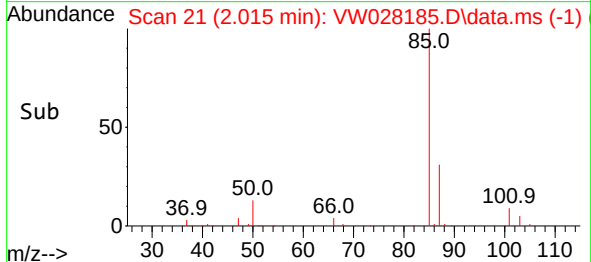

#3
Chloromethane
Concen: 24.164 ug/L
RT: 2.222 min Scan# 55
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 50 Resp: 49222
Ion Ratio Lower Upper
50 100
52 33.0 22.7 42.1


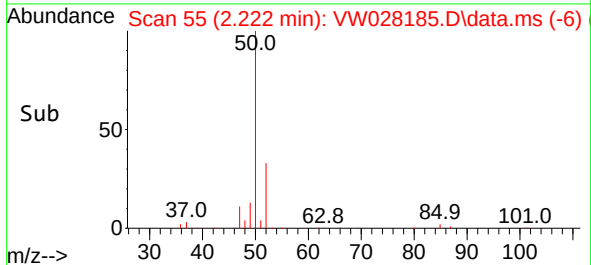






#5
 Vinyl chloride
 Concen: 23.750 ug/L
 RT: 2.369 min Scan# 79
 Delta R.T. -0.006 min
 Lab File: VW028185.D
 Acq: 14 Mar 2024 17:51




Instrument :
 MSVOA_W
 ClientSampleId :


Tgt Ion: 62 Resp: 54686
 Ion Ratio Lower Upper
 62 100
 64 35.8 22.5 41.7

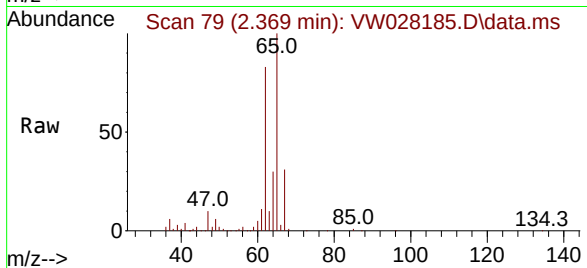

#6
 Bromomethane
 Concen: 24.339 ug/L
 RT: 2.795 min Scan# 149
 Delta R.T. 0.006 min
 Lab File: VW028185.D
 Acq: 14 Mar 2024 17:51

Tgt Ion: 94 Resp: 33376
 Ion Ratio Lower Upper
 94 100
 96 89.5 60.8 113.0




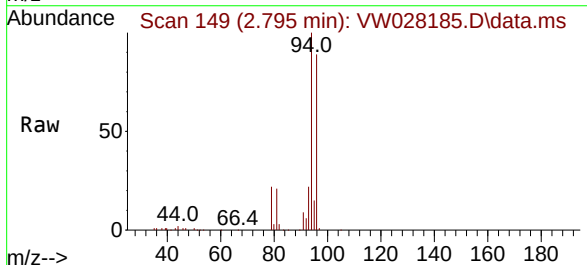




#8
Chloroethane
Concen: 23.794 ug/L
RT: 2.936 min Scan# 172
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 64 Resp: 29448
Ion Ratio Lower Upper
64 100
66 33.1 22.9 42.5



#9
Trichlorofluoromethane
Concen: 28.361 ug/L
RT: 3.271 min Scan# 227
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion:101 Resp: 78954
Ion Ratio Lower Upper
101 100
103 63.9 50.9 76.3




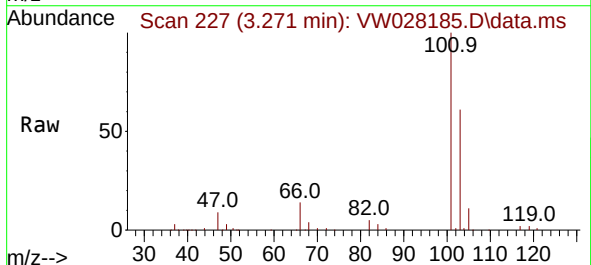


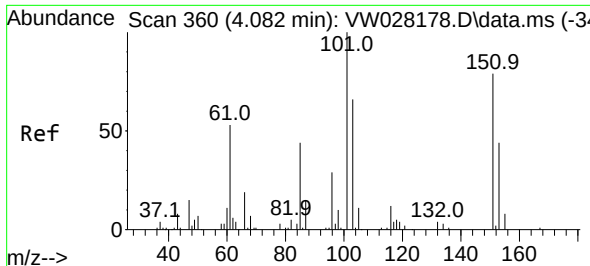

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 23.485 ug/L m
 RT: 4.076 min Scan# 3
 Delta R.T. -0.006 min
 Lab File: VW028185.D
 Acq: 14 Mar 2024 17:51




Instrument :
 MSVOA_W
 ClientSampleId :


Tgt Ion:101 Resp: 64951
 Ion Ratio Lower Upper
 101 100
 85 40.4 36.4 54.6
 151 70.6 58.4 87.6

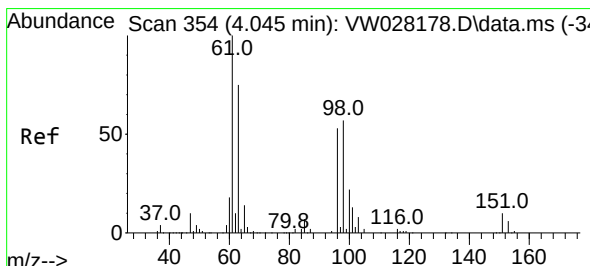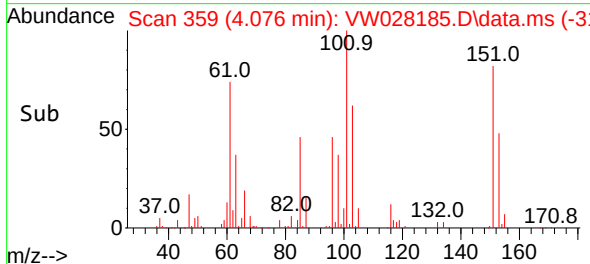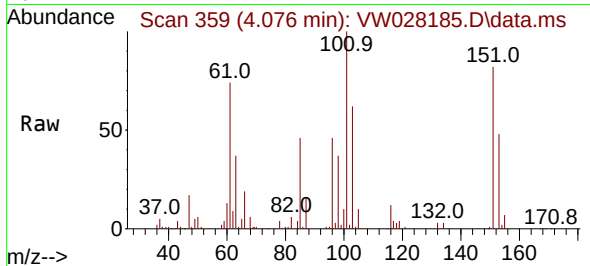

#12
 1,1-Dichloroethene
 Concen: 24.071 ug/L
 RT: 4.045 min Scan# 354
 Delta R.T. 0.000 min
 Lab File: VW028185.D
 Acq: 14 Mar 2024 17:51

Tgt Ion: 96 Resp: 61539
 Ion Ratio Lower Upper
 96 100
 61 190.0 132.2 245.4
 63 150.5 104.6 194.2

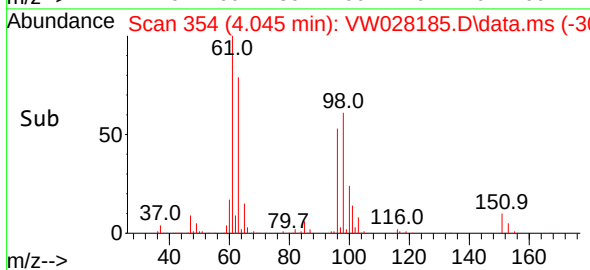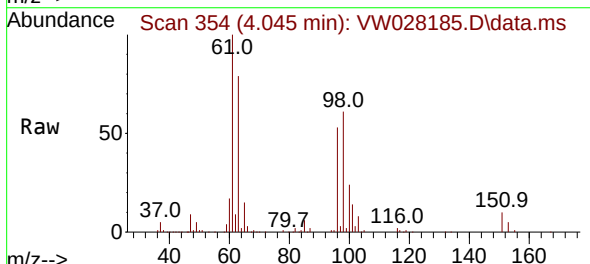



#13

Acetone

Concen: 63.070 ug/L

RT: 4.118 min Scan# 30

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 43 Resp: 47845

Ion Ratio Lower Upper

43 100

58 28.2 0.0 57.8

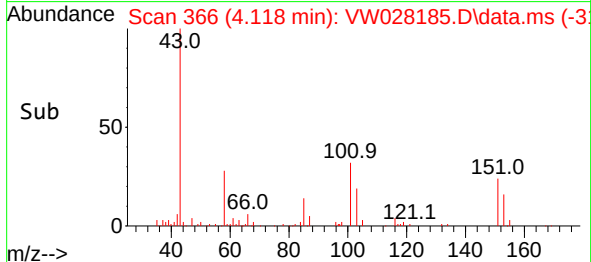

#14

Carbon disulfide

Concen: 23.587 ug/L

RT: 4.387 min Scan# 410

Delta R.T. -0.006 min

Lab File: VW028185.D




Acq: 14 Mar 2024 17:51


Tgt Ion: 76 Resp: 188083

Ion Ratio Lower Upper

76 100

78 9.7 7.1 10.7




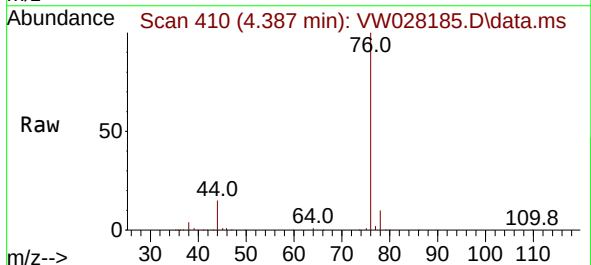




#15
Methyl Acetate
Concen: 26.515 ug/L
RT: 4.673 min Scan# 41
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 43 Resp: 30983
Ion Ratio Lower Upper
43 100
74 23.1 18.2 27.2



#16
Methylene chloride
Concen: 21.274 ug/L
RT: 4.923 min Scan# 498
Delta R.T. 0.006 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 84 Resp: 64105
Ion Ratio Lower Upper
84 100
86 69.3 43.1 80.1
49 134.6 89.4 166.0









#17
trans-1,2-Dichloroethene
Concen: 23.422 ug/L
RT: 5.435 min Scan# 581
Delta R.T. 0.006 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 96 Resp: 63637
Ion Ratio Lower Upper
96 100
61 153.6 98.4 182.8
98 63.1 45.6 84.8

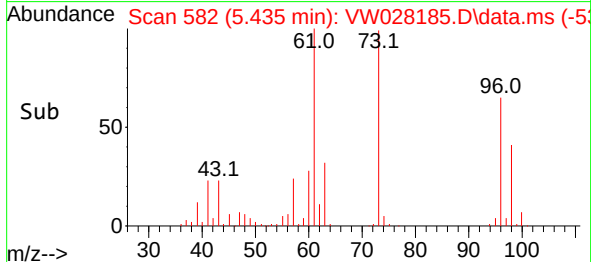

#18
Methyl tert-butyl Ether
Concen: 28.189 ug/L
RT: 5.423 min Scan# 580
Delta R.T. -0.006 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 73 Resp: 115551
Ion Ratio Lower Upper
73 100
43 22.8 18.2 27.4
57 12.7 17.4 26.2#

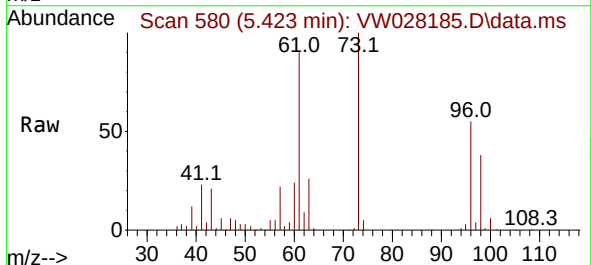



#19

1,1-Dichloroethane

Concen: 24.125 ug/L

RT: 6.222 min Scan# 710

Delta R.T. 0.006 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion: 63 Resp: 126897

Ion Ratio Lower Upper

63 100

65 29.5 22.1 41.1

83 13.5 9.0 16.6



#20

cis-1,2-Dichloroethene

Concen: 24.287 ug/L

RT: 7.173 min Scan# 867

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51




Tgt Ion: 96 Resp: 71265


Ion Ratio Lower Upper

96 100

61 138.3 95.7 177.7

98 69.3 43.9 81.5









#22
2-Butanone
Concen: 58.744 ug/L
RT: 7.167 min Scan# 866
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 43 Resp: 50596
Ion Ratio Lower Upper
43 100
72 26.2 12.8 38.4

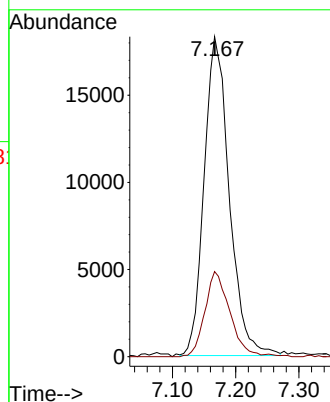

#23
Bromochloromethane
Concen: 24.183 ug/L
RT: 7.520 min Scan# 924
Delta R.T. 0.006 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 128 Resp: 31371
Ion Ratio Lower Upper
128 100
49 169.4 116.6 216.6
130 131.3 80.1 148.7
51 52.2 40.1 60.1









#25
Chloroform
Concen: 24.510 ug/L
RT: 7.679 min Scan# 91
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 83 Resp: 132723
Ion Ratio Lower Upper
83 100
85 64.3 44.5 82.7



#27
1,2-Dichloroethane
Concen: 25.166 ug/L
RT: 8.398 min Scan# 1068
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 62 Resp: 96236
Ion Ratio Lower Upper
62 100
98 8.7 5.9 8.9


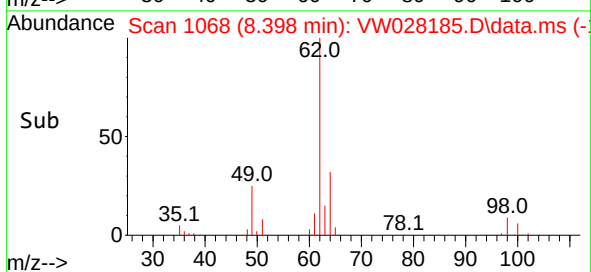




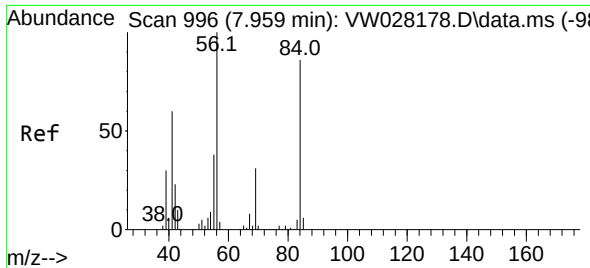

#29
Cyclohexane
Concen: 23.045 ug/L
RT: 7.959 min Scan# 996
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 56 Resp: 106056
Ion Ratio Lower Upper
56 100
69 30.4 24.0 36.0
84 85.7 68.4 102.6

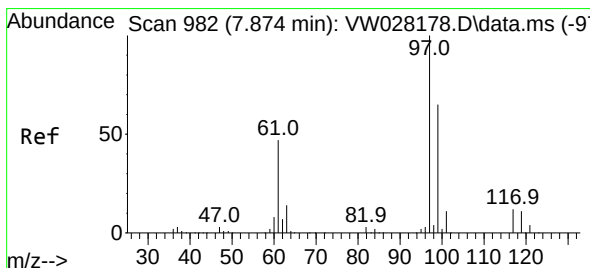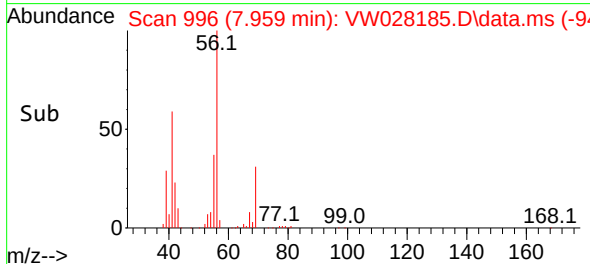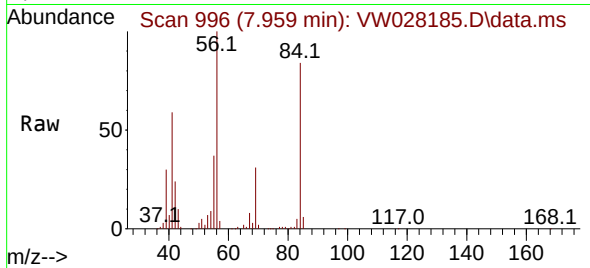

#30
1,1,1-Trichloroethane
Concen: 25.336 ug/L
RT: 7.874 min Scan# 982
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 97 Resp: 117181
Ion Ratio Lower Upper
97 100
99 63.9 51.3 76.9
61 45.2 37.0 55.6


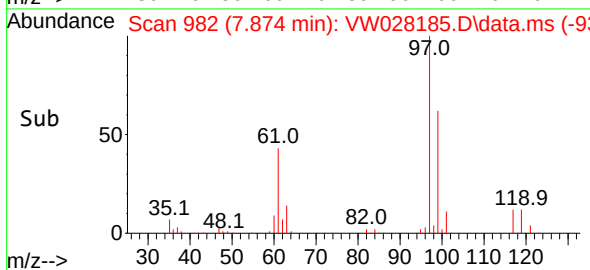

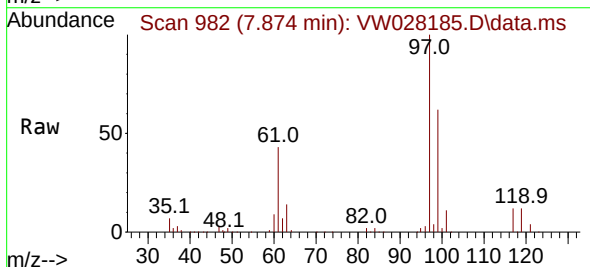


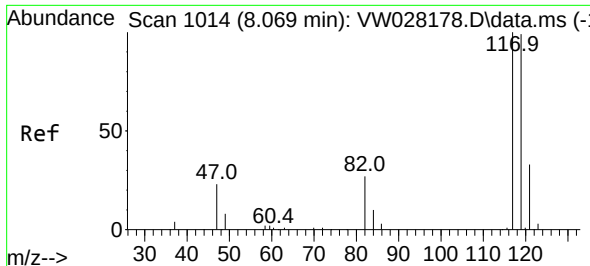

#31
Carbon tetrachloride
Concen: 23.755 ug/L
RT: 8.069 min Scan# 1014
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:117 Resp: 103058
Ion Ratio Lower Upper
117 100
119 97.4 78.2 117.4

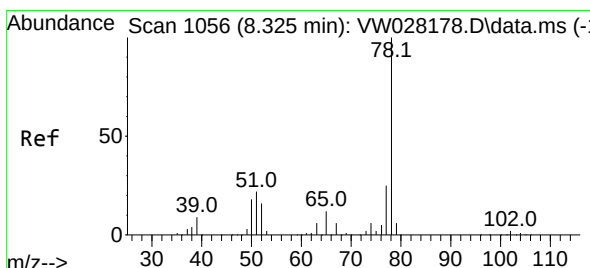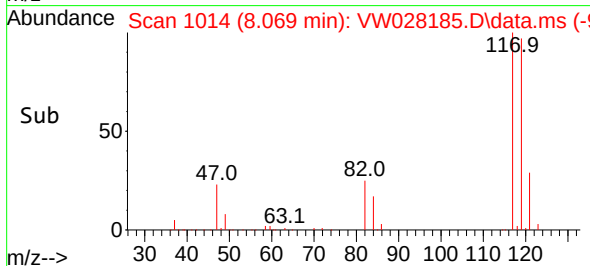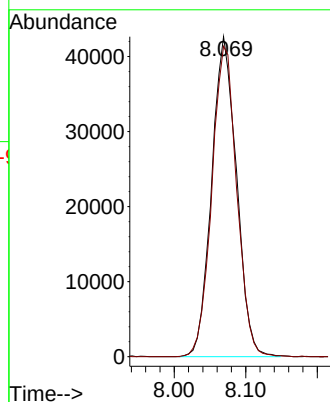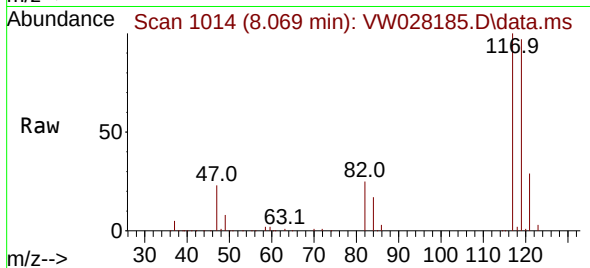

#33
Benzene
Concen: 24.849 ug/L
RT: 8.325 min Scan# 1056
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 78 Resp: 269796

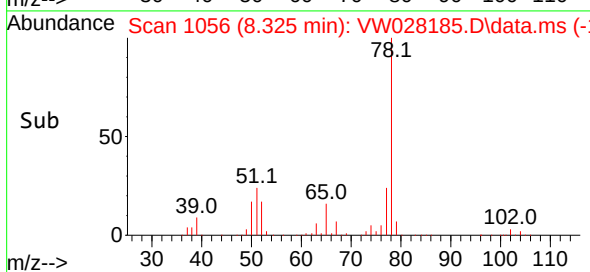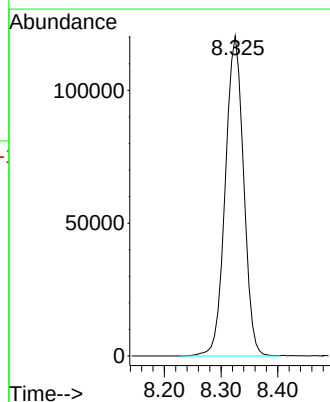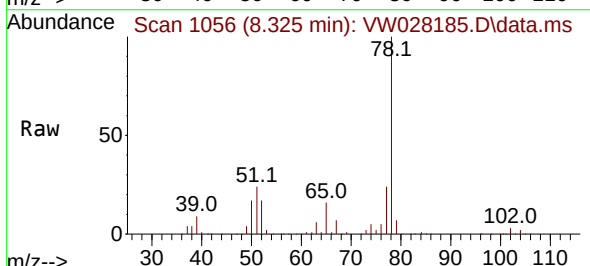

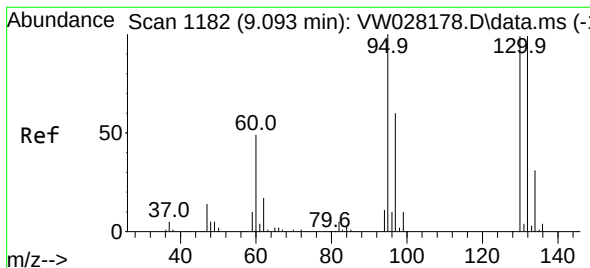

#34

Trichloroethene

Concen: 24.437 ug/L

RT: 9.093 min Scan# 1182

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion: 95 Resp: 74023





Ion Ratio Lower Upper

95 100

97 63.3 42.4 78.6

132 96.7 69.4 128.8

130 93.6 69.7 129.4

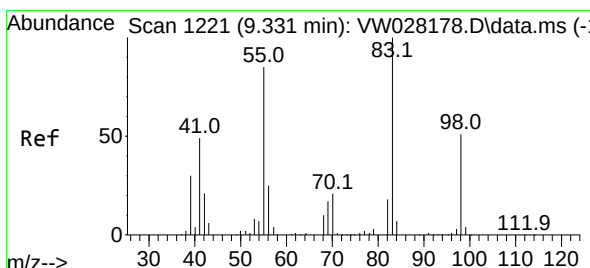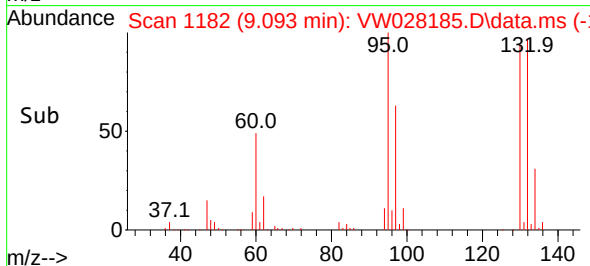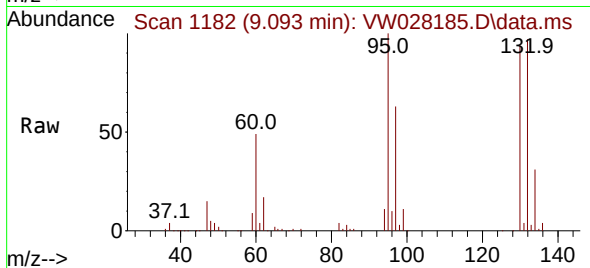

#35

Methylcyclohexane

Concen: 18.704 ug/L

RT: 9.331 min Scan# 1221

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51




Tgt Ion: 83 Resp: 95769


Ion Ratio Lower Upper

83 100

55 81.1 64.2 96.4

98 48.6 38.3 57.5

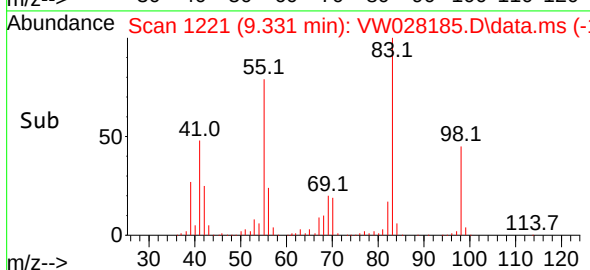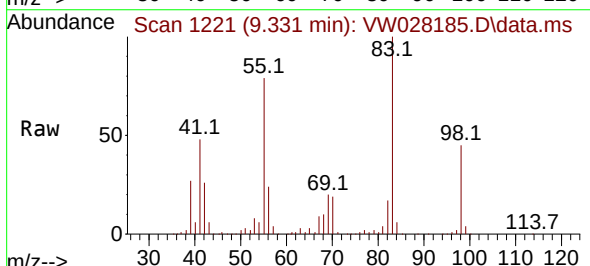



#37

1,2-Dichloropropane

Concen: 25.056 ug/L

RT: 9.367 min Scan# 11

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 63 Resp: 69582

Ion Ratio Lower Upper

63 100

112 4.5 3.8 5.8



#38

Bromodichloromethane

Concen: 25.574 ug/L

RT: 9.642 min Scan# 1272

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51




Tgt Ion: 83 Resp: 95753


Ion Ratio Lower Upper

83 100

85 62.2 45.8 85.2

127 7.5 6.5 9.7





#39

cis-1,3-Dichloropropene

Concen: 26.137 ug/L

RT: 10.069 min Scan# 11

Delta R.T. -0.006 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 75 Resp: 116243

Ion Ratio Lower Upper

75 100

77 32.7 22.5 41.7

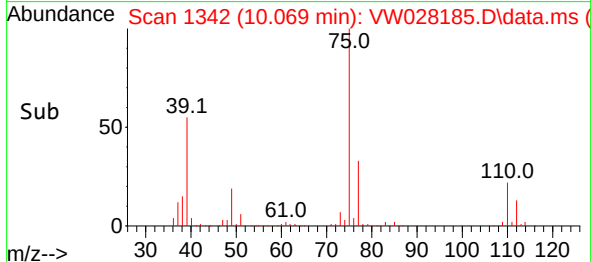

#40

4-Methyl-2-pentanone

Concen: 59.884 ug/L

RT: 10.209 min Scan# 1365

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51




Tgt Ion: 43 Resp: 91797


Ion Ratio Lower Upper

43 100

58 37.3 30.1 45.1

100 14.8 11.8 17.8




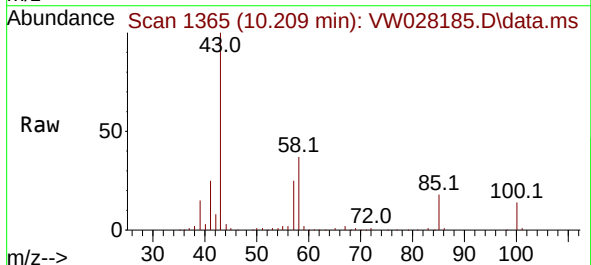




#42
Toluene
Concen: 24.349 ug/L
RT: 10.386 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 91 Resp: 288531
Ion Ratio Lower Upper
91 100
92 57.9 40.8 75.8

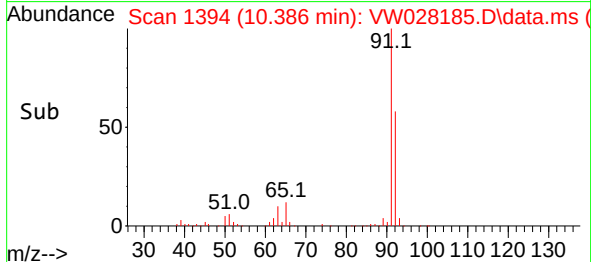

#44
trans-1,3-Dichloropropene
Concen: 26.685 ug/L
RT: 10.605 min Scan# 1430
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 75 Resp: 100201
Ion Ratio Lower Upper
75 100
77 29.4 23.0 42.6




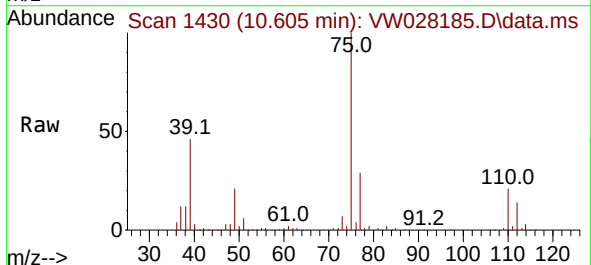




#45
1,1,2-Trichloroethane
Concen: 25.621 ug/L
RT: 10.788 min Scan# 1459
Delta R.T. 0.006 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:	97	Resp:	51408
Ion	Ratio	Lower	Upper
97	100		
99	61.6	43.4	80.6
83	85.3	59.4	110.4
85	52.5	38.4	71.4



#46
Tetrachloroethene
Concen: 91.225 ug/L
RT: 10.861 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion:	164	Resp:	222746
Ion	Ratio	Lower	Upper
164	100		
129	91.3	64.0	119.0
131	88.9	62.6	116.3
166	117.9	84.7	157.3

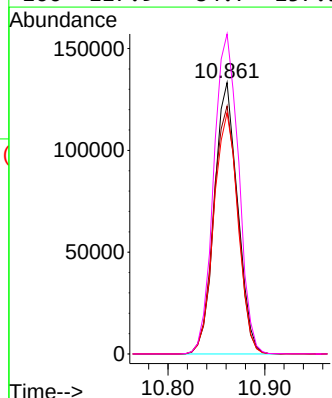



#48

2-Hexanone

Concen: 61.618 ug/L

RT: 10.965 min Scan# 1489

Delta R.T. 0.000 min


Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W

ClientSampleId :



Tgt Ion: 43 Resp: 73990




Ion Ratio Lower Upper

43 100

58 54.2 40.6 61.0

57 19.5 15.7 23.5

100 12.2 9.7 14.5



#49

Dibromochloromethane

Concen: 25.703 ug/L

RT: 11.123 min Scan# 1515

Delta R.T. 0.000 min

Lab File: VW028185.D




Acq: 14 Mar 2024 17:51


Tgt Ion: 129 Resp: 61078

Ion Ratio Lower Upper

129 100

127 72.7 53.1 98.7









#50
1,2-Dibromoethane
Concen: 25.698 ug/L
RT: 11.233 min Scan# 1533
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:107 Resp: 49304
Ion Ratio Lower Upper
107 100
109 96.6 64.4 119.6
188 3.8 3.4 5.2

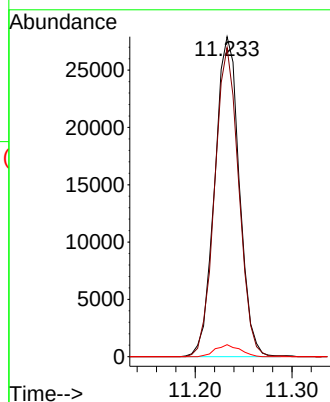

#51
Chlorobenzene
Concen: 23.447 ug/L
RT: 11.654 min Scan# 1602
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion:112 Resp: 176351
Ion Ratio Lower Upper
112 100
114 31.2 21.8 40.6
77 61.0 50.6 76.0


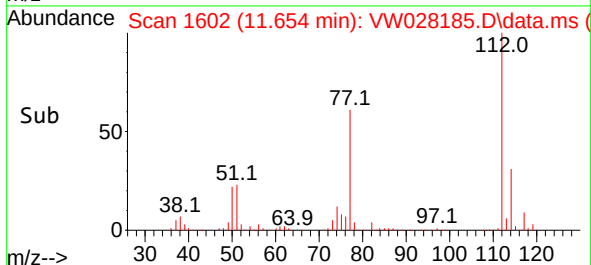






#52
Ethylbenzene
Concen: 23.090 ug/L
RT: 11.727 min Scan# 1614
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 91 Resp: 319397
Ion Ratio Lower Upper
91 100
106 30.0 21.3 39.5



#53
m,p-Xylene
Concen: 22.845 ug/L
RT: 11.836 min Scan# 1632
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 106 Resp: 118917
Ion Ratio Lower Upper
106 100
91 219.3 147.1 273.1









#54
o-Xylene
Concen: 23.380 ug/L
RT: 12.160 min Scan# 1
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:106 Resp: 112859
Ion Ratio Lower Upper
106 100
91 230.3 149.2 277.2



#55
Styrene
Concen: 23.335 ug/L
RT: 12.178 min Scan# 1688
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion:104 Resp: 193487
Ion Ratio Lower Upper
104 100
78 49.4 33.2 61.7





#57

1,1,2-Tetrachloroethane

Concen: 25.576 ug/L

RT: 12.708 min Scan# 1

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion: 83 Resp: 58698

Ion Ratio Lower Upper

83 100

85 61.7 47.0 87.2

131 10.8 8.9 13.3



#59

Bromoform

Concen: 31.880 ug/L

RT: 12.349 min Scan# 1716

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51




Tgt Ion:173 Resp: 36185


Ion Ratio Lower Upper

173 100

175 46.4 39.8 59.6


254 9.3 8.5 12.7








#60
Isopropylbenzene
Concen: 27.338 ug/L
RT: 12.458 min Scan# 1734
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Instrument :
MSVOA_W
ClientSampleId :







Tgt Ion:105 Resp: 307668
Ion Ratio Lower Upper
105 100
120 24.7 21.0 31.6
77 15.9 13.7 20.5



#61
1,2,3-Trichloropropane
Concen: 31.738 ug/L
RT: 12.763 min Scan# 1784
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion: 75 Resp: 45882
Ion Ratio Lower Upper
75 100
77 32.1 26.0 39.0
110 39.1 32.2 48.2

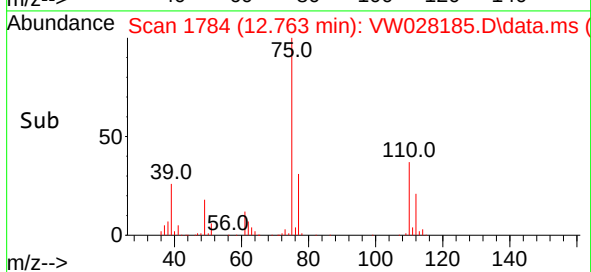



#62

1,3,5-Trimethylbenzene

Concen: 24.684 ug/L

RT: 12.940 min Scan# 1813

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion:105 Resp: 186395

Ion Ratio Lower Upper

105 100

120 47.6 38.2 57.2



#63

1,2,4-Trimethylbenzene

Concen: 25.137 ug/L

RT: 13.245 min Scan# 1863

Delta R.T. 0.000 min

Lab File: VW028185.D




Acq: 14 Mar 2024 17:51


Tgt Ion:105 Resp: 229197

Ion Ratio Lower Upper

105 100


120 43.9 35.6 53.4








#64
1,3-Dichlorobenzene
Concen: 22.881 ug/L
RT: 13.495 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Instrument :
MSVOA_W
ClientSampleId :







Tgt Ion:146 Resp: 114881
Ion Ratio Lower Upper
146 100
111 42.6 28.5 52.9
148 61.4 43.0 80.0



#65
1,4-Dichlorobenzene
Concen: 23.607 ug/L
RT: 13.574 min Scan# 1917
Delta R.T. 0.000 min
Lab File: VW028185.D
Acq: 14 Mar 2024 17:51

Tgt Ion:146 Resp: 118521
Ion Ratio Lower Upper
146 100
111 38.7 28.8 53.6
148 57.9 45.3 84.1

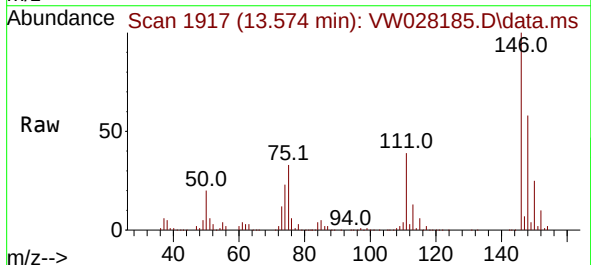



#67

1,2-Dichlorobenzene

Concen: 23.439 ug/L

RT: 13.867 min Scan# 1965

Delta R.T. 0.006 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion:146 Resp: 101345

Ion Ratio Lower Upper

146 100

111 41.8 34.2 51.2

148 68.0 48.1 72.1



#68

1,2-Dibromo-3-chloropropane

Concen: 29.070 ug/L

RT: 14.476 min Scan# 2065

Delta R.T. 0.000 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51




Tgt Ion: 75 Resp: 9872


Ion Ratio Lower Upper

75 100

155 72.6 61.1 91.7


157 89.4 74.2 111.4

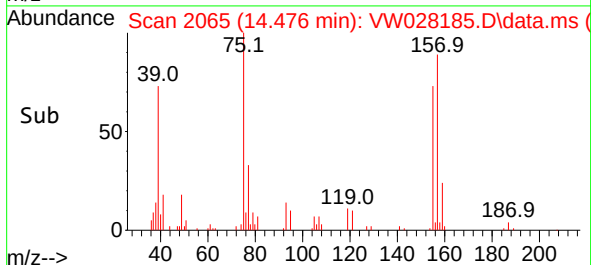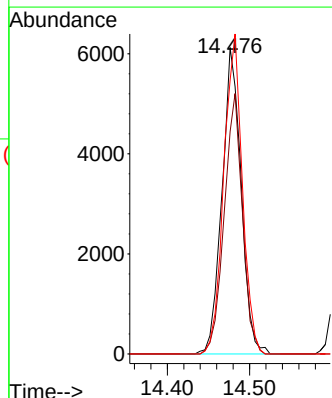






#69
 1,3,5-Trichlorobenzene
 Concen: 15.504 ug/L
 RT: 14.623 min Scan# 2089
 Delta R.T. 0.000 min
 Lab File: VW028185.D
 Acq: 14 Mar 2024 17:51

Instrument :
 MSVOA_W
 ClientSampleId :







Tgt Ion:180	Resp:	54223
Ion Ratio	Lower	Upper
180	100	
182	93.6	76.6 114.8
184	29.2	23.5 35.3
145	30.0	24.9 37.3



#70
 1,2,4-trichlorobenzene
 Concen: 13.687 ug/L
 RT: 15.129 min Scan# 2172
 Delta R.T. 0.000 min
 Lab File: VW028185.D
 Acq: 14 Mar 2024 17:51

Tgt Ion:180	Resp:	40666
Ion Ratio	Lower	Upper
180	100	
182	97.2	73.8 110.8
145	31.9	25.0 37.6

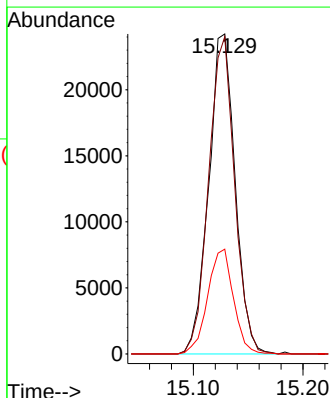



#71

Naphthalene

Concen: 20.258 ug/L

RT: 15.360 min Scan# 2210

Delta R.T. 0.006 min


Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Instrument :

MSVOA_W

ClientSampleId :






Tgt Ion:128 Resp: 103306

Ion Ratio Lower Upper

128 100

127 13.4 10.9 16.3

129 10.5 8.9 13.3



#72

1,2,3-Trichlorobenzene

Concen: 13.023 ug/L

RT: 15.549 min Scan# 2241

Delta R.T. 0.006 min

Lab File: VW028185.D

Acq: 14 Mar 2024 17:51

Tgt Ion:180 Resp: 31897

Ion Ratio Lower Upper

180 100

182 95.1 76.0 114.0

145 33.4 27.1 40.7

