
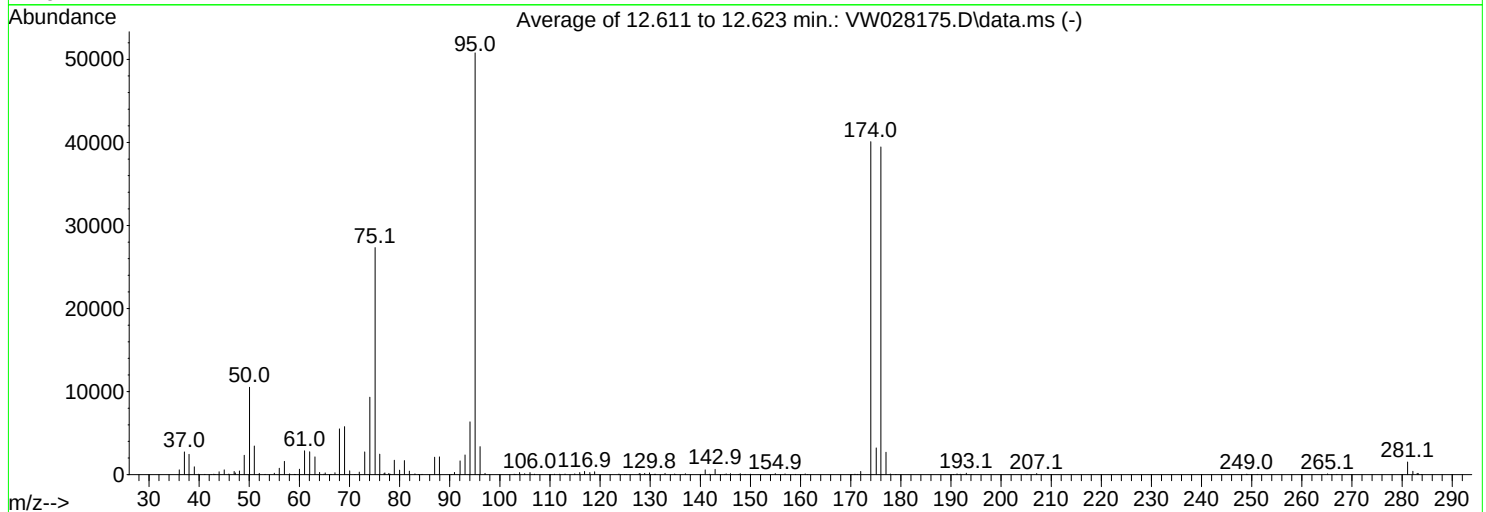


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031424\
Data File : VW028175.D
Acq On : 14 Mar 2024 12:27
Operator : SY/MD
Sample : BFB453
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB453

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Title : SFAM01.0
Last Update : Fri Mar 15 01:46:51 2024

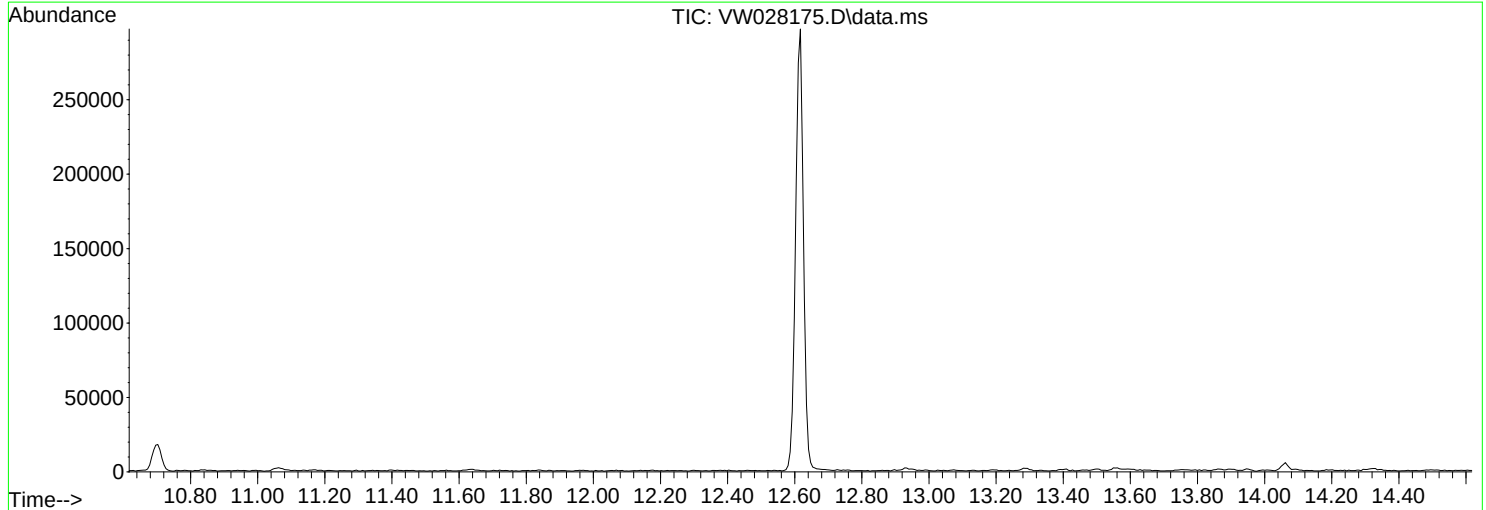

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	10529	PASS
75	95	30	80	53.8	27333	PASS
95	95	100	100	100.0	50787	PASS
96	95	5	9	6.6	3366	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.0	40099	PASS
175	174	5	9	8.0	3224	PASS
176	174	95	101	98.4	39459	PASS
177	176	5	9	6.8	2693	PASS

m/z	Abundance
36.20	66.0
37.70	52.0
38.30	79.0
39.90	177.0
44.20	85.0
48.40	64.0
56.10	62.0
56.90	57.0
61.60	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

m/z	Abundance
36.00	658.0
37.00	3210.0
38.00	2764.0
39.00	955.0
40.10	255.0
42.40	55.0
43.00	53.0
43.20	52.0
44.00	375.0
45.00	687.0
46.00	72.0
47.00	727.0
48.10	441.0
49.00	2727.0
50.00	12175.0
51.00	3951.0
51.90	190.0
53.10	53.0
55.10	170.0
56.00	839.0
57.00	1687.0
58.10	128.0
59.00	95.0
60.00	635.0
61.10	3147.0
62.10	2827.0
63.10	2457.0
64.00	290.0
65.20	402.0
66.30	52.0
67.10	232.0
68.00	6025.0
69.00	6214.0
70.10	456.0
71.90	377.0
73.00	3182.0
74.10	10455.0
75.10	30744.0
76.10	2603.0
76.90	410.0
77.90	287.0
79.00	2048.0
80.00	607.0
81.00	1976.0
81.90	411.0
83.10	96.0
87.00	2277.0
88.00	2617.0
90.90	270.0
92.00	1745.0
93.10	2649.0
94.10	6424.0
95.10	53528.0
96.10	3545.0
97.10	152.0
103.20	122.0
104.00	304.0
105.00	139.0
106.10	249.0
106.90	86.0
109.90	68.0
110.90	99.0
111.90	89.0
113.00	76.0
114.90	109.0
116.10	250.0
116.90	425.0
117.90	251.0
118.90	294.0
123.80	94.0
125.20	72.0
127.80	241.0
128.90	179.0
130.00	154.0
130.80	88.0
131.20	67.0
133.00	204.0
134.90	96.0
137.10	141.0
140.00	77.0
140.90	624.0
142.00	86.0
143.00	702.0
144.00	63.0
145.20	152.0
146.00	111.0
147.70	136.0
148.90	94.0
152.10	56.0
155.00	145.0
157.10	112.0
159.00	109.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

160.90	110.0
170.90	89.0
172.10	377.0
174.00	39592.0
175.10	3237.0
176.00	35328.0
177.00	2754.0
178.00	103.0
179.00	59.0
190.50	57.0
191.20	128.0
191.80	70.0
193.10	312.0
194.10	76.0
205.10	69.0
207.10	193.0
208.10	71.0
249.00	149.0
251.10	108.0
265.10	146.0
265.90	81.0
267.00	109.0
281.10	2719.0
282.20	627.0
283.00	471.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

m/z	Abundance
36.10	809.0
37.10	2955.0
38.00	2860.0
39.00	1065.0
40.10	244.0
41.20	64.0
42.90	119.0
44.00	427.0
45.00	578.0
45.90	100.0
47.20	639.0
48.00	607.0
49.00	2351.0
50.00	11442.0
51.00	3903.0
52.00	150.0
55.00	238.0
56.00	1046.0
57.10	1947.0
58.10	57.0
59.20	76.0
60.00	629.0
61.00	3415.0
62.00	3173.0
63.10	2387.0
64.00	285.0
65.10	224.0
66.30	69.0
67.10	223.0
68.00	6156.0
69.00	6417.0
70.10	569.0
71.10	72.0
72.00	308.0
73.10	2893.0
74.10	10136.0
75.10	30616.0
76.00	2978.0
77.10	419.0
77.80	187.0
78.90	1798.0
80.00	575.0
80.90	1540.0
82.00	513.0
83.00	116.0
83.80	52.0
84.40	66.0
87.00	2472.0
87.90	2188.0
90.40	79.0
91.00	320.0
92.00	1855.0
93.00	2673.0
94.10	7337.0
95.00	57776.0
96.00	3708.0
97.00	181.0
102.90	72.0
103.90	270.0
104.90	110.0
106.00	241.0
106.90	95.0
110.10	52.0
110.90	72.0
112.00	108.0
113.00	93.0
115.00	78.0
115.90	298.0
116.90	451.0
118.00	271.0
119.00	435.0
123.70	80.0
124.90	83.0
128.00	307.0
128.80	146.0
129.80	247.0
131.00	119.0
132.90	235.0
135.10	117.0
136.90	147.0
140.10	54.0
141.00	682.0
141.80	66.0
143.00	787.0
145.10	160.0
146.00	164.0
147.90	225.0
150.00	85.0
154.90	141.0
156.90	72.0
160.90	95.0
161.40	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

170.20	58.0
171.90	352.0
174.00	46776.0
175.10	3849.0
176.00	47696.0
177.10	3060.0
177.90	62.0
191.20	103.0
191.80	64.0
193.00	174.0
205.20	73.0
207.10	146.0
249.20	146.0
265.20	168.0
281.10	1094.0
282.10	500.0
283.20	341.0
283.90	56.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

m/z	Abundance
36.00	445.0
37.10	2040.0
38.10	1710.0
39.10	806.0
39.90	230.0
41.10	70.0
43.10	93.0
44.00	466.0
45.00	495.0
46.00	72.0
47.00	458.0
48.00	272.0
49.00	1916.0
50.10	7969.0
51.10	2480.0
52.10	127.0
53.20	70.0
54.90	129.0
56.00	614.0
57.00	1334.0
57.90	83.0
60.00	707.0
61.00	2036.0
62.10	2270.0
63.00	1553.0
64.10	259.0
64.90	196.0
67.10	230.0
68.00	4329.0
69.00	4717.0
70.00	353.0
71.90	245.0
73.00	2110.0
74.00	7406.0
75.10	20640.0
76.00	1844.0
77.00	201.0
78.10	164.0
78.90	1380.0
80.00	451.0
81.00	1594.0
82.00	360.0
83.00	92.0
84.50	64.0
87.00	1554.0
88.00	1619.0
90.90	241.0
92.10	1391.0
93.00	1816.0
94.00	5306.0
95.10	41056.0
96.10	2844.0
97.00	138.0
102.80	83.0
103.90	172.0
104.90	83.0
105.90	249.0
113.00	72.0
114.90	94.0
115.80	193.0
116.80	259.0
118.00	224.0
118.80	331.0
123.70	57.0
127.80	160.0
129.00	131.0
129.80	210.0
130.80	115.0
134.80	131.0
136.90	71.0
141.00	447.0
142.80	425.0
144.90	117.0
145.90	91.0
148.00	150.0
148.90	54.0
150.00	67.0
154.90	103.0
156.80	111.0
160.90	67.0
170.80	89.0
171.30	120.0
172.00	427.0
174.00	33928.0
175.10	2586.0
176.00	35352.0
177.00	2264.0
177.80	94.0
191.20	77.0
191.90	60.0
193.00	54.0
207.10	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

281.20

282.10

283.20

748.0

96.0

135.0

Instrument :

MSVOA_W

ClientSampleId :

BFB453