

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031524\
 Data File : VW028206.D
 Acq On : 15 Mar 2024 12:29
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK413

Quant Time: Mar 18 01:31:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 18 01:23:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	189132	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	177188	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	89812	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	54989	24.849	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.400%
7) Chloroethane-d5	2.905	69	40098	25.936	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.760%
11) 1,1-Dichloroethene-d2	4.027	65	35863	25.556	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	102.240%
21) 2-Butanone-d5	7.075	46	39968	61.236	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.480%
24) Chloroform-d	7.648	84	158471	28.415	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	113.640%
26) 1,2-Dichloroethane-d4	8.307	65	93637	30.467	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	121.880%
32) Benzene-d6	8.276	84	310931	28.742	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	114.960%
36) 1,2-Dichloropropane-d6	9.276	67	90088	28.938	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.760%
41) Toluene-d8	10.325	98	289214	28.984	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	115.920%
43) trans-1,3-Dichloroprop...	10.575	79	39749	28.112	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	112.440%
47) 2-Hexanone-d5	10.922	63	32394	62.951	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.900%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	67896	29.524	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	118.080%
66) 1,2-Dichlorobenzene-d4	13.848	152	99233	30.331	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	121.320%#
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3014	0.675	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031524\
Data File : VW028206.D
Acq On : 15 Mar 2024 12:29
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK413

Quant Time: Mar 18 01:31:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 18 01:23:58 2024
Response via : Initial Calibration

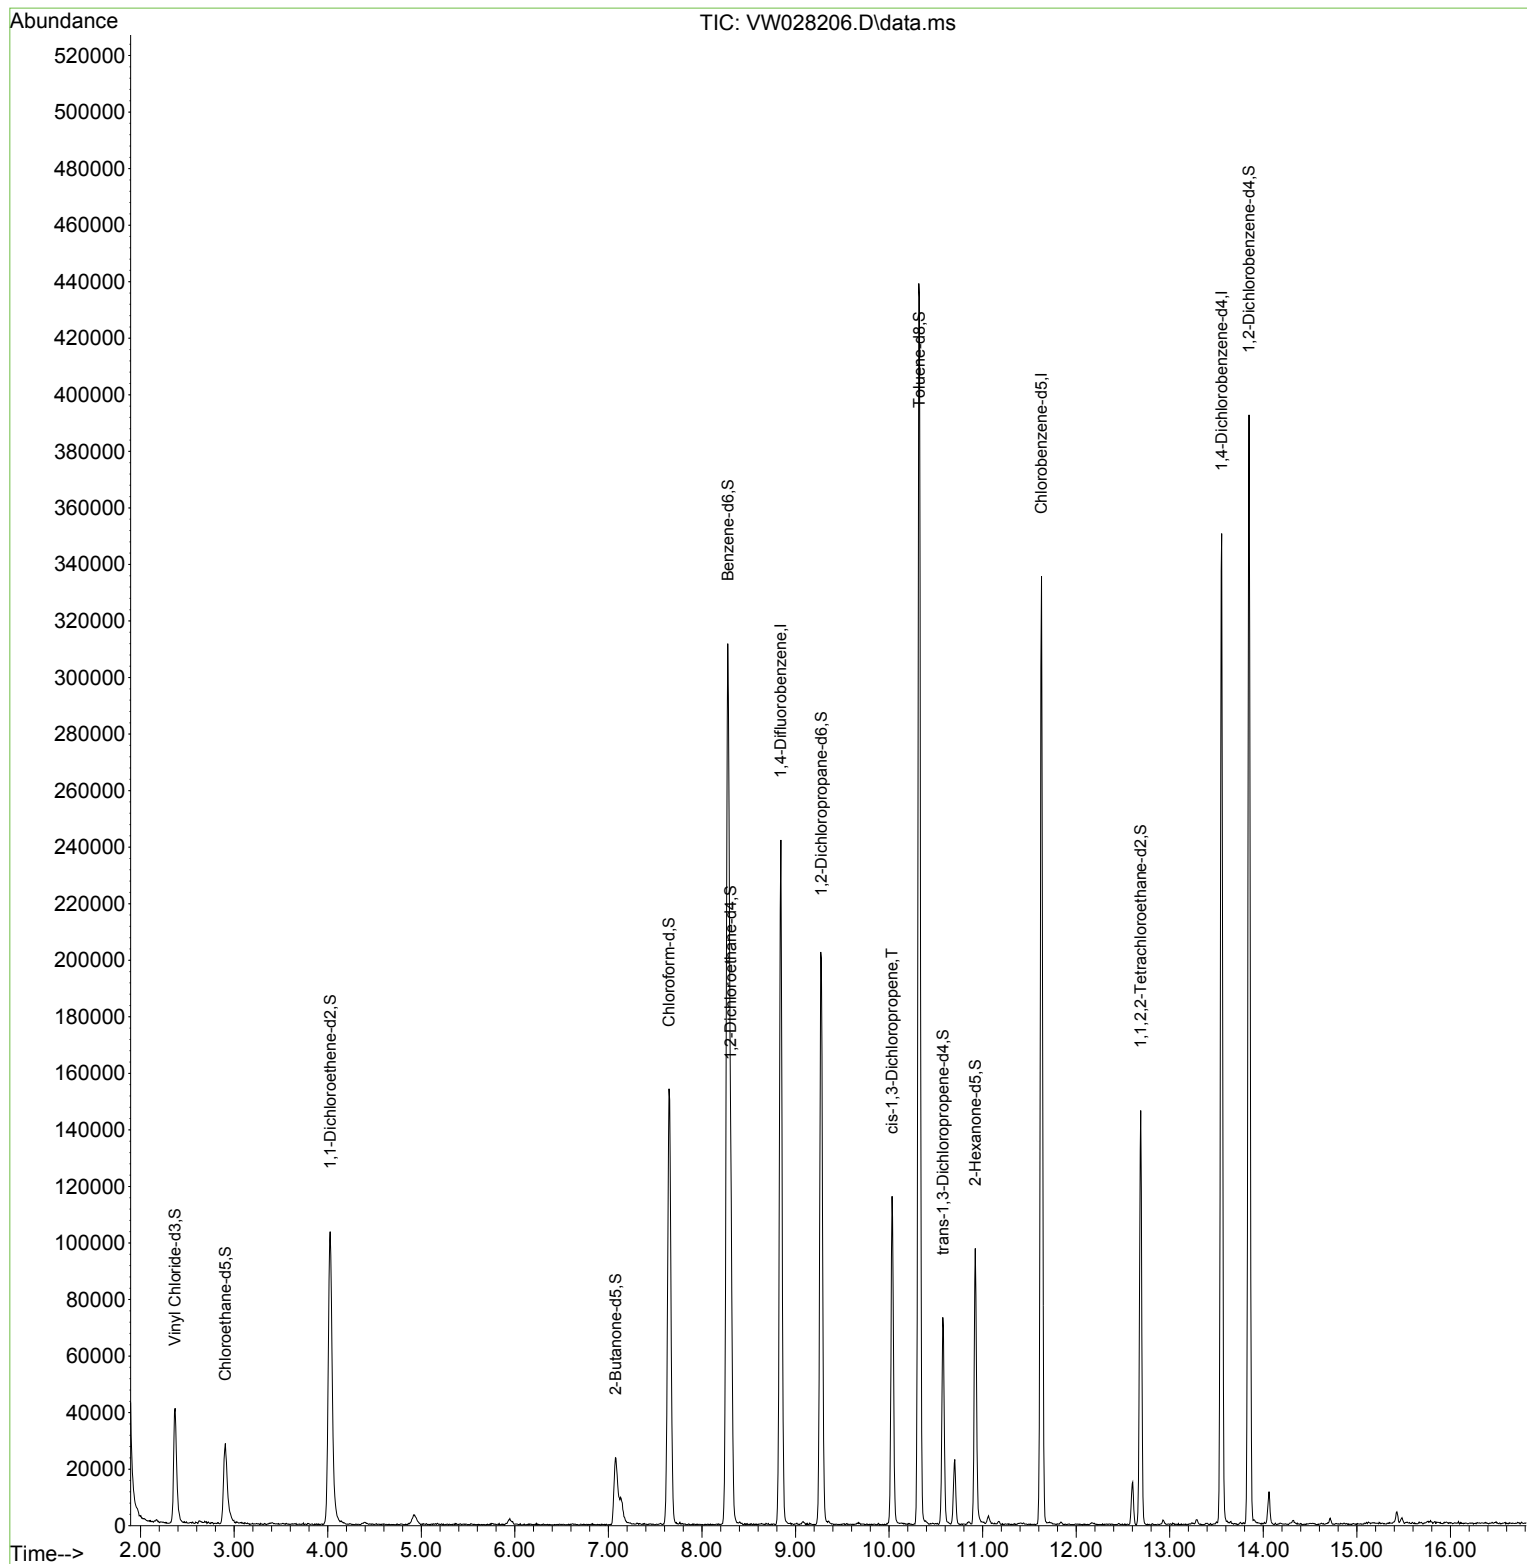

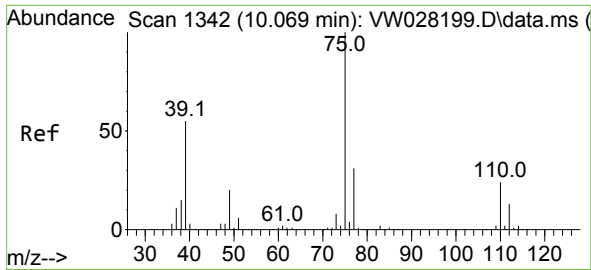

#39
 cis-1,3-Dichloropropene
 Concen: 0.675 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW028206.D
 Acq: 15 Mar 2024 12:29

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK413

Tgt Ion: 75 Resp: 3014
 Ion Ratio Lower Upper
 75 100
 77 49.5 22.5 41.7#

