

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031524\
 Data File : VW028208.D
 Acq On : 15 Mar 2024 13:52
 Operator : SY/MD
 Sample : P1742-13
 Misc : 4.99g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Mar 18 01:32:25 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 18 01:23:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	221248	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	199677	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	101173	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	46439	17.939	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.760%
7) Chloroethane-d5	2.899	69	34573	19.116	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.480%
11) 1,1-Dichloroethene-d2	4.027	65	30840	18.787	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.160%
21) 2-Butanone-d5	7.081	46	33539	43.927	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.860%
24) Chloroform-d	7.648	84	133190	20.415	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.680%
26) 1,2-Dichloroethane-d4	8.307	65	79605	22.142	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.560%
32) Benzene-d6	8.276	84	263024	21.575	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.320%
36) 1,2-Dichloropropane-d6	9.276	67	76313	21.752	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.000%
41) Toluene-d8	10.325	98	244254	21.722	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.880%
43) trans-1,3-Dichloroprop...	10.575	79	33372	20.944	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.760%
47) 2-Hexanone-d5	10.922	63	25576	44.104	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	57922	22.350	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.400%
66) 1,2-Dichlorobenzene-d4	13.848	152	83562	22.673	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.680%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	2667	0.530	ug/L	Qvalue # 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031524\
Data File : VW028208.D
Acq On : 15 Mar 2024 13:52
Operator : SY/MD
Sample : P1742-13
Misc : 4.99g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Mar 18 01:32:25 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 18 01:23:58 2024
Response via : Initial Calibration

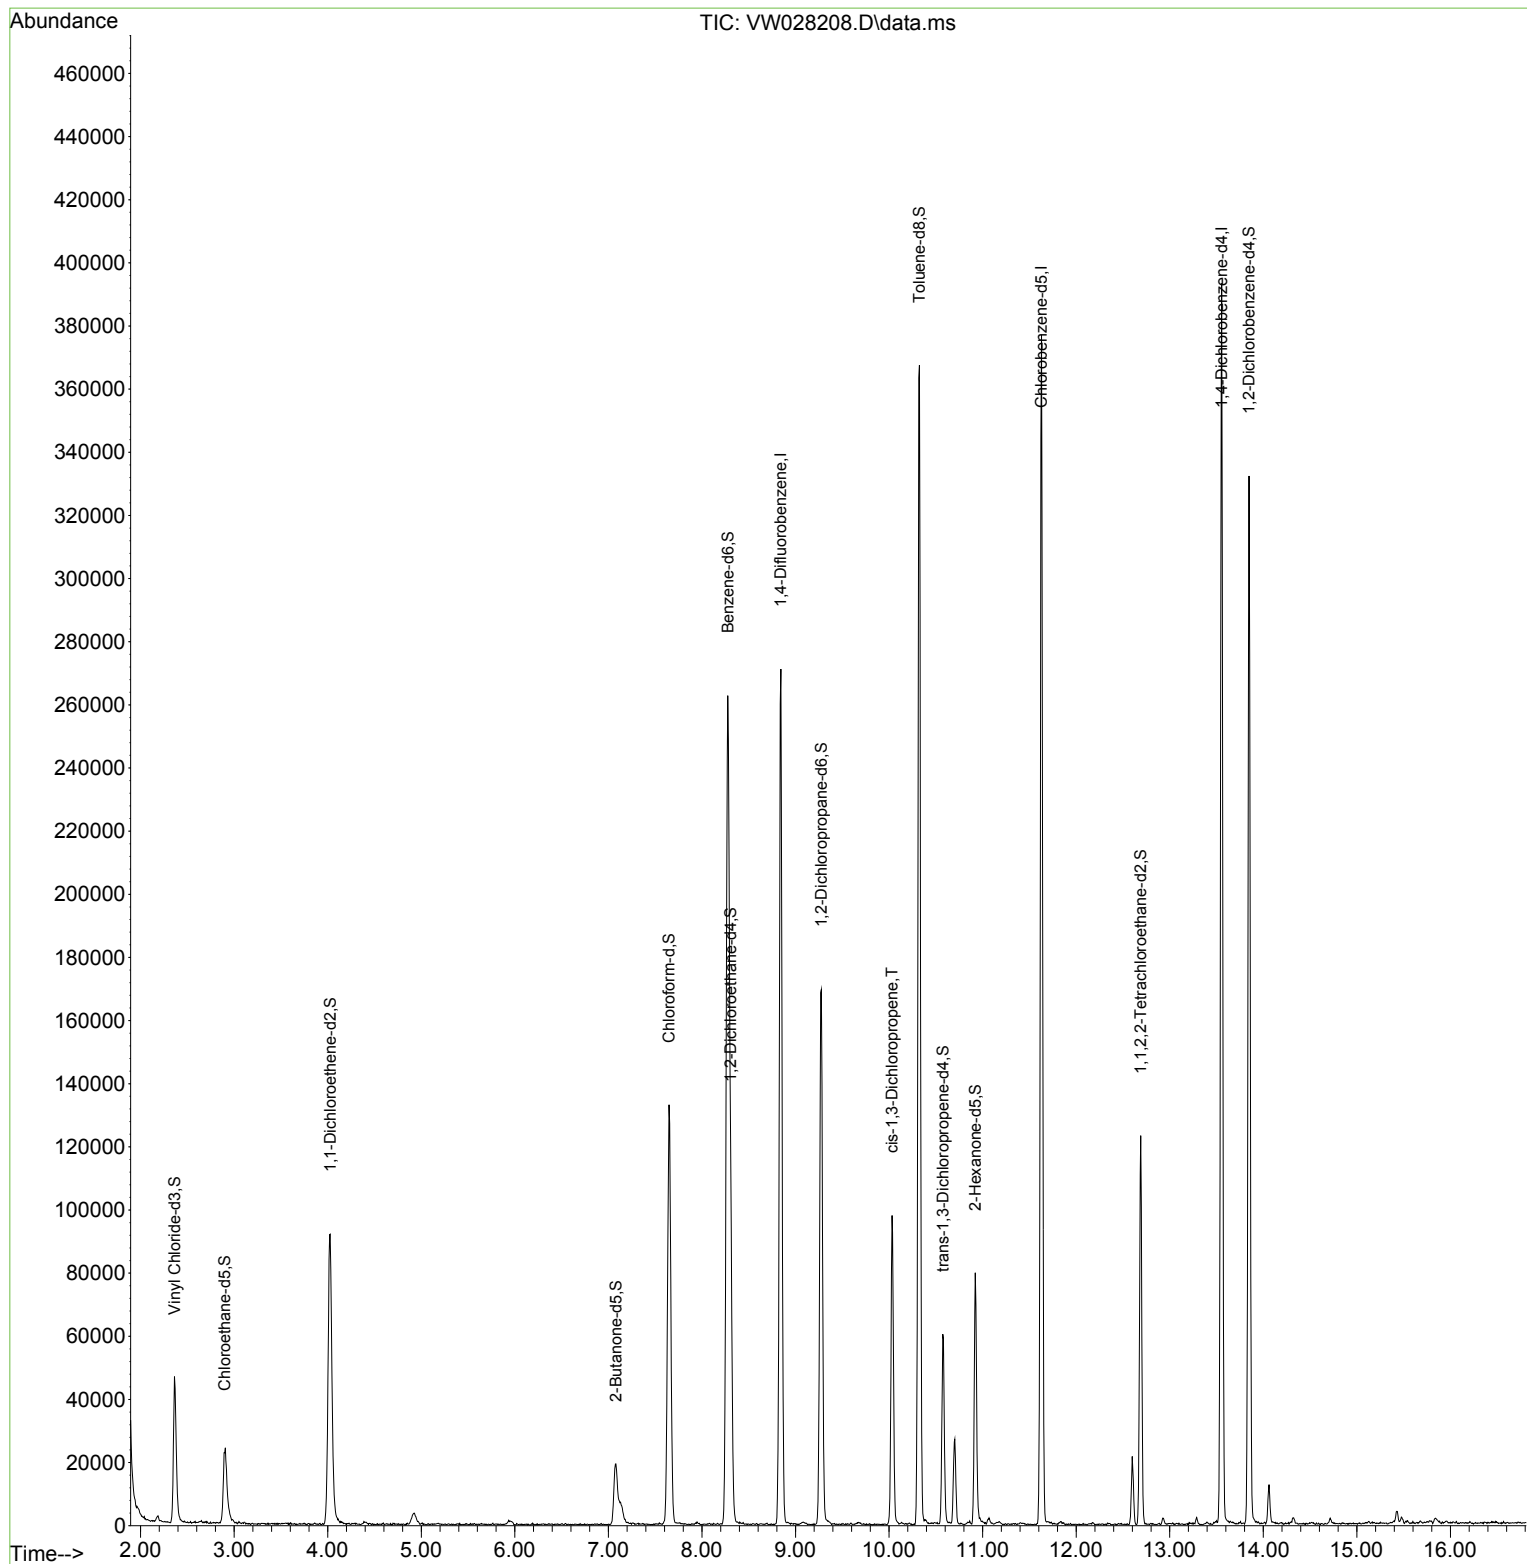

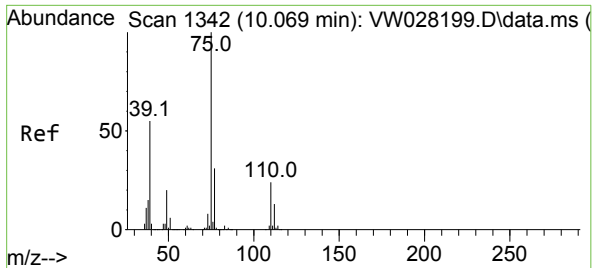

#39
 cis-1,3-Dichloropropene
 Concen: 0.530 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW028208.D
 Acq: 15 Mar 2024 13:52

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Tgt Ion: 75 Resp: 2667
 Ion Ratio Lower Upper
 75 100
 77 48.6 22.5 41.7#

