

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031623\
 Data File : VW025402.D
 Acq On : 16 Mar 2023 18:30
 Operator : SY/MD
 Sample : 01927-15
 Misc : 6.84g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DCAR0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/17/2023
 Supervised By :Mahesh Dadoda 03/17/2023

Quant Time: Mar 17 01:38:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 17 01:35:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	955622	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	784246	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	306644	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	199370	12.548	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	50.200%		
7) Chloroethane-d5	2.899	69	206250	18.040	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.160%		
11) 1,1-Dichloroethene-d2	4.027	63	421538	13.736	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	54.960%		
21) 2-Butanone-d5	7.075	46	172057	44.116	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.240%		
24) Chloroform-d	7.648	84	610997	22.178	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.720%		
26) 1,2-Dichloroethane-d4	8.307	65	343190m	23.209	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.840%		
32) Benzene-d6	8.276	84	1281648	23.917	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.680%		
36) 1,2-Dichloropropane-d6	9.270	67	405368	24.453	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	97.800%		
41) Toluene-d8	10.319	98	1088958	23.048	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	92.200%		
43) trans-1,3-Dichloroprop...	10.575	79	140540	21.290	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.160%		
47) 2-Hexanone-d5	10.922	63	113325	47.539	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.080%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	282983	23.300	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.200%		
66) 1,2-Dichlorobenzene-d4	13.848	152	264278	23.176	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.720%		
Target Compounds					Qvalue	
13) Acetone	4.125	43	36767	9.807	ug/L	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031623\
Data File : VW025402.D
Acq On : 16 Mar 2023 18:30
Operator : SY/MD
Sample : 01927-15
Misc : 6.84g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DCAR0

Quant Time: Mar 17 01:38:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 17 01:35:38 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/17/2023
Supervised By :Mahesh Dadoda 03/17/2023

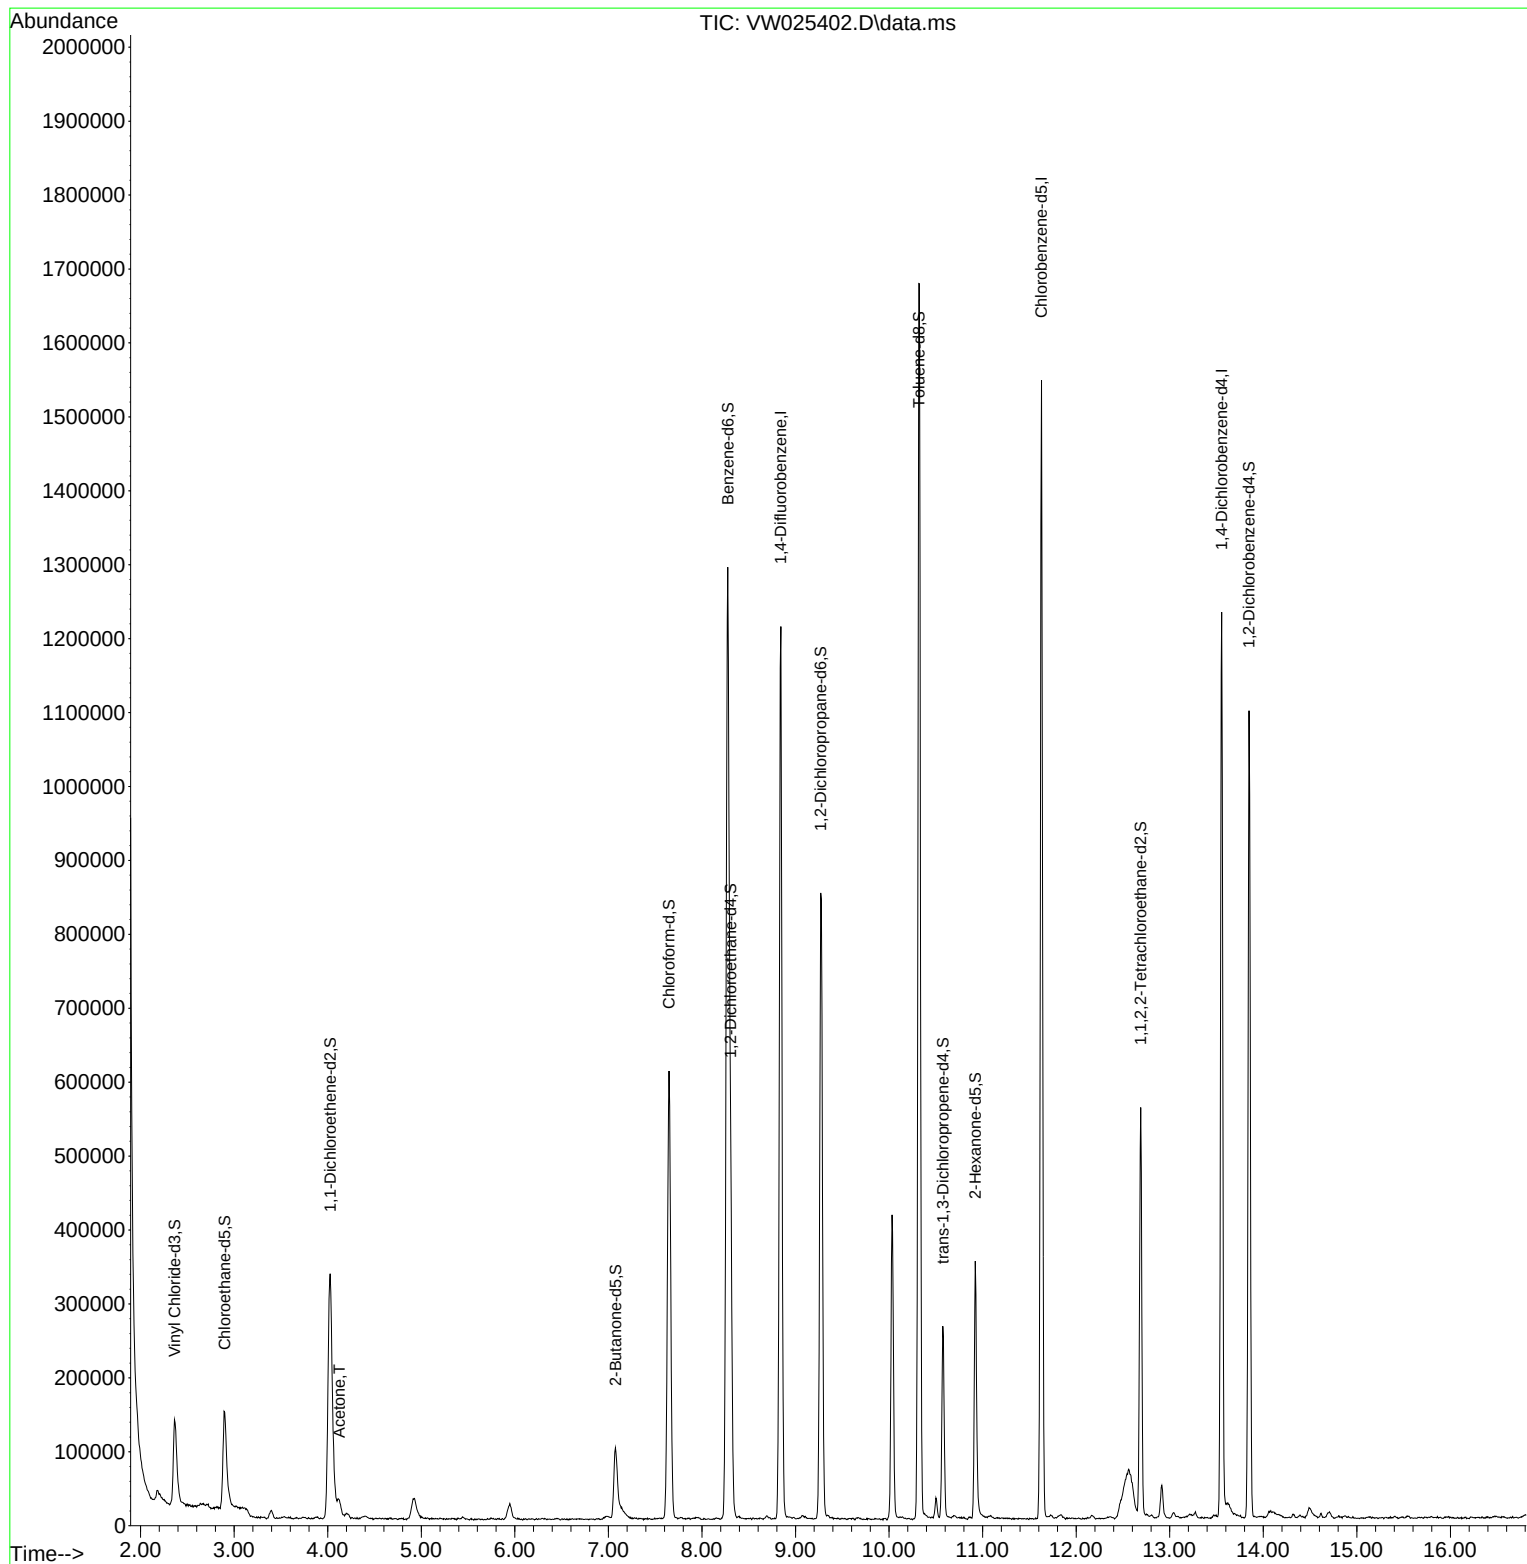

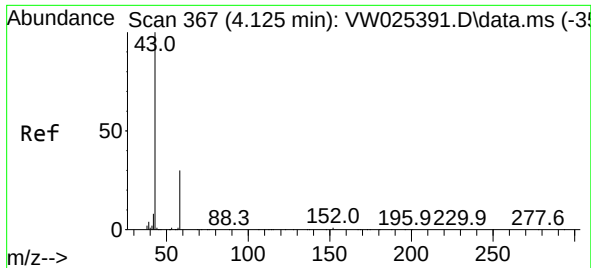

#13
Acetone
Concen: 9.807 ug/L
RT: 4.125 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW025402.D
Acq: 16 Mar 2023 18:30

Instrument :
MSVOA_W
ClientSampleId :
DCAR0

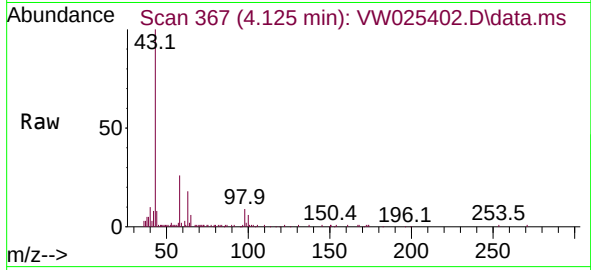

Tgt Ion: 43 Resp: 3676
Ion Ratio Lower Upper
43 100
58 15.0 0.0 60.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/17/2023
Supervised By :Mahesh Dadoda 03/17/2023

