
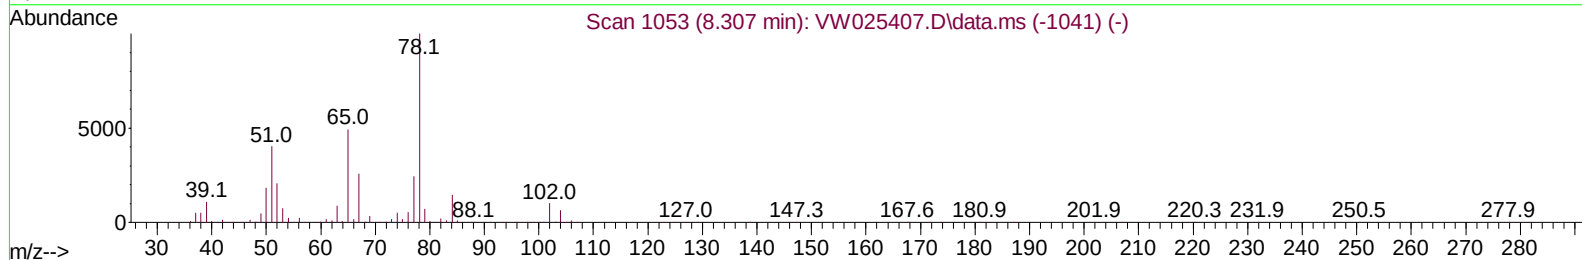
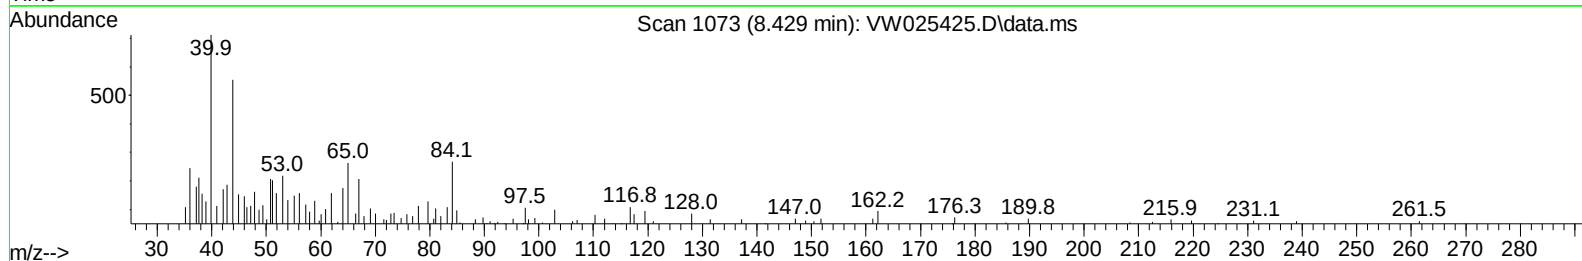


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031723\
Data File : VW025425.D
Acq On : 17 Mar 2023 19:19
Operator : SY/MD
Sample : 01977-12
Misc : 6.80g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 21:44:11 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 17 21:39:25 2023
Response via : Initial Calibration

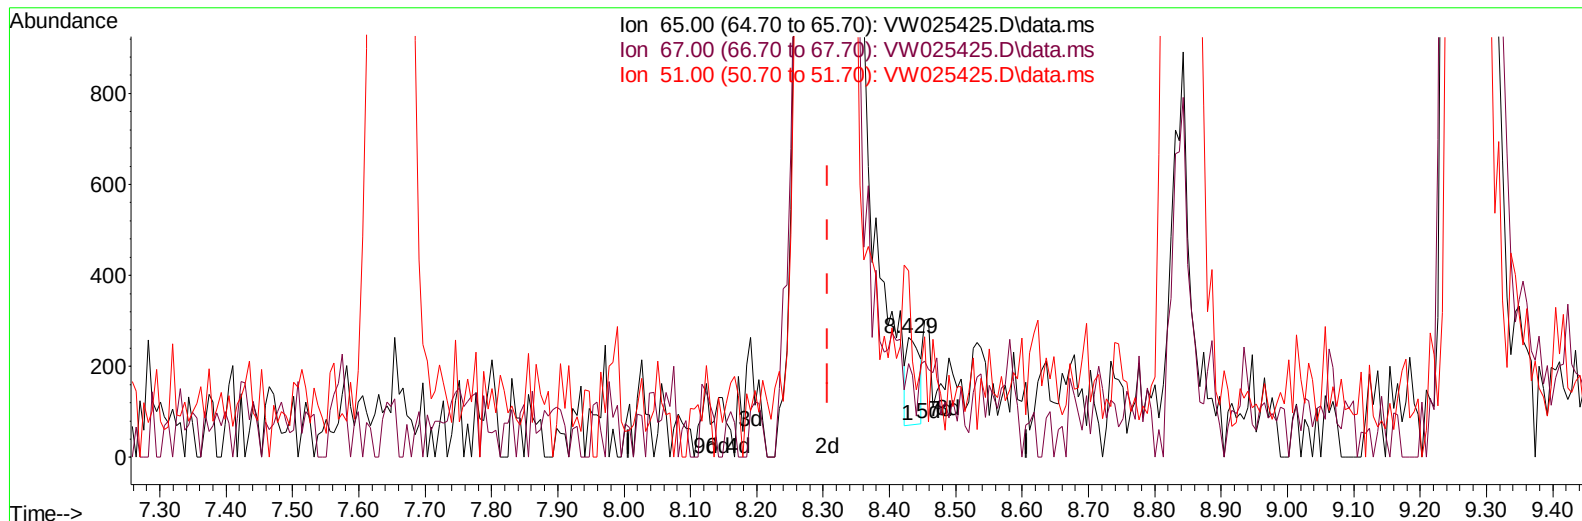

TIC: VW025425.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.429min (+ 0.122) 0.02 ug/L

response 251

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	39.04
51.00	111.10	101.59
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031723\
 Data File : VW025425.D
 Acq On : 17 Mar 2023 19:19
 Operator : SY/MD
 Sample : 01977-12
 Misc : 6.80g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 21:44:11 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 17 21:39:25 2023
 Response via : Initial Calibration

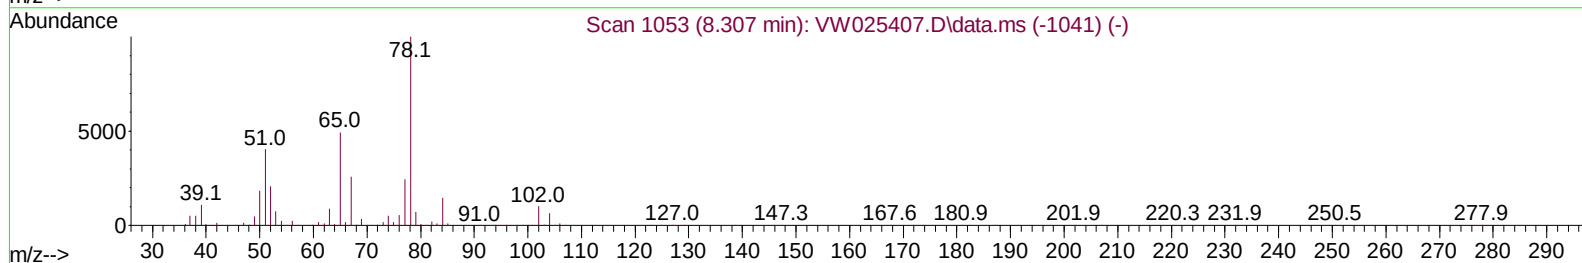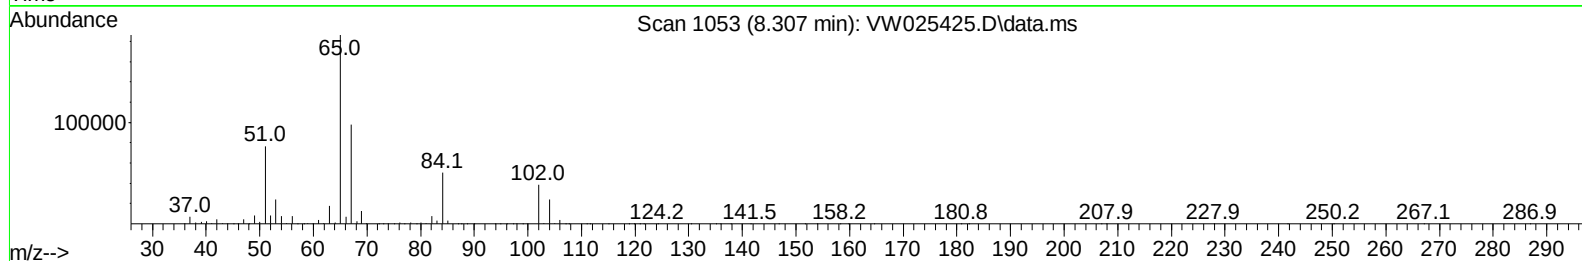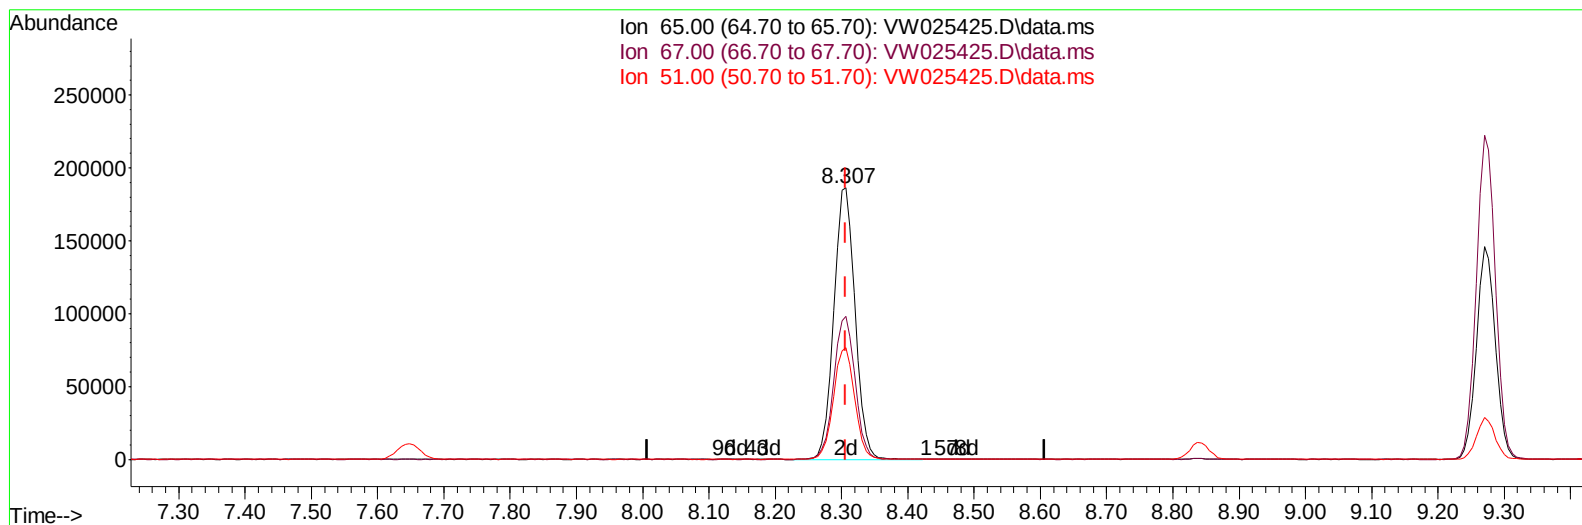

TIC: VW025425.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.307min (+ 0.000) 25.01 ug/L m****response 414398**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	0.02#
51.00	111.10	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031723\
 Data File : VW025426.D
 Acq On : 17 Mar 2023 19:43
 Operator : SY/MD
 Sample : 01977-13
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 21:44:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 17 21:39:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1065499	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	891278	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	307041	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	201850	11.394	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	45.560%	
7) Chloroethane-d5	2.899	69	199765	15.671	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	62.680%	
11) 1,1-Dichloroethene-d2	4.021	63	441310	12.897	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	51.600%	
21) 2-Butanone-d5	7.075	46	255670	58.794	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	117.580%	
24) Chloroform-d	7.648	84	661474	21.535	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	86.120%	
26) 1,2-Dichloroethane-d4	8.307	65	402058	24.387	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.560%	
32) Benzene-d6	8.276	84	1358487	22.307	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	89.240%	
36) 1,2-Dichloropropane-d6	9.270	67	451947	23.988	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	95.960%	
41) Toluene-d8	10.319	98	1200695	22.362	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	89.440%	
43) trans-1,3-Dichloroprop...	10.575	79	178623	23.810	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	95.240%	
47) 2-Hexanone-d5	10.922	63	179670	66.319	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	132.640%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	371294	26.900	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	107.600%	
66) 1,2-Dichlorobenzene-d4	13.855	152	266089	23.304	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	93.200%	
Target Compounds						
16) Methylene chloride	4.917	84	131085	8.835	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW031723\
Data File : VW025426.D
Acq On : 17 Mar 2023 19:43
Operator : SY/MD
Sample : 01977-13
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 21:44:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 17 21:39:25 2023
Response via : Initial Calibration

