

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025437.D
 Acq On : 20 Mar 2023 12:50
 Operator : SY/MD
 Sample : 01977-20
 Misc : 7.65g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGA5

Quant Time: Mar 20 23:52:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	847735	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	668496	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	206986	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	163962	11.632	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	46.520%
7) Chloroethane-d5	2.899	69	161116	15.886	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.560%
11) 1,1-Dichloroethene-d2	3.777	63	168	0.006	ug/L	-0.24
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.040%#
21) 2-Butanone-d5	7.075	46	274024	79.202	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	158.400%#
24) Chloroform-d	7.648	84	515873	21.109	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.440%
26) 1,2-Dichloroethane-d4	8.307	65	337254	25.711	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.840%
32) Benzene-d6	8.276	84	1049836	22.984	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.920%
36) 1,2-Dichloropropane-d6	9.276	67	358144	25.345	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.360%
41) Toluene-d8	10.325	98	871131	21.630	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.520%
43) trans-1,3-Dichloroprop...	10.575	79	149499	26.569	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	106.280%
47) 2-Hexanone-d5	10.922	63	184668	90.881	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	181.760%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	337805	32.630	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	130.520%#
66) 1,2-Dichlorobenzene-d4	13.849	152	174995	22.735	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.920%
Target Compounds					Qvalue	
13) Acetone	4.119	43	34663	10.422	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025437.D
Acq On : 20 Mar 2023 12:50
Operator : SY/MD
Sample : 01977-20
Misc : 7.65g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGA5

Quant Time: Mar 20 23:52:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

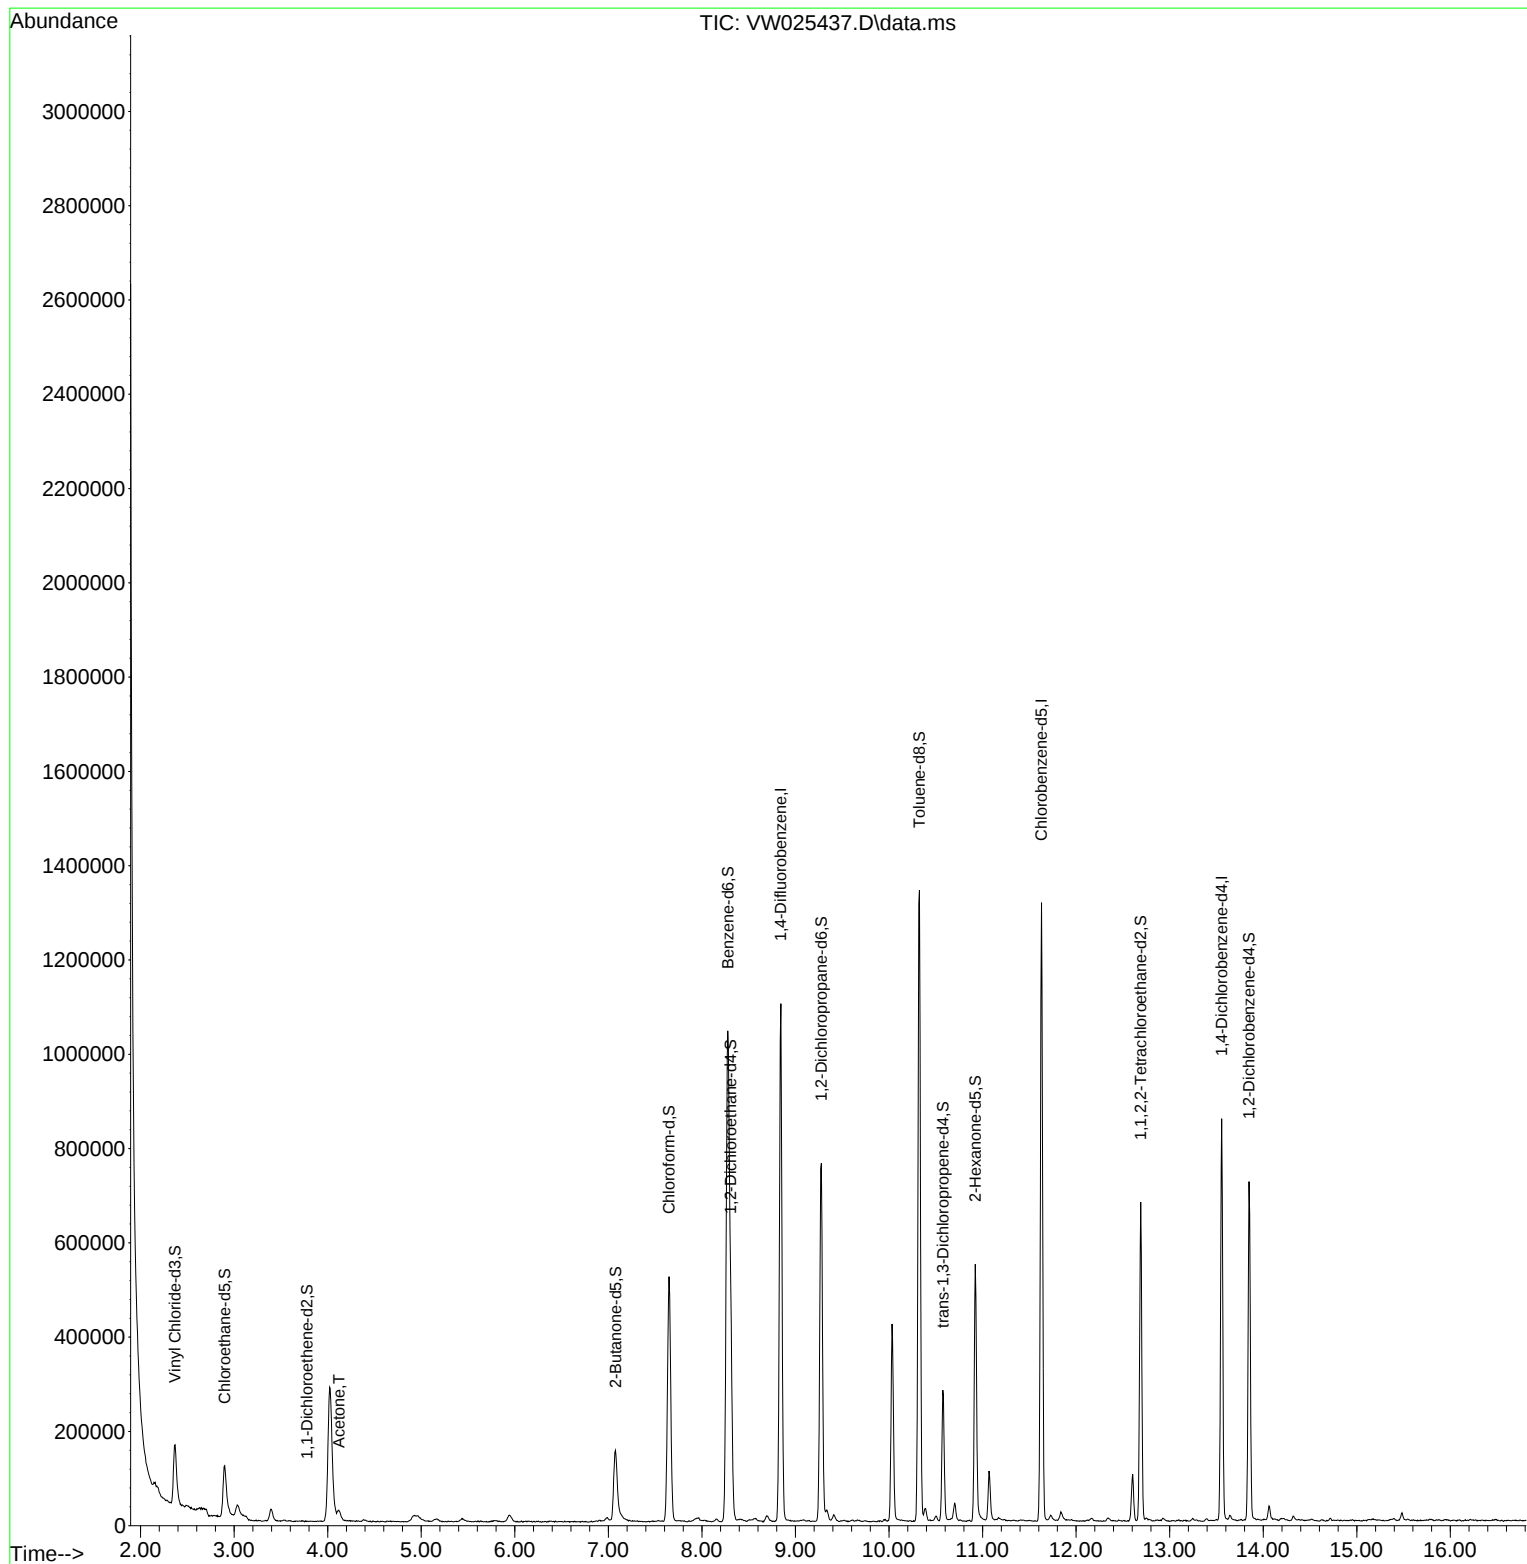

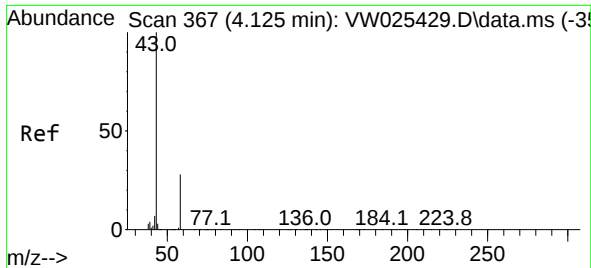

#13
 Acetone
 Concen: 10.422 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025437.D
 Acq: 20 Mar 2023 12:50

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGA5

Tgt Ion: 43 Resp: 34663
 Ion Ratio Lower Upper
 43 100
 58 26.7 0.0 60.0

