

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025440.D
 Acq On : 20 Mar 2023 14:02
 Operator : SY/MD
 Sample : 01977-22
 Misc : 7.15g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGA7

Quant Time: Mar 20 23:53:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1016431	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	927304	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	433430	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	178496	10.562	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	42.240%
7) Chloroethane-d5	2.893	69	177525	14.599	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.400%
11) 1,1-Dichloroethene-d2	4.021	63	383294	11.742	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.960%
21) 2-Butanone-d5	7.075	46	265250	63.942	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	127.880%
24) Chloroform-d	7.648	84	578669	19.748	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.000%
26) 1,2-Dichloroethane-d4	8.301	65	370081	23.531	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.120%
32) Benzene-d6	8.276	84	1211744	19.124	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.480%
36) 1,2-Dichloropropane-d6	9.270	67	410090	20.921	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.680%
41) Toluene-d8	10.325	98	1080848	19.347	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.400%
43) trans-1,3-Dichloroprop...	10.575	79	169836	21.759	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.040%
47) 2-Hexanone-d5	10.922	63	183255	65.015	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	130.020%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	385504	26.844	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.360%
66) 1,2-Dichlorobenzene-d4	13.849	152	369958	22.953	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.800%
Target Compounds					Qvalue	
13) Acetone	4.119	43	33381	8.371	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025440.D
Acq On : 20 Mar 2023 14:02
Operator : SY/MD
Sample : 01977-22
Misc : 7.15g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGA7

Quant Time: Mar 20 23:53:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

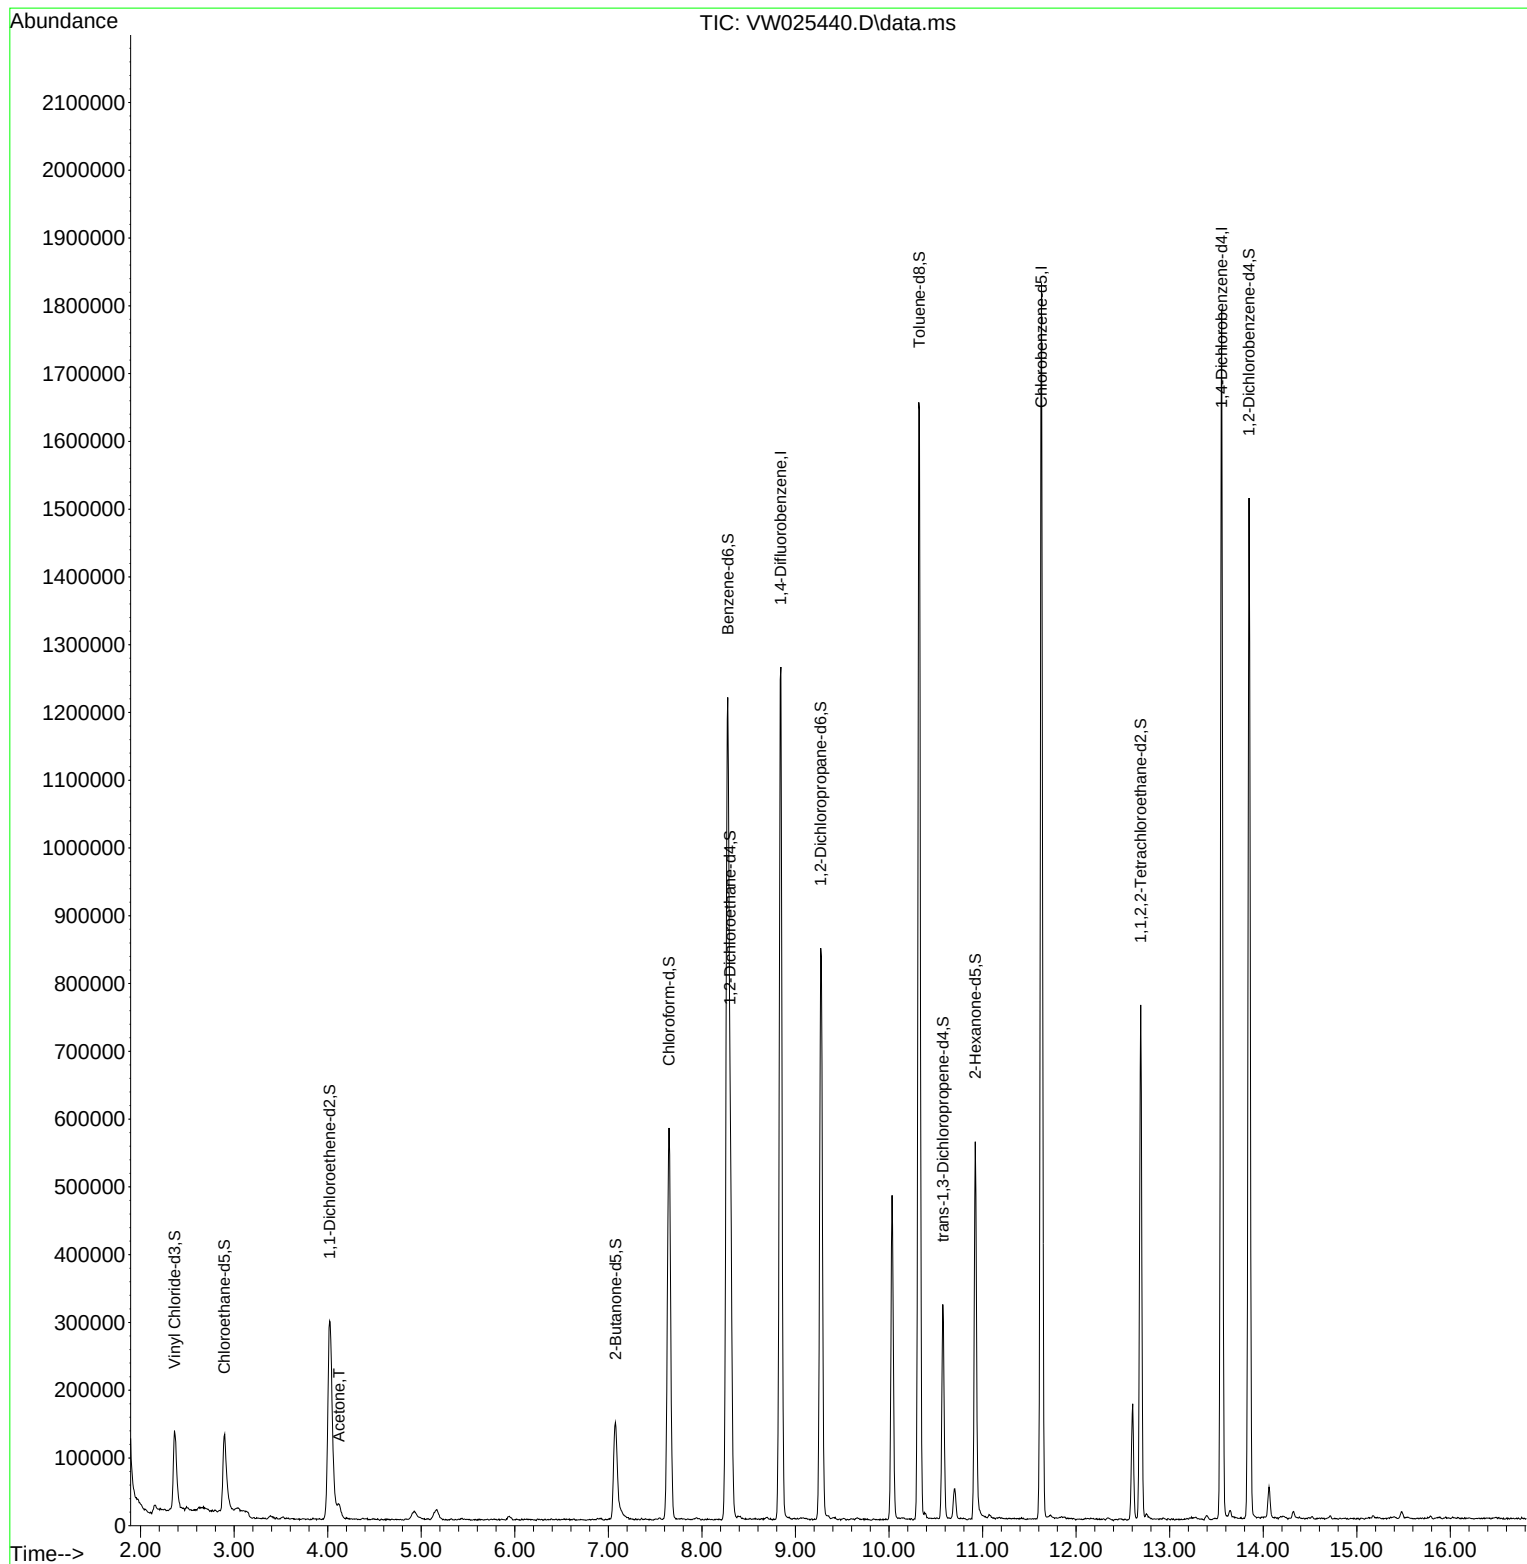

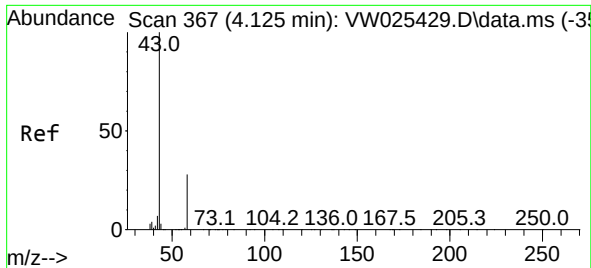

#13
 Acetone
 Concen: 8.371 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025440.D
 Acq: 20 Mar 2023 14:02

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGA7

Tgt Ion: 43 Resp: 33381
 Ion Ratio Lower Upper
 43 100
 58 31.0 0.0 60.0

