

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025444.D
 Acq On : 20 Mar 2023 15:37
 Operator : SY/MD
 Sample : 01979-02
 Misc : 6.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGA8

Quant Time: Mar 20 23:53:52 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1086835	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	980639	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	444707	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	200881	11.116	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	44.480%
7) Chloroethane-d5	2.899	69	192338	14.792	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.160%
11) 1,1-Dichloroethene-d2	4.027	63	425711	12.197	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.800%
21) 2-Butanone-d5	7.075	46	259407	58.482	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.960%
24) Chloroform-d	7.648	84	638163	20.368	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.480%
26) 1,2-Dichloroethane-d4	8.307	65	389492	23.161	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.640%
32) Benzene-d6	8.276	84	1327263	19.808	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.240%
36) 1,2-Dichloropropane-d6	9.270	67	437119	21.087	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	84.360%
41) Toluene-d8	10.325	98	1179119	19.959	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.840%
43) trans-1,3-Dichloroprop...	10.575	79	182077	22.058	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.240%
47) 2-Hexanone-d5	10.922	63	185771	62.323	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	124.640%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	393567	25.915	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.680%
66) 1,2-Dichlorobenzene-d4	13.848	152	392312	23.723	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.880%
Target Compounds					Qvalue	
13) Acetone	4.124	43	41413	9.712	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025444.D
Acq On : 20 Mar 2023 15:37
Operator : SY/MD
Sample : 01979-02
Misc : 6.08g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGA8

Quant Time: Mar 20 23:53:52 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

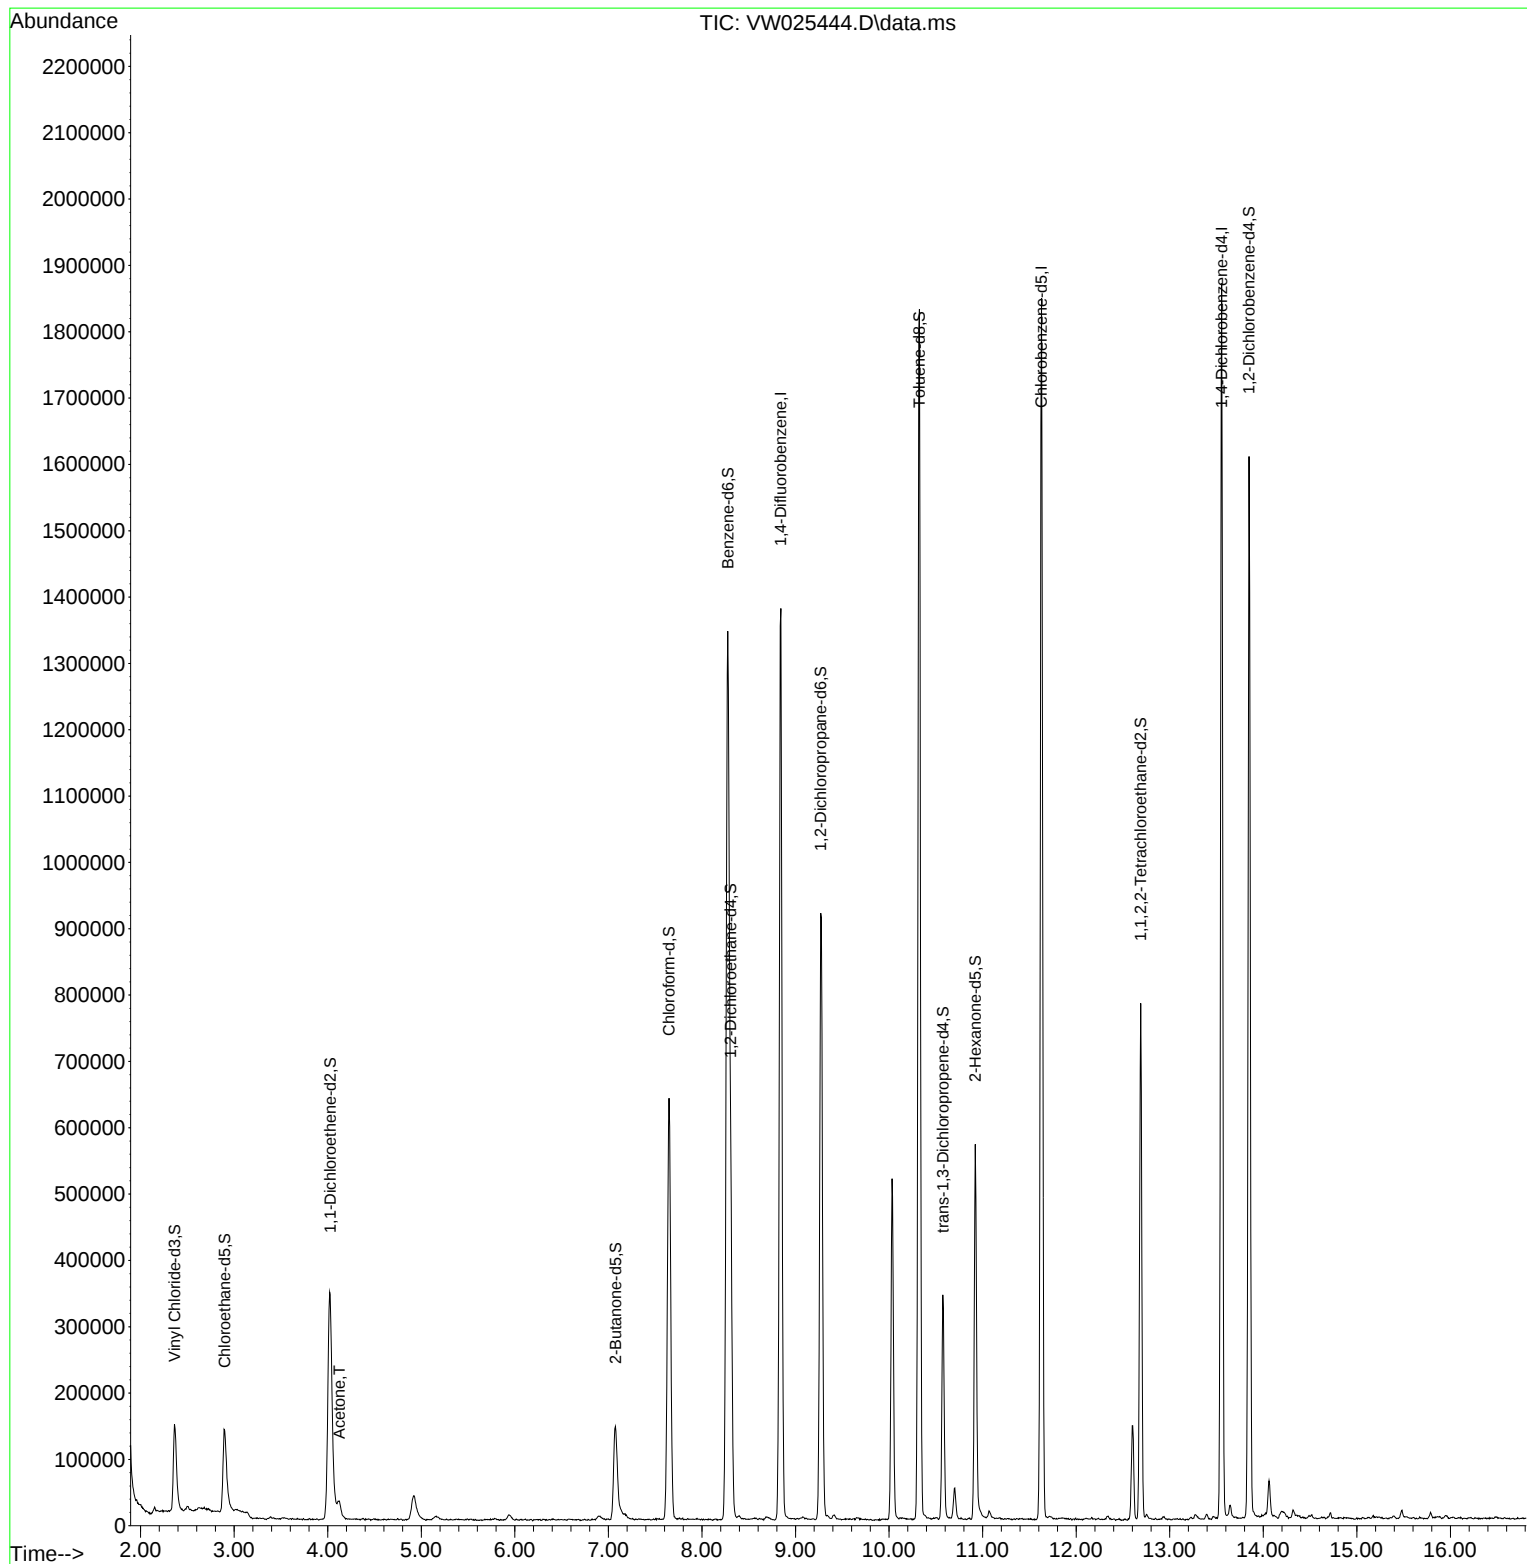

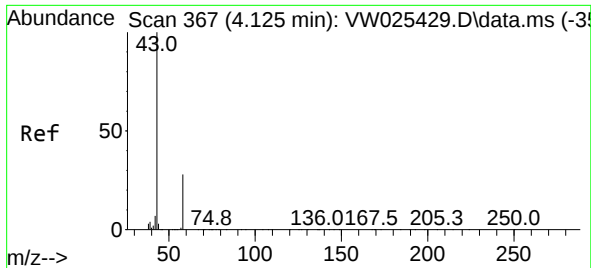

#13
 Acetone
 Concen: 9.712 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW025444.D
 Acq: 20 Mar 2023 15:37

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGA8

Tgt Ion: 43 Resp: 41413
 Ion Ratio Lower Upper
 43 100
 58 31.3 0.0 60.0

