

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025446.D
 Acq On : 20 Mar 2023 16:25
 Operator : SY/MD
 Sample : 01979-04
 Misc : 7.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETGC2

Quant Time: Mar 20 23:54:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1041044	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	937094	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	452064	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	172943	9.991	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	39.960%
7) Chloroethane-d5	2.899	69	168861	13.558	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.240%
11) 1,1-Dichloroethene-d2	4.021	63	364667	10.908	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.640%#
21) 2-Butanone-d5	7.075	46	240540	56.614	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.220%
24) Chloroform-d	7.648	84	552250	18.401	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.600%
26) 1,2-Dichloroethane-d4	8.301	65	351003	21.790	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.160%
32) Benzene-d6	8.270	84	1140874	17.818	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.280%
36) 1,2-Dichloropropane-d6	9.270	67	384191	19.395	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	77.600%
41) Toluene-d8	10.319	98	1010453	17.898	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.600%
43) trans-1,3-Dichloroprop...	10.575	79	157359	19.950	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.800%
47) 2-Hexanone-d5	10.922	63	166297	58.382	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	116.760%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	354991	24.461	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.840%
66) 1,2-Dichlorobenzene-d4	13.848	152	331268	19.705	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.840%
Target Compounds					Qvalue	
13) Acetone	4.119	43	103117	25.247	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025446.D
Acq On : 20 Mar 2023 16:25
Operator : SY/MD
Sample : 01979-04
Misc : 7.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETGC2

Quant Time: Mar 20 23:54:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

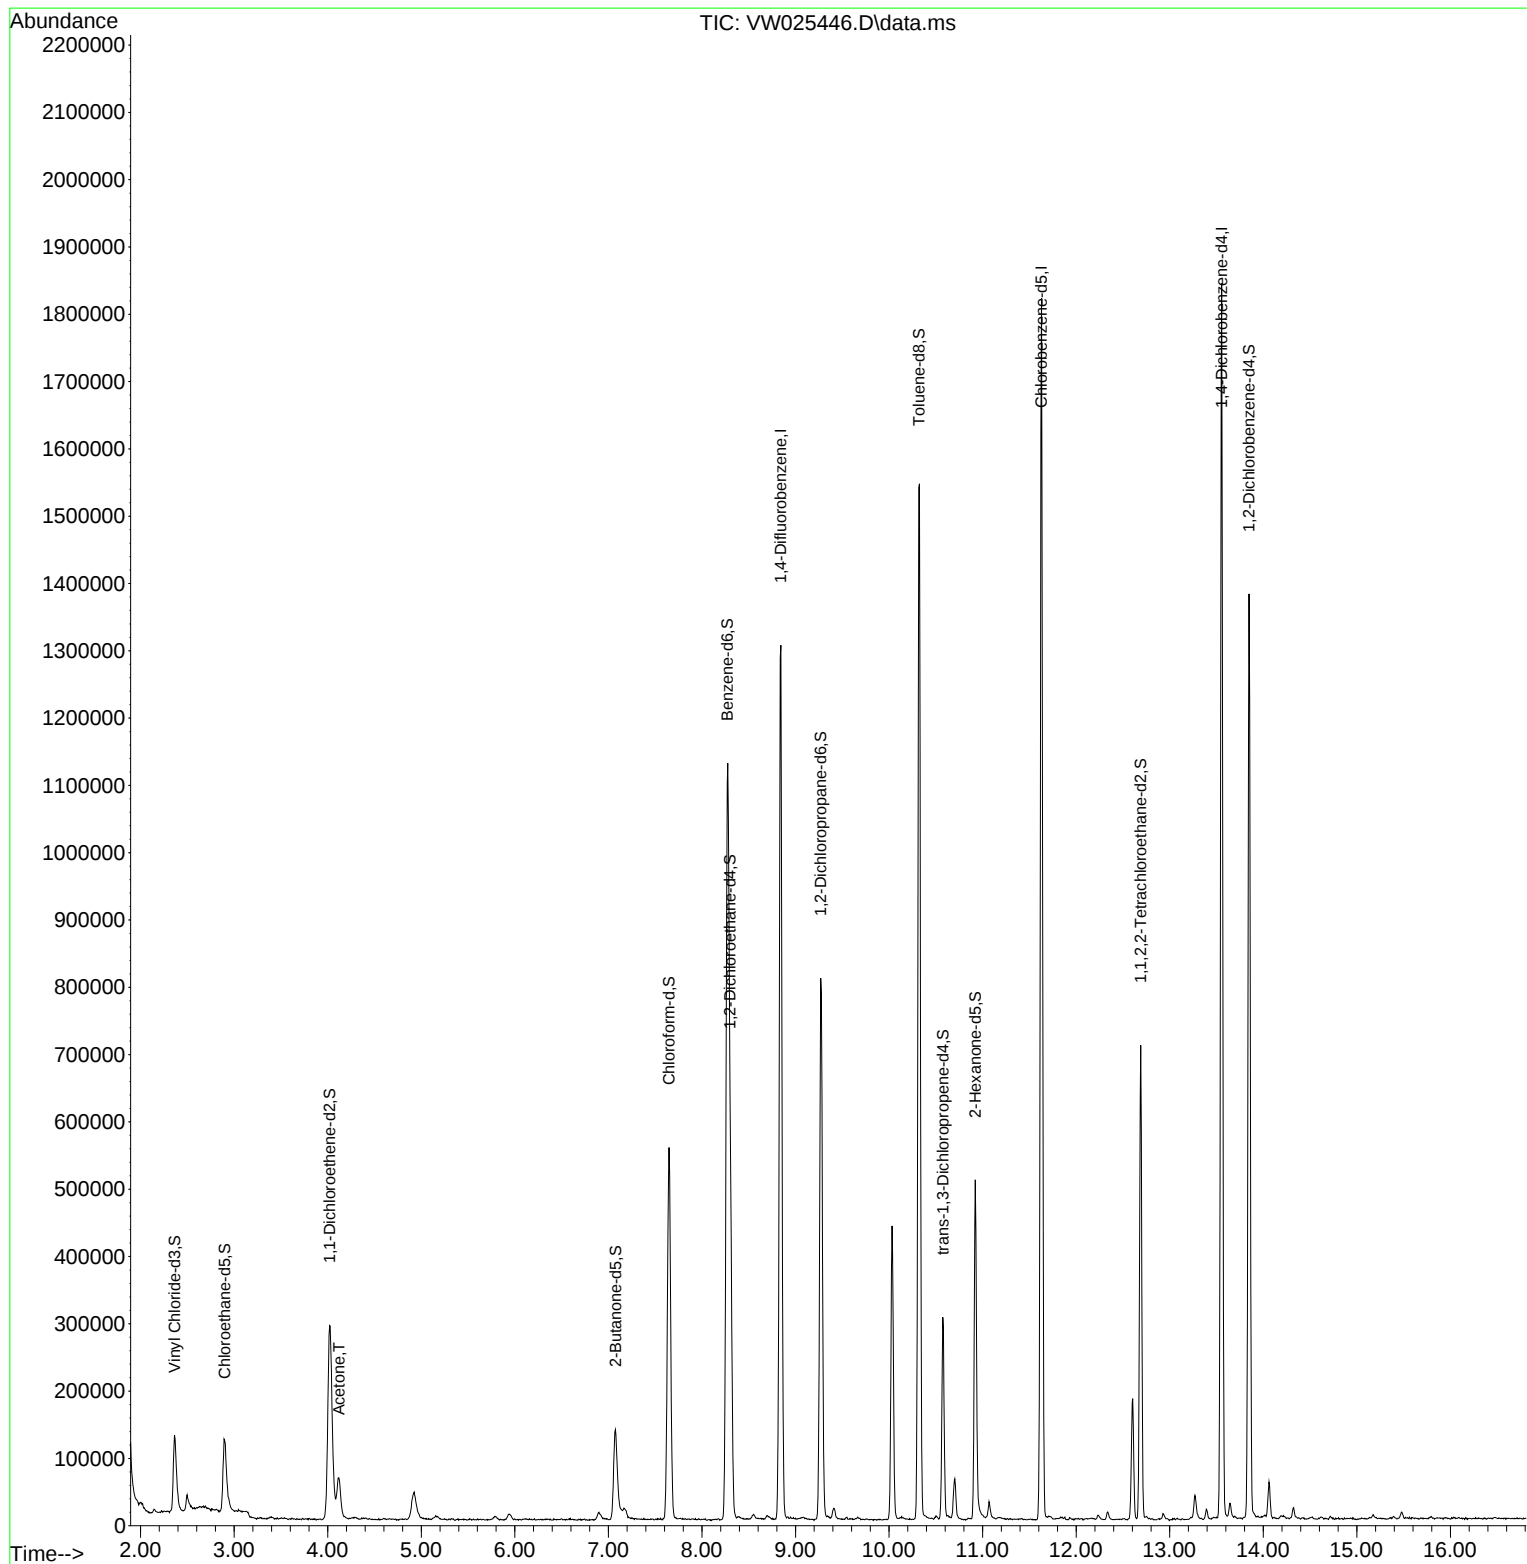

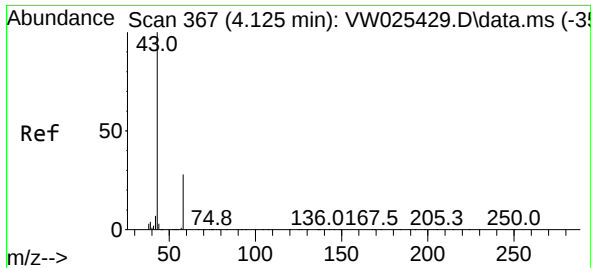

#13
 Acetone
 Concen: 25.247 ug/L
 RT: 4.119 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025446.D
 Acq: 20 Mar 2023 16:25

Instrument :
 MSVOA_W
 ClientSampleId :
 ETGC2

Tgt Ion: 43 Resp: 103117
 Ion Ratio Lower Upper
 43 100
 58 30.3 0.0 60.0

