

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025447.D
 Acq On : 20 Mar 2023 16:49
 Operator : SY/MD
 Sample : 01979-05
 Misc : 7.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB0

Quant Time: Mar 20 23:54:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	806810	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	711516	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	319059	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	150939	11.252	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	45.000%
7) Chloroethane-d5	2.899	69	145196	15.042	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.160%
11) 1,1-Dichloroethene-d2	4.021	63	325219	12.552	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.200%
21) 2-Butanone-d5	7.075	46	197460	59.967	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.940%
24) Chloroform-d	7.648	84	476509	20.487	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.960%
26) 1,2-Dichloroethane-d4	8.307	65	294314	23.575	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.320%
32) Benzene-d6	8.270	84	963038	19.809	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.240%
36) 1,2-Dichloropropane-d6	9.270	67	328967	21.872	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.480%
41) Toluene-d8	10.325	98	859473	20.051	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.200%
43) trans-1,3-Dichloroprop...	10.575	79	130577	21.803	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.200%
47) 2-Hexanone-d5	10.922	63	128571	59.448	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.900%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	287353	26.078	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	261249	22.018	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.080%
Target Compounds					Qvalue	
13) Acetone	4.118	43	41987	13.264	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025447.D
Acq On : 20 Mar 2023 16:49
Operator : SY/MD
Sample : 01979-05
Misc : 7.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB0

Quant Time: Mar 20 23:54:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

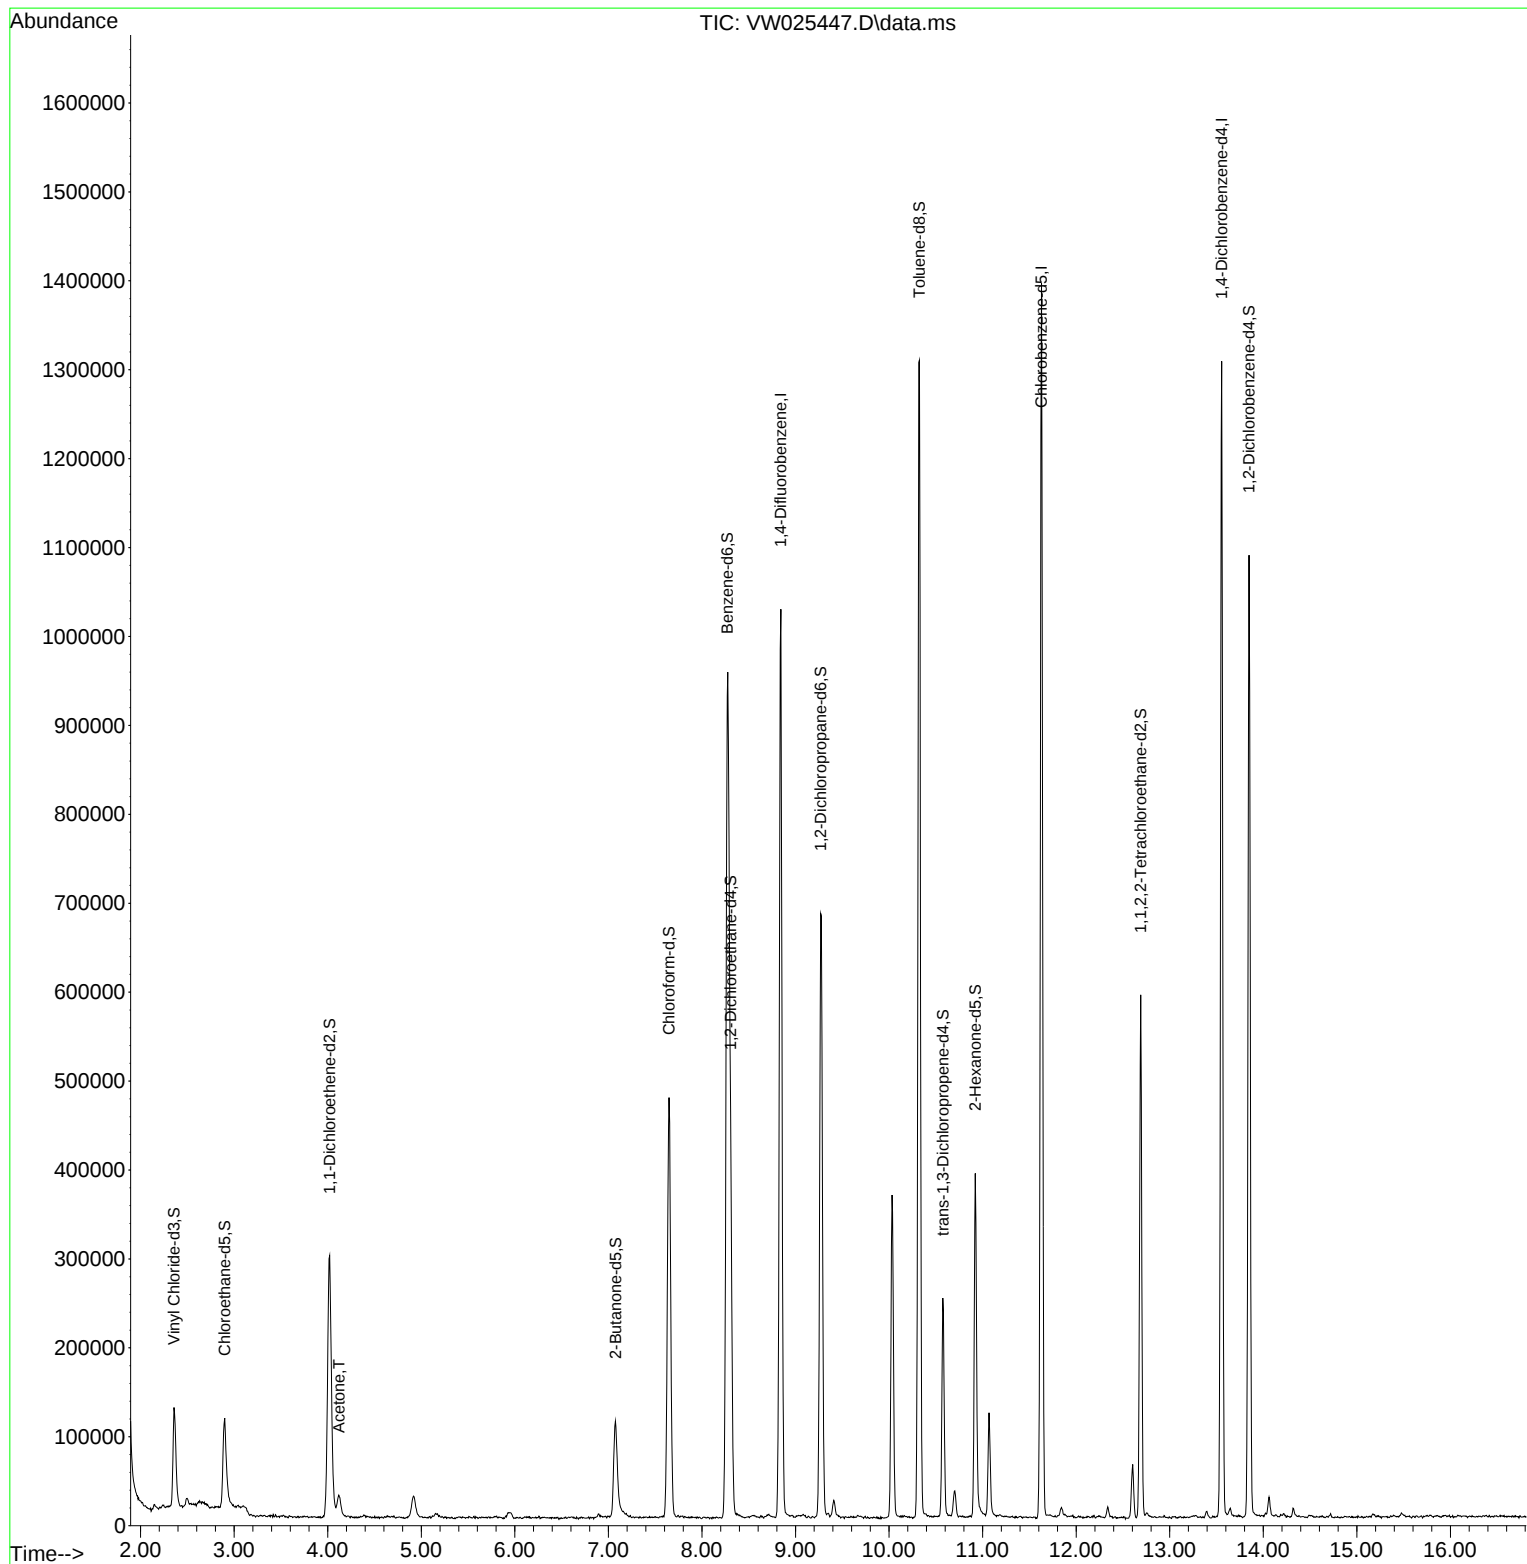

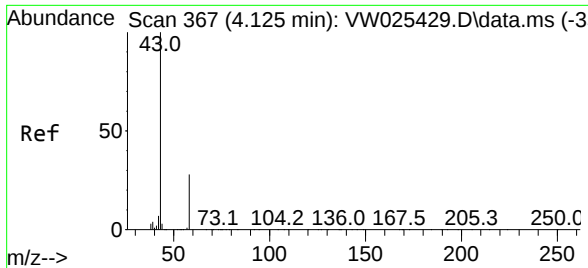

#13
 Acetone
 Concen: 13.264 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW025447.D
 Acq: 20 Mar 2023 16:49

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB0

Tgt Ion: 43	Resp: 41987
Ion Ratio	Lower Upper
43	100
58	27.8 0.0 60.0

