

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025451.D
 Acq On : 20 Mar 2023 18:25
 Operator : SY/MD
 Sample : 01979-09
 Misc : 6.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB5

Quant Time: Mar 20 23:55:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1111592	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	1006542	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	474381	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	173938	9.411	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	37.640%
7) Chloroethane-d5	2.893	69	171700	12.911	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	51.640%
11) 1,1-Dichloroethene-d2	4.021	63	380034	10.646	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	42.600%#
21) 2-Butanone-d5	7.075	46	232190	51.181	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.360%
24) Chloroform-d	7.648	84	569922	17.785	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.120%
26) 1,2-Dichloroethane-d4	8.410	65	250	0.015	ug/L	0.10
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.276	84	1175322	17.089	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	68.360%
36) 1,2-Dichloropropane-d6	9.270	67	394957	18.563	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.240%
41) Toluene-d8	10.325	98	1063062	17.531	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.120%
43) trans-1,3-Dichloroprop...	10.575	79	160350	18.926	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.720%
47) 2-Hexanone-d5	10.922	63	158487	51.801	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.600%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	349553	22.425	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.680%
66) 1,2-Dichlorobenzene-d4	13.848	152	333547	18.907	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.640%
Target Compounds					Qvalue	
13) Acetone	4.118	43	164694	37.764	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025451.D
Acq On : 20 Mar 2023 18:25
Operator : SY/MD
Sample : 01979-09
Misc : 6.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB5

Quant Time: Mar 20 23:55:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

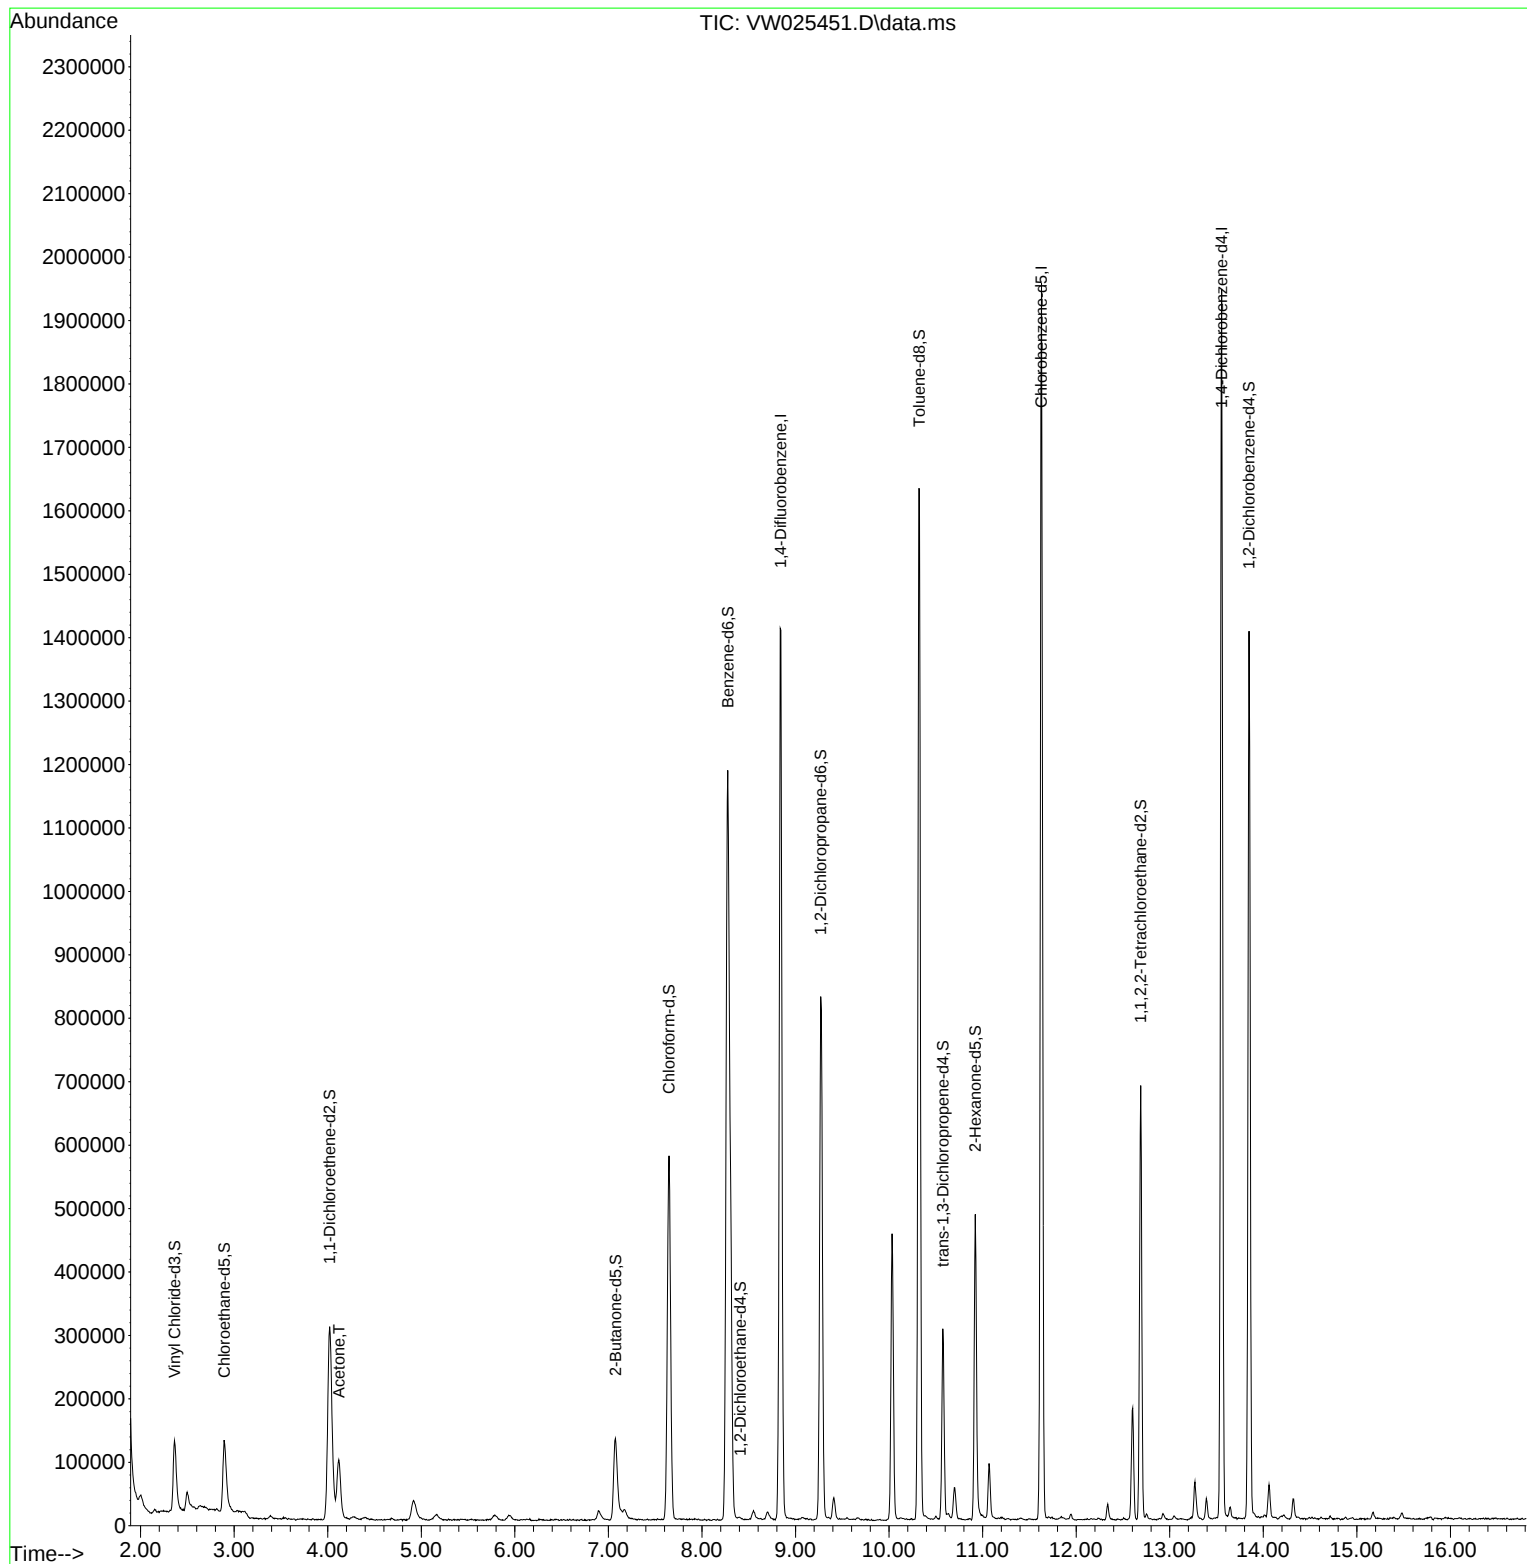

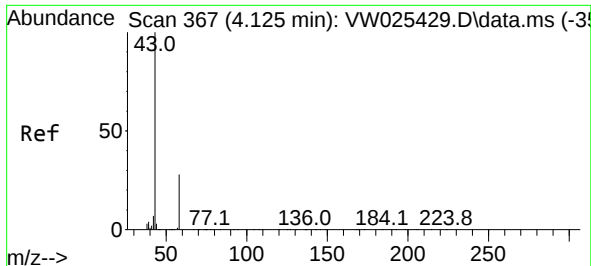

#13

Acetone

Concen: 37.764 ug/L

RT: 4.118 min Scan# 3

Delta R.T. -0.006 min

Lab File: VW025451.D

Acq: 20 Mar 2023 18:25

Instrument :

MSVOA_W

ClientSampleId :

EYGB5

Tgt Ion: 43 Resp: 164694

Ion Ratio Lower Upper

43 100

58 29.1 0.0 60.0

