




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025439.D
 Acq On : 20 Mar 2023 13:38
 Operator : SY/MD
 Sample : 01977-21
 Misc : 6.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGA6

Manual IntegrationsAPPROVED

Quant Time: Mar 20 23:52:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

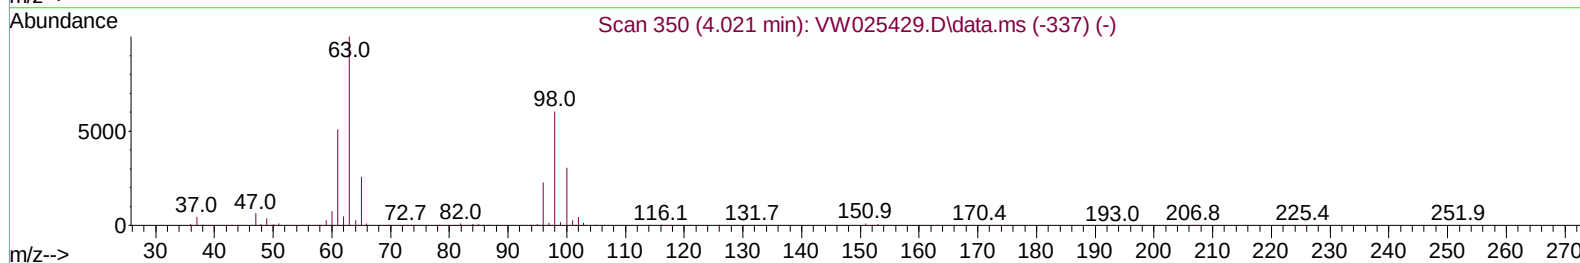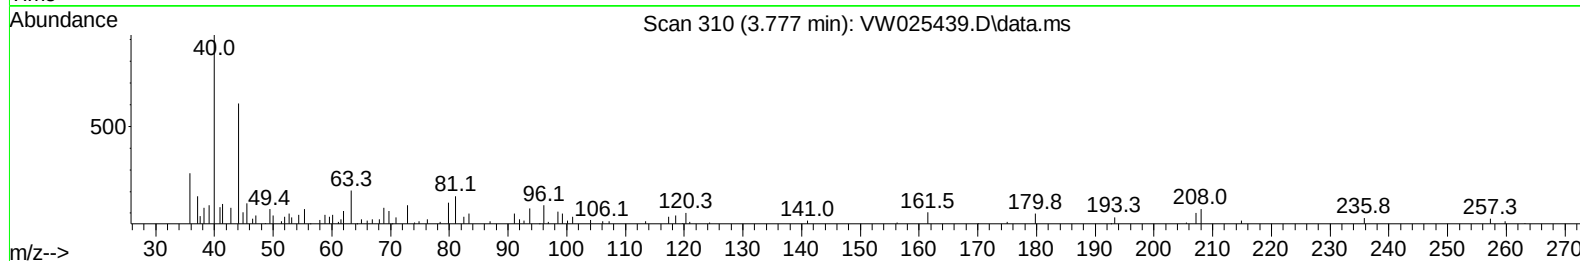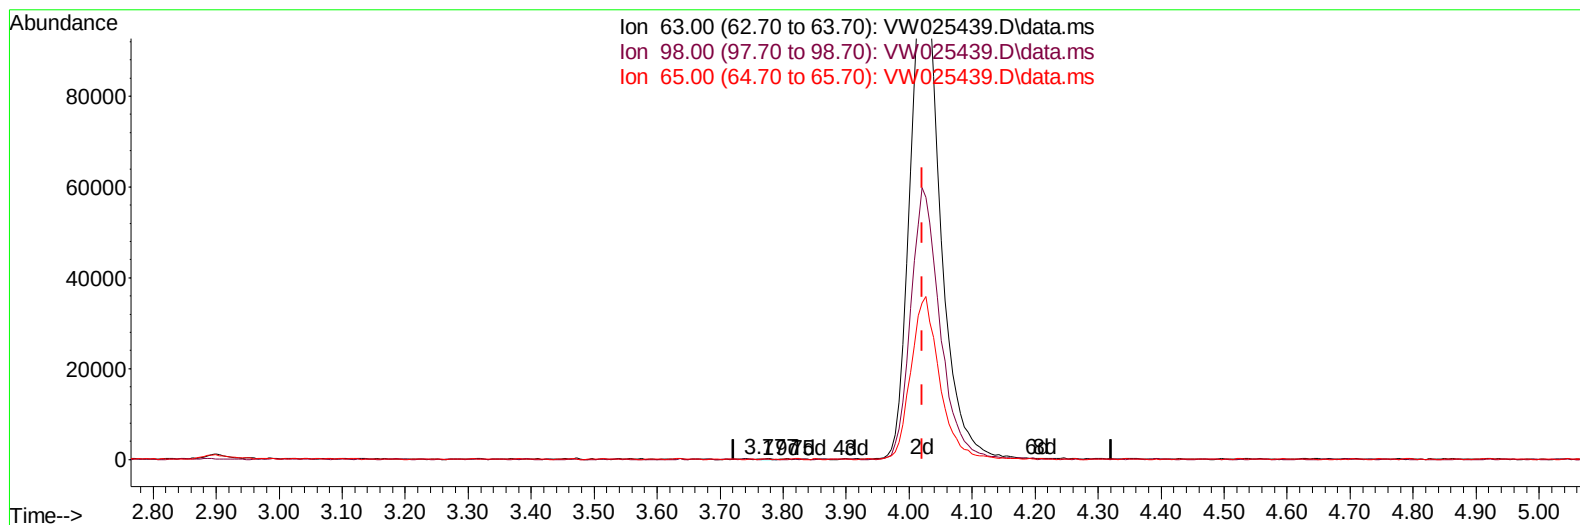

TIC: VW025439.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.777min (-0.244) 0.00 ug/L

response 130

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	48.46
65.00	23.70	18.46
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025439.D
Acq On : 20 Mar 2023 13:38
Operator : SY/MD
Sample : 01977-21
Misc : 6.92g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGA6

Manual IntegrationsAPPROVED

Quant Time: Mar 20 23:52:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/21/2023
Supervised By :Mahesh Dadoda 03/21/2023

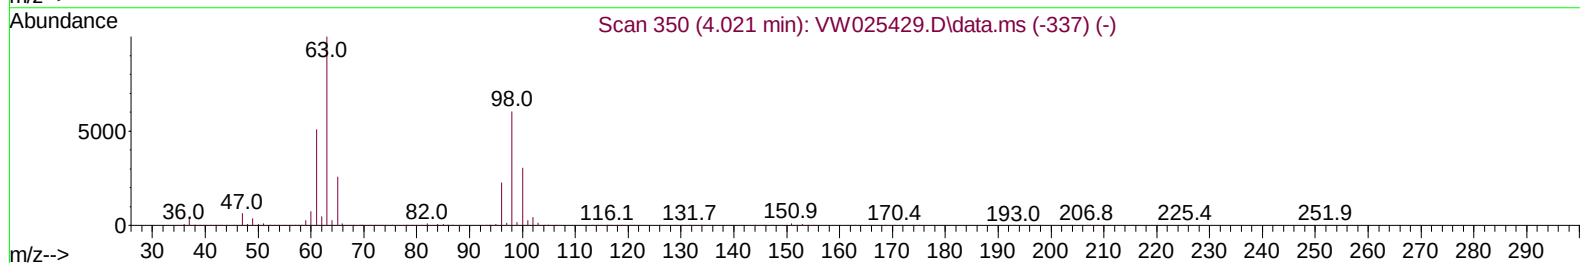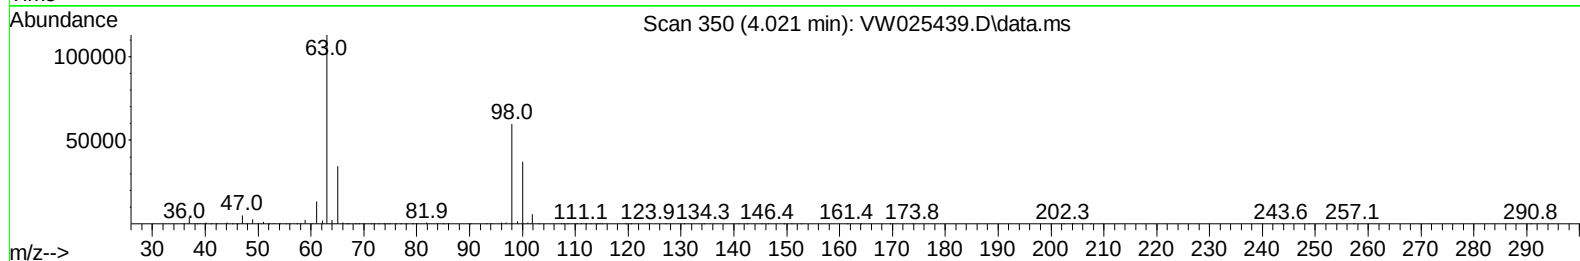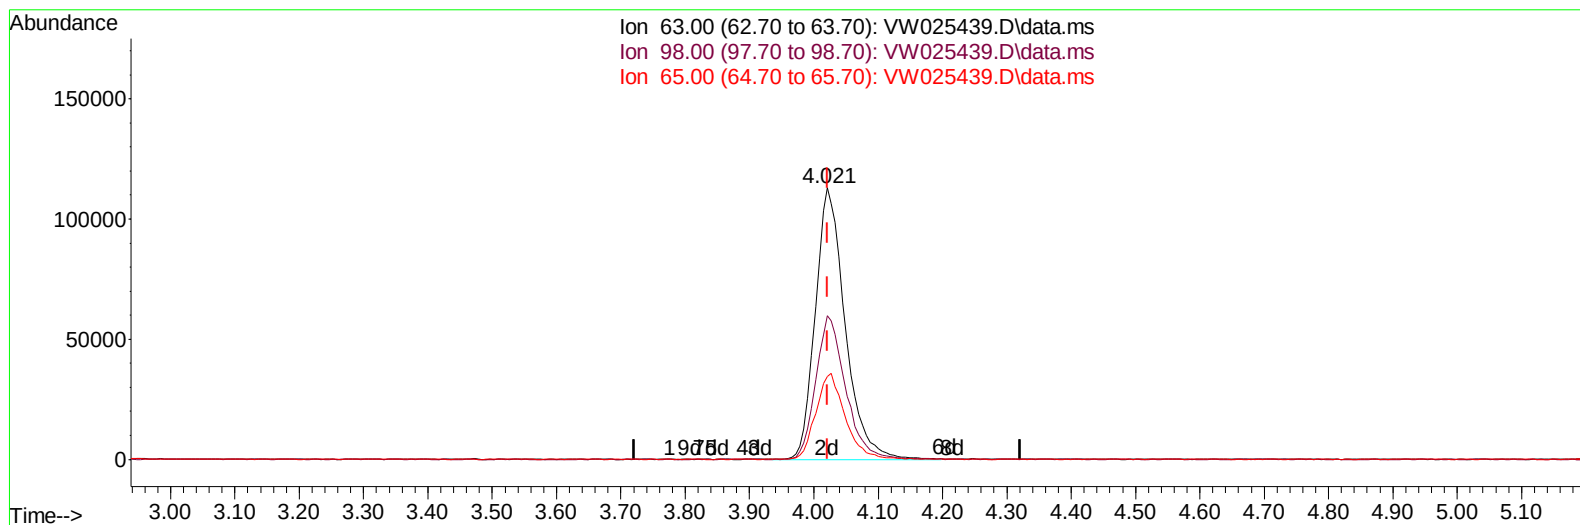

TIC: VW025439.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.000) 10.83 ug/L m

response 364174

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	0.02#
65.00	23.70	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025439.D
 Acq On : 20 Mar 2023 13:38
 Operator : SY/MD
 Sample : 01977-21
 Misc : 6.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGA6

Manual IntegrationsAPPROVED

Quant Time: Mar 20 23:52:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		1047568	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		928275	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		431758	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		172144	9.883	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	39.520%	
7) Chloroethane-d5	2.899	69		166753	13.305	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.240%	
11) 1,1-Dichloroethene-d2	4.021	63		364174m	10.825	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.320%#	
21) 2-Butanone-d5	7.075	46		231008	54.032	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.060%	
24) Chloroform-d	7.654	84		531298	17.593	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	70.360%	
26) 1,2-Dichloroethane-d4	8.307	65		329235	20.311	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.240%	
32) Benzene-d6	8.276	84		1116136	17.597	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	70.400%	
36) 1,2-Dichloropropane-d6	9.270	67		366060	18.655	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.640%	
41) Toluene-d8	10.325	98		1004742	17.966	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	71.880%	
43) trans-1,3-Dichloroprop...	10.575	79		152975	19.578	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.320%	
47) 2-Hexanone-d5	10.922	63		159286	56.452	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.900%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		332998	23.164	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.640%	
66) 1,2-Dichlorobenzene-d4	13.848	152		322827	20.106	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.440%	
Target Compounds							
13) Acetone	4.118	43		42505	10.342	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025439.D
Acq On : 20 Mar 2023 13:38
Operator : SY/MD
Sample : 01977-21
Misc : 6.92g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGA6

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/21/2023
Supervised By :Mahesh Dadoda 03/21/2023

Quant Time: Mar 20 23:52:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

