




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025445.D
 Acq On : 20 Mar 2023 16:01
 Operator : SY/MD
 Sample : 01979-03
 Misc : 6.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB9

Manual IntegrationsAPPROVED

Quant Time: Mar 20 23:54:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

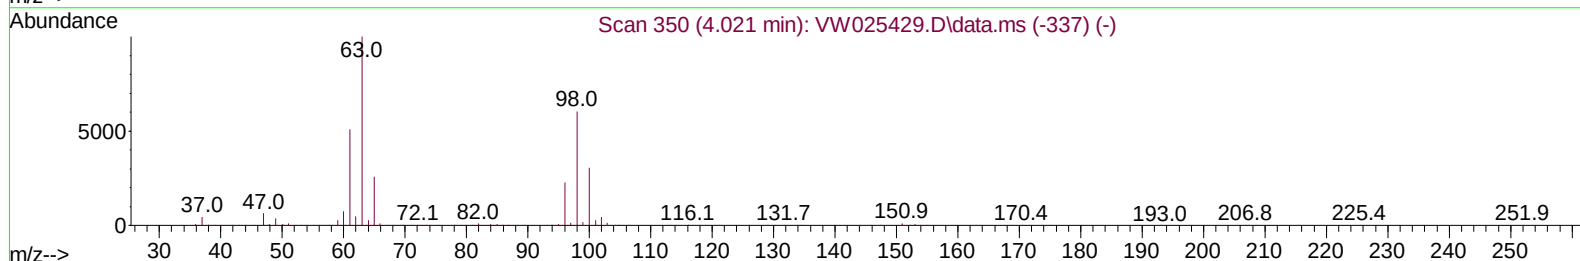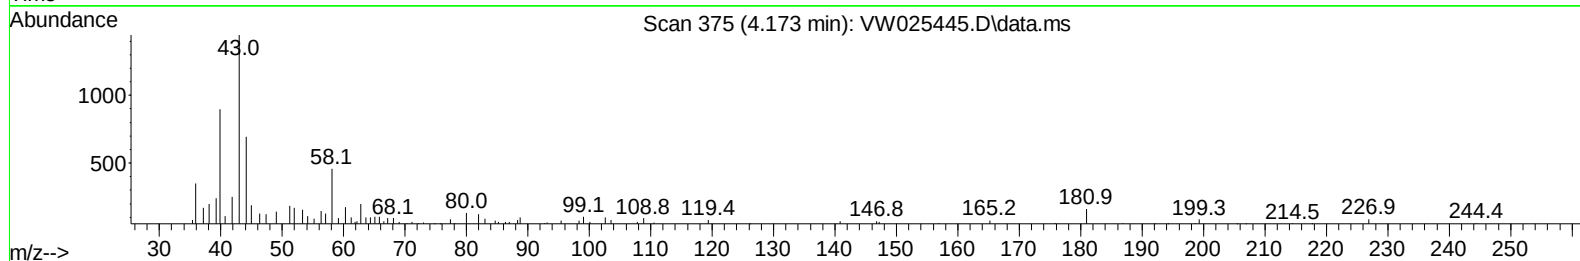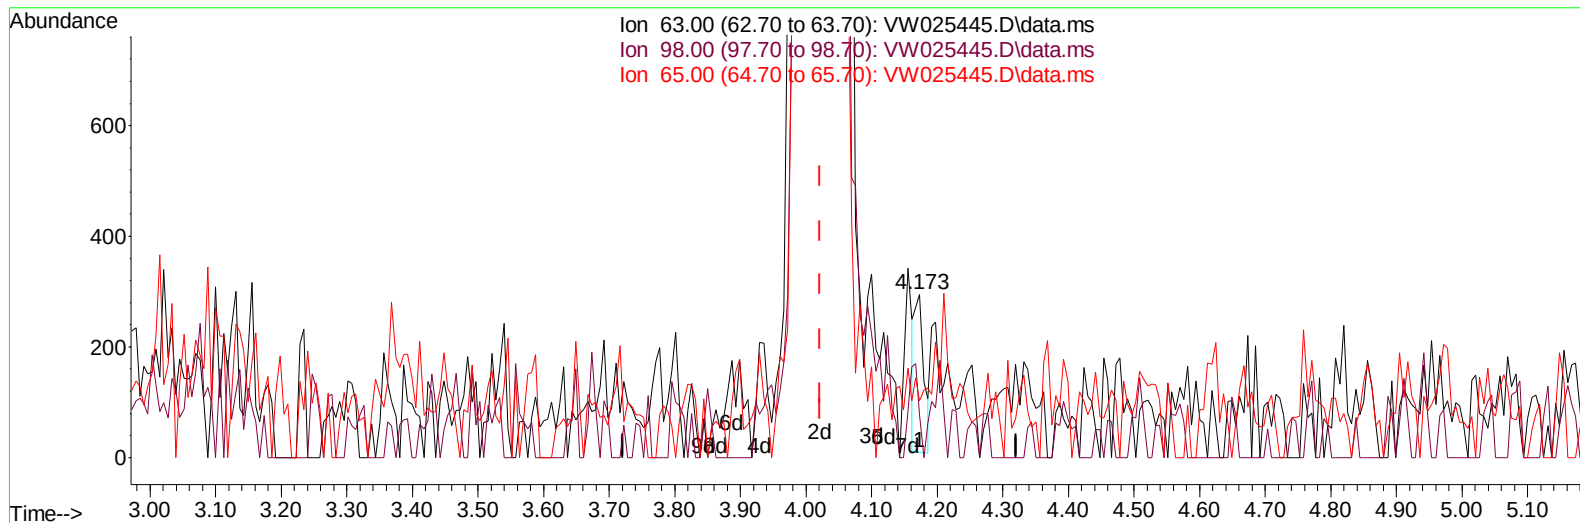

TIC: VW025445.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.173min (+ 0.152) 0.04 ug/L

response 282

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	64.18
65.00	23.70	25.53
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025445.D
 Acq On : 20 Mar 2023 16:01
 Operator : SY/MD
 Sample : 01979-03
 Misc : 6.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

Quant Time: Mar 20 23:54:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

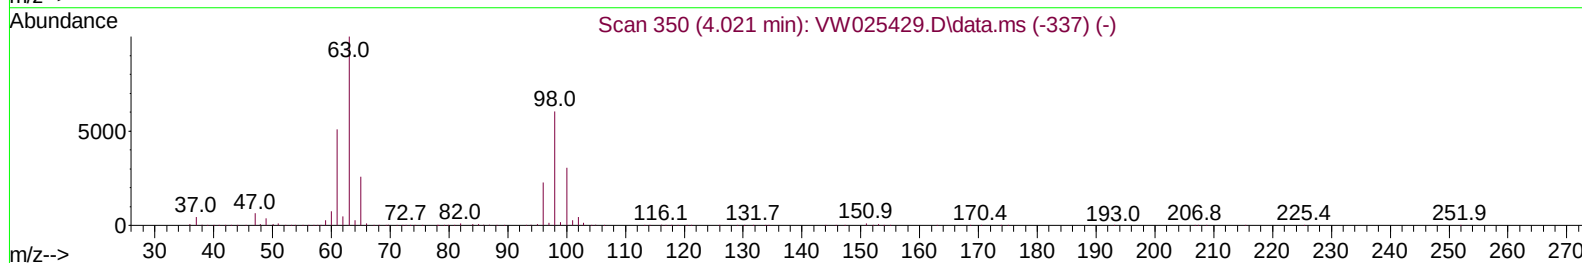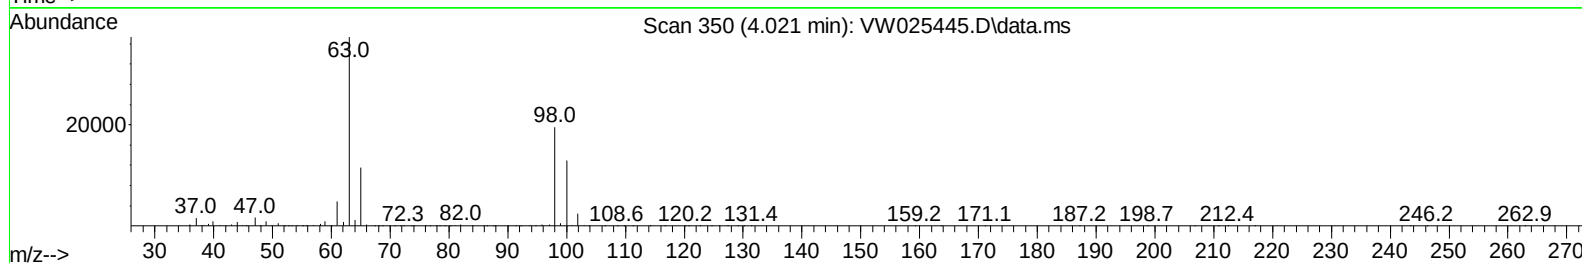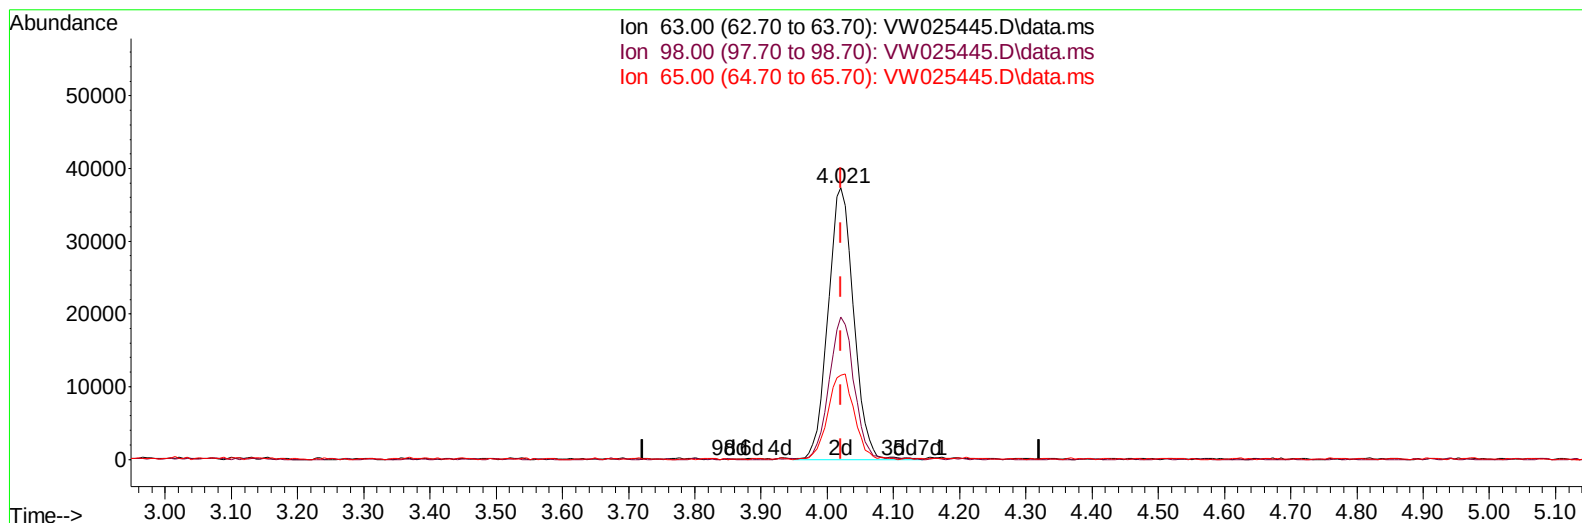

TIC: VW025445.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.000) 15.24 ug/L m

response 100484

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	0.18#
65.00	23.70	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
 Data File : VW025445.D
 Acq On : 20 Mar 2023 16:01
 Operator : SY/MD
 Sample : 01979-03
 Misc : 6.82g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EYGB9

Manual IntegrationsAPPROVED

Quant Time: Mar 20 23:54:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Mar 20 23:49:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/21/2023
 Supervised By :Mahesh Dadoda 03/21/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		205312	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		181145	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		71112	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.357	65		48127	14.098	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	56.400%		
7) Chloroethane-d5	2.893	69		47413	19.302	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	77.200%		
11) 1,1-Dichloroethene-d2	4.021	63		100484m	15.240	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	60.960%		
21) 2-Butanone-d5	7.081	46		53306	63.616	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	127.240%		
24) Chloroform-d	7.654	84		134141	22.663	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	90.640%		
26) 1,2-Dichloroethane-d4	8.307	65		82696	26.031	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	104.120%		
32) Benzene-d6	8.276	84		268387	21.683	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	86.720%		
36) 1,2-Dichloropropane-d6	9.276	67		88927	23.224	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	92.880%		
41) Toluene-d8	10.325	98		221992	20.342	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	81.360%		
43) trans-1,3-Dichloroprop...	10.581	79		34336	22.519	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	90.080%		
47) 2-Hexanone-d5	10.922	63		29912	54.325	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	108.640%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		82175	29.293	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	117.160%		
66) 1,2-Dichlorobenzene-d4	13.848	152		62466	23.621	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	94.480%		
Target Compounds							
13) Acetone	4.124	43		36247	44.999	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032023\
Data File : VW025445.D
Acq On : 20 Mar 2023 16:01
Operator : SY/MD
Sample : 01979-03
Misc : 6.82g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EYGB9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/21/2023
Supervised By :Mahesh Dadoda 03/21/2023

Quant Time: Mar 20 23:54:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Mar 20 23:49:37 2023
Response via : Initial Calibration

